

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC112221AL\
 Data File : FC056995.D
 Signal(s) : FID1A.CH
 Acq On : 22 Nov 2021 18:47
 Operator : AJ\MA
 Sample : M4766-07DL 50X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 CHRT-27165DL

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/23/2021
 Supervised By :mohammad ahmed 11/26/2021

Integration File: autoint1.e
 Quant Time: Nov 23 00:10:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 111921.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 19 00:52:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.591	131779	1.136 ug/mlm
Spiked Amount 50.000		Recovery =	2.27%
12) S 1-chlorooctadecane (S...	13.025	79214	0.870 ug/mlm
Spiked Amount 50.000		Recovery =	1.74%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC112221AL\
Data File : FC056995.D
Signal(s) : FID1A.CH
Acq On : 22 Nov 2021 18:47
Operator : AJ\MA
Sample : M4766-07DL 50X
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
CHRT-27165DL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/23/2021
Supervised By :mohammad ahmed 11/26/2021

Integration File: autoint1.e
Quant Time: Nov 23 00:10:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 111921.M
Quant Title : GC Extractables
QLast Update : Fri Nov 19 00:52:49 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

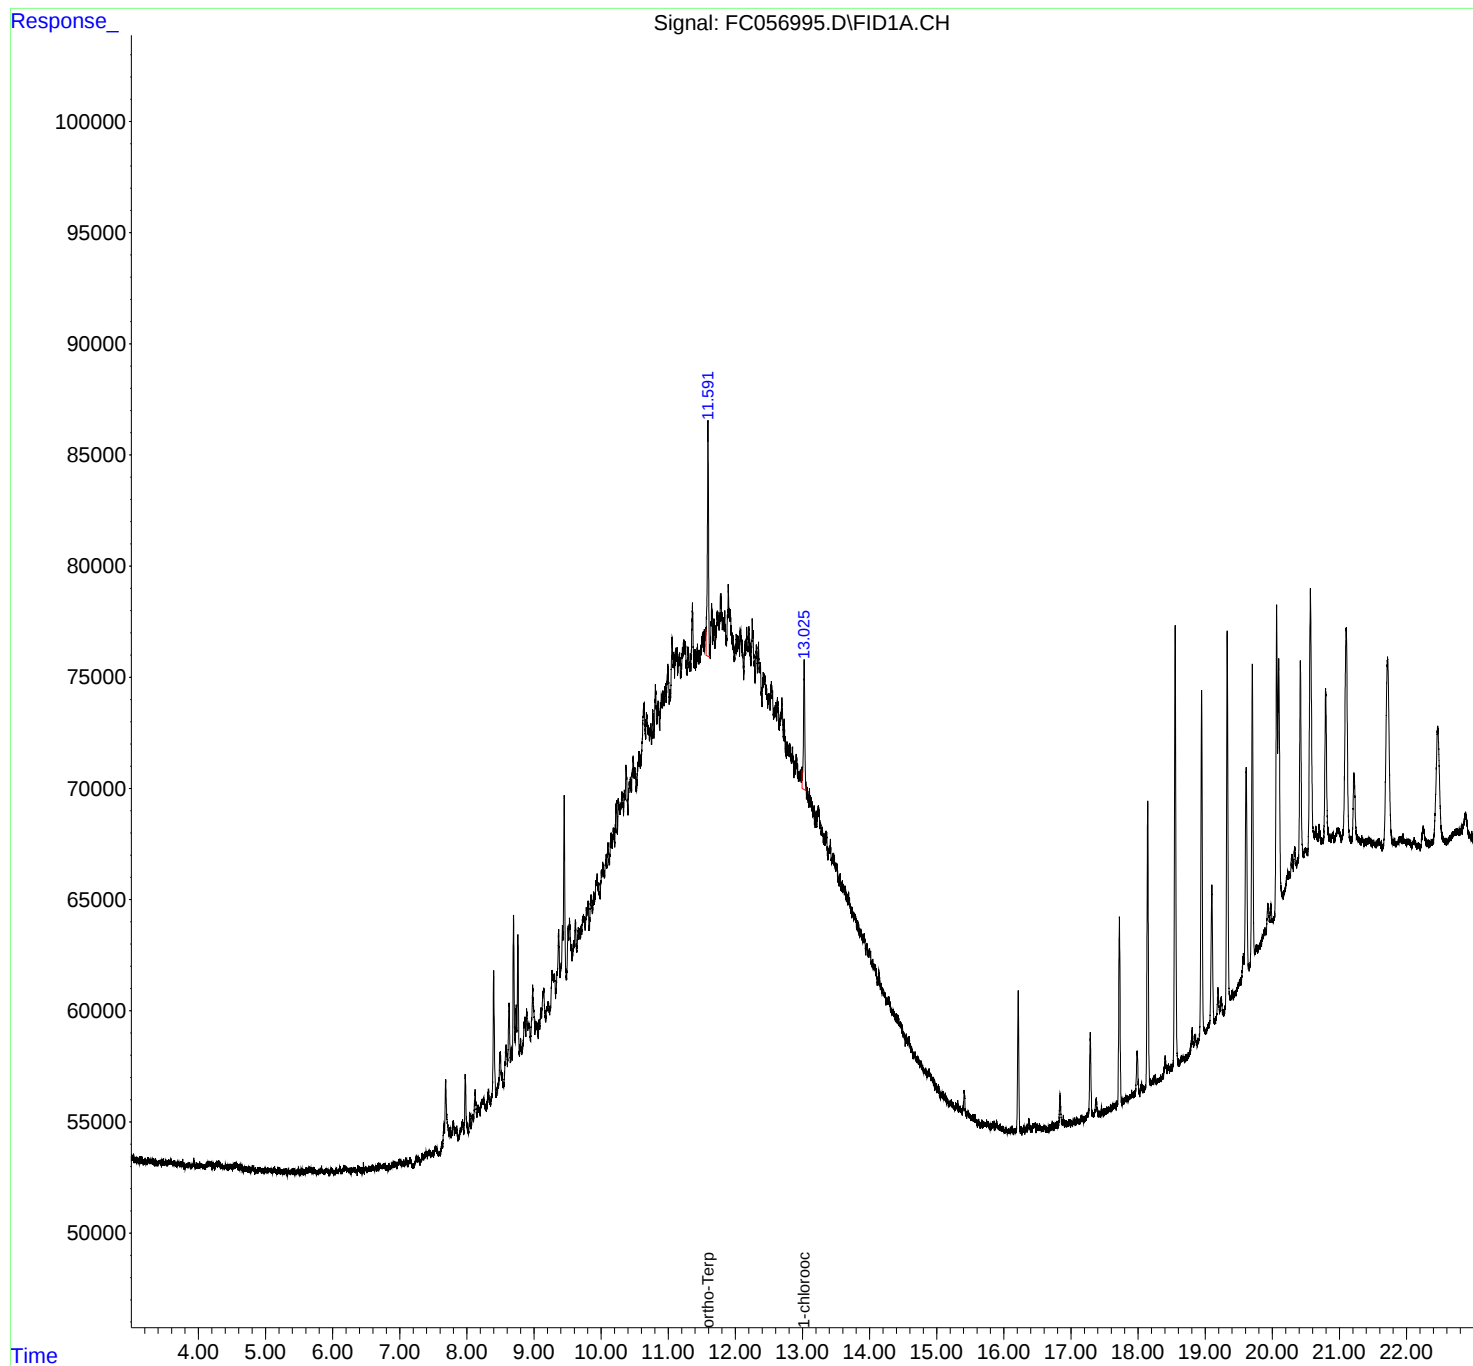

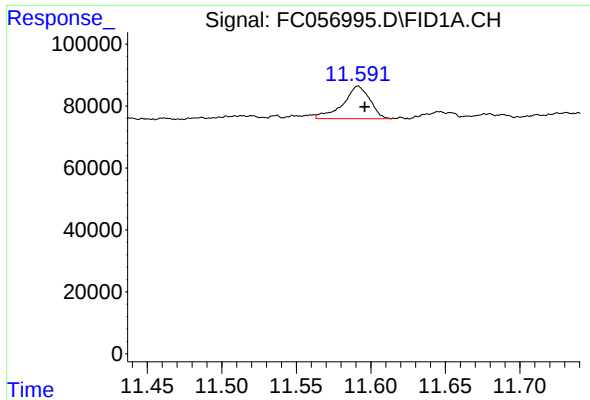

#9 ortho-Terphenyl (SURR)

R.T.: 11.591 min
Delta R.T.: -0.004 min
Response: 131779
Conc: 1.14 ug/ml

Instrument :

FID_C

ClientSampleId :


CHRT-27165DL

Manual Integrations

APPROVED

Reviewed By :Ankita Jodhani 11/23/2021

Supervised By :mohammad ahmed 11/26/2021

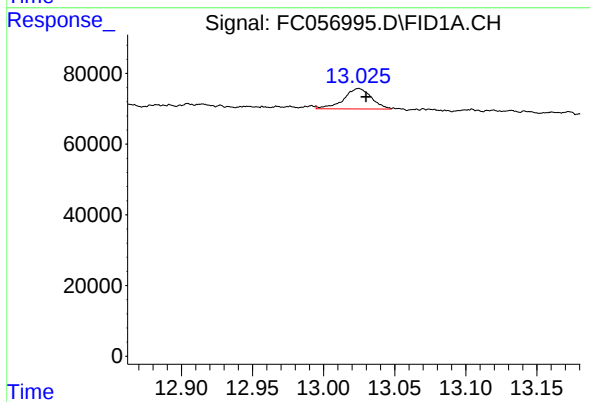

#12 1-chlorooctadecane (SURR)

R.T.: 13.025 min
Delta R.T.: -0.005 min
Response: 79214
Conc: 0.87 ug/ml m