

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC112321AL\
 Data File : FC057050.D
 Signal(s) : FID1A.CH
 Acq On : 24 Nov 2021 6:24
 Operator : AJ\MA
 Sample : M4812-01D
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 SETTING-TANK-01

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/24/2021
 Supervised By :mohammad ahmed 11/24/2021

Integration File: autoint1.e
 Quant Time: Nov 24 06:50:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 111921.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 19 00:52:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.590	3031307	26.121 ug/ml
Spiked Amount 50.000		Recovery =	52.24%
12) S 1-chlorooctadecane (S...	13.022	2330569	25.600 ug/mlm
Spiked Amount 50.000		Recovery =	51.20%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC112321AL\
Data File : FC057050.D
Signal(s) : FID1A.CH
Acq On : 24 Nov 2021 6:24
Operator : AJ\MA
Sample : M4812-01D
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
SETTING-TANK-01


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/24/2021
Supervised By :mohammad ahmed 11/24/2021

Integration File: autoint1.e
Quant Time: Nov 24 06:50:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 111921.M
Quant Title : GC Extractables
QLast Update : Fri Nov 19 00:52:49 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

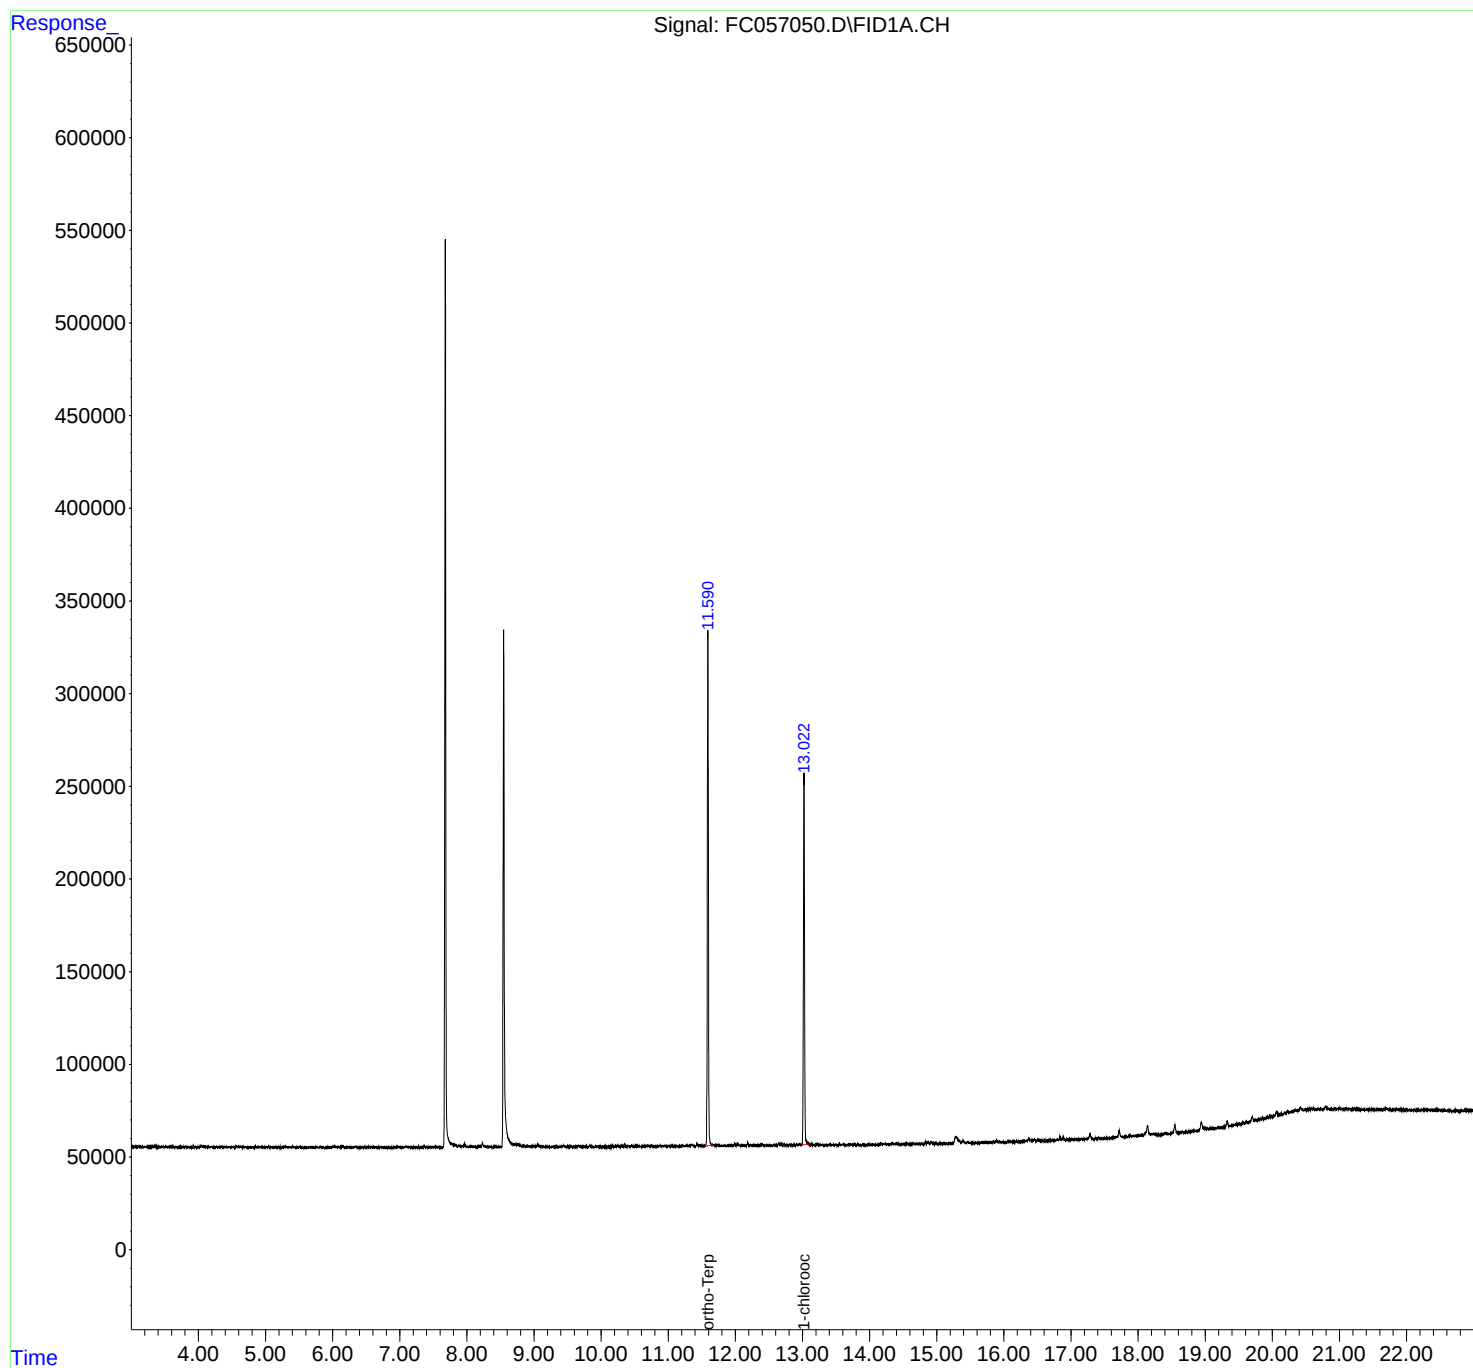

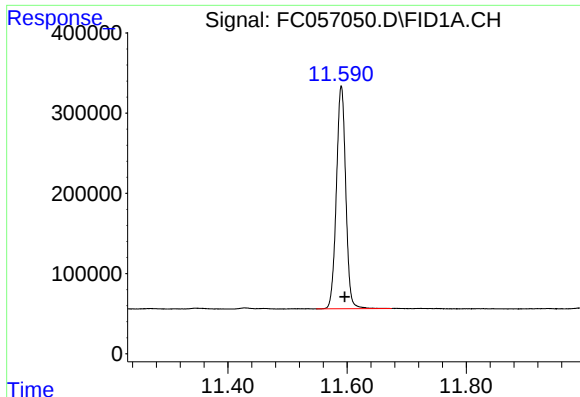

#9 ortho-Terphenyl (SURR)

R.T.: 11.590 min
Delta R.T.: -0.005 min
Response: 3031307
Conc: 26.12 ug/ml

Instrument :

FID_C


ClientSampleId :

SETTING-TANK-01

Manual Integrations

APPROVED

Reviewed By :Ankita Jodhani 11/24/2021
Supervised By :mohammad ahmed 11/24/2021

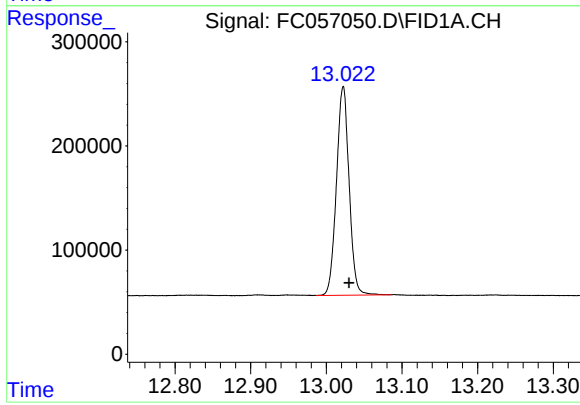

#12 1-chlorooctadecane (SURR)

R.T.: 13.022 min
Delta R.T.: -0.008 min
Response: 2330569
Conc: 25.60 ug/ml m