

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC112421AL\
 Data File : FC057072.D
 Signal(s) : FID1A.CH
 Acq On : 24 Nov 2021 21:44
 Operator : AJ\MA
 Sample : M4808-02DL 40X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 CHRT-20001DL

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/26/2021
 Supervised By :mohammad ahmed 11/26/2021

Integration File: autoint1.e
 Quant Time: Nov 25 02:09:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 111921.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 19 00:52:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.589	171202	1.475 ug/mlm
Spiked Amount 50.000		Recovery =	2.95%
12) S 1-chlorooctadecane (S...	13.021	102859	1.130 ug/mlm
Spiked Amount 50.000		Recovery =	2.26%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC112421AL\
Data File : FC057072.D
Signal(s) : FID1A.CH
Acq On : 24 Nov 2021 21:44
Operator : AJ\MA
Sample : M4808-02DL 40X
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
CHRT-20001DL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/26/2021
Supervised By :mohammad ahmed 11/26/2021

Integration File: autoint1.e
Quant Time: Nov 25 02:09:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 111921.M
Quant Title : GC Extractables
QLast Update : Fri Nov 19 00:52:49 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

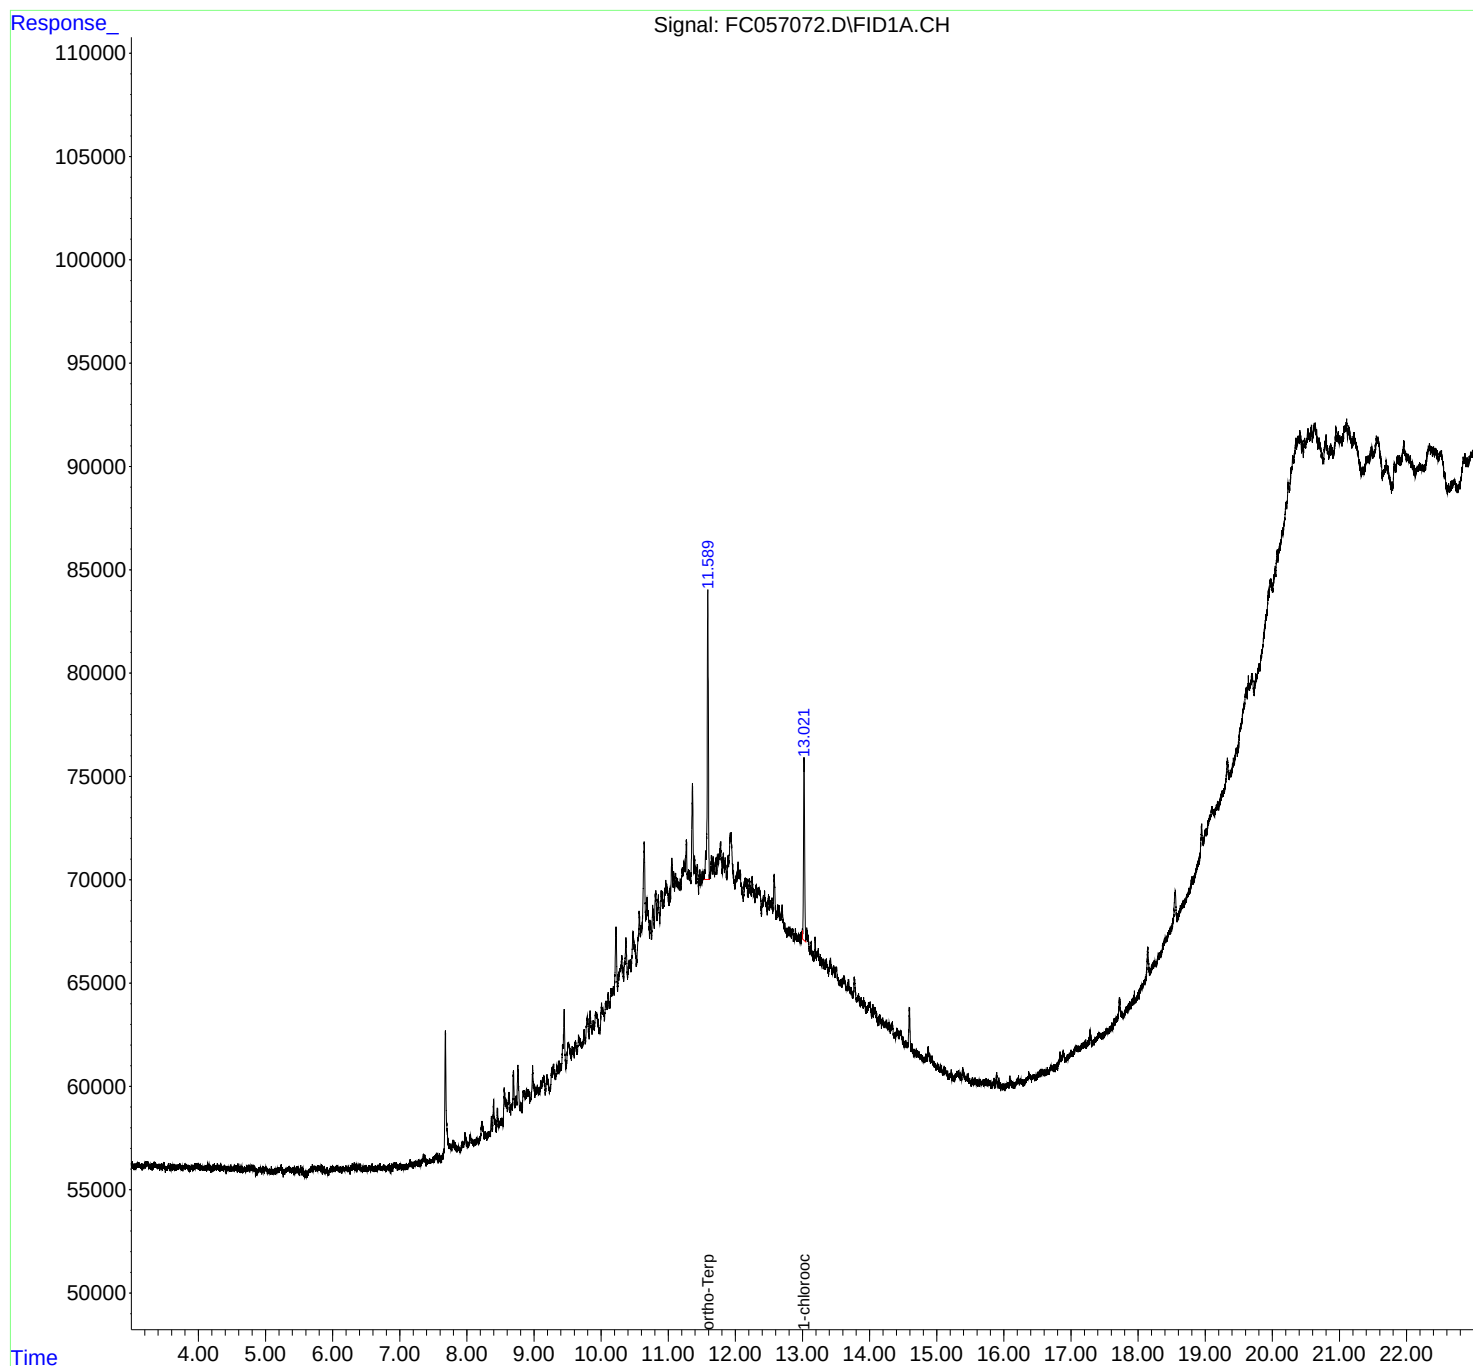

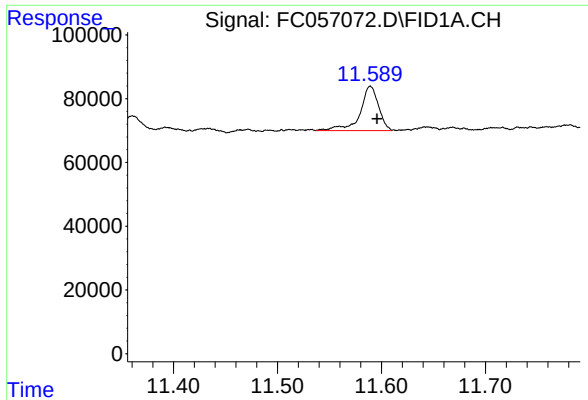


#9 ortho-Terphenyl (SURR)

R.T.: 11.589 min
Delta R.T.: -0.007 min
Response: 171202
Conc: 1.48 ug/ml

Instrument :
FID_C
ClientSampleId :
CHRT-20001DL

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/26/2021
Supervised By :mohammad ahmed 11/26/2021

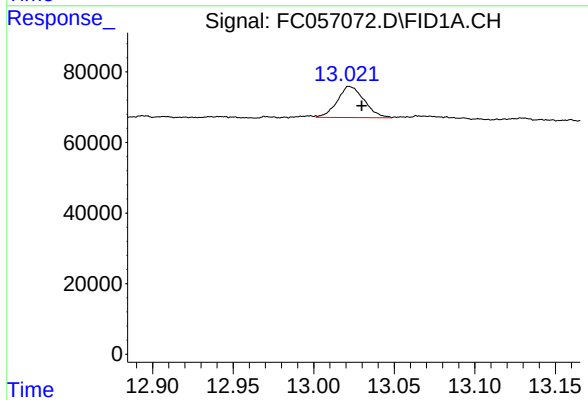

#12 1-chlorooctadecane (SURR)

R.T.: 13.021 min
Delta R.T.: -0.009 min
Response: 102859
Conc: 1.13 ug/ml m