

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC112923AL\
 Data File : FC065312.D
 Signal(s) : FID1A.ch
 Acq On : 29 Nov 2023 08:57
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 23:46:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 112423.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 24 13:28:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.480	158908	0.840 ug/ml
11) T n-Heneicosane (C21)	13.095	148153	0.802 ug/ml
13) T n-Docosane (C22)	13.683	147752	0.819 ug/ml
14) T n-Tetracosane (C24)	14.781	90765	0.524 ug/ml
15) T n-Hexacosane (C26)	15.799	110015	0.661 ug/ml
16) T n-Octacosane (C28)	16.744	63727	0.398 ug/ml
18) T n-Dotriacontane (C32)	18.456	92020	0.585 ug/ml
19) T n-Tetratriacontane (C34)	19.233	102978	0.667 ug/ml
20) T n-Hexatriacontane (C36)	19.978	40336	0.263 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC112923AL\
Data File : FC065312.D
Signal(s) : FID1A.ch
Acq On : 29 Nov 2023 08:57
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 29 23:46:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 112423.M
Quant Title : GC Extractables
QLast Update : Fri Nov 24 13:28:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

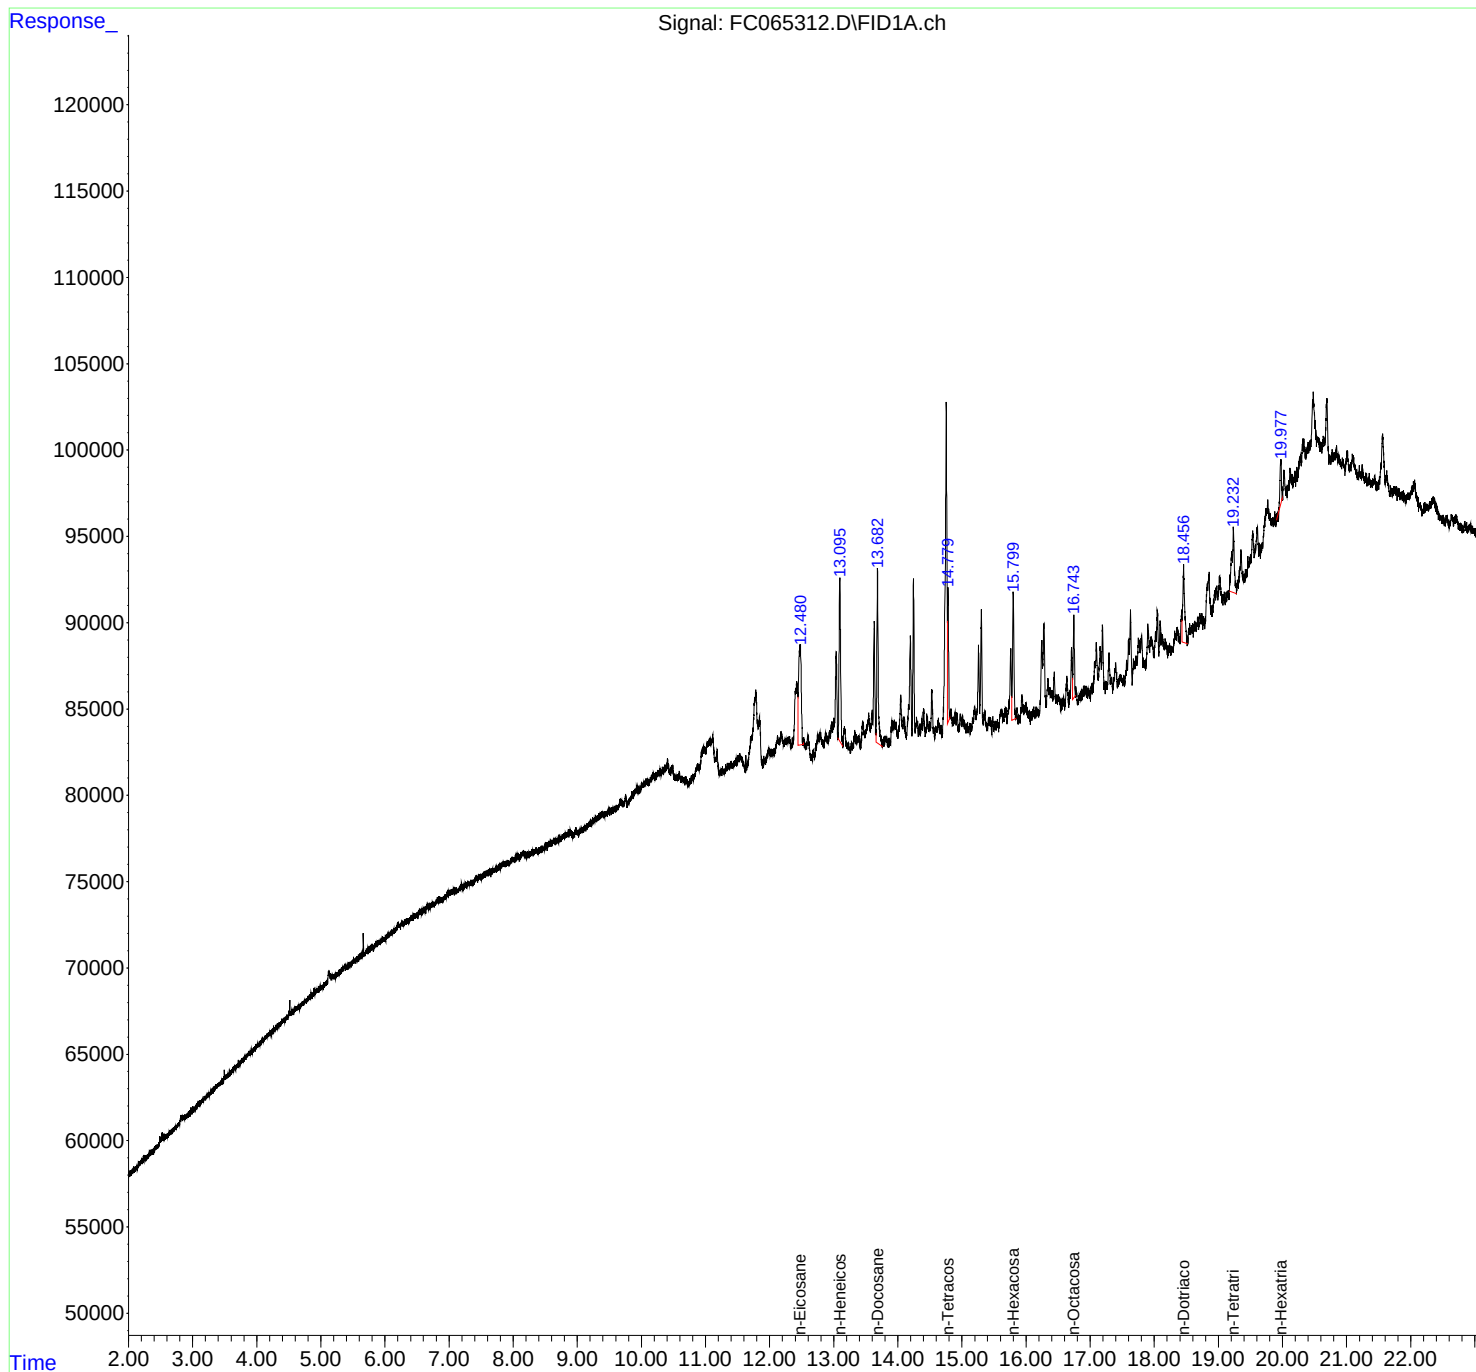


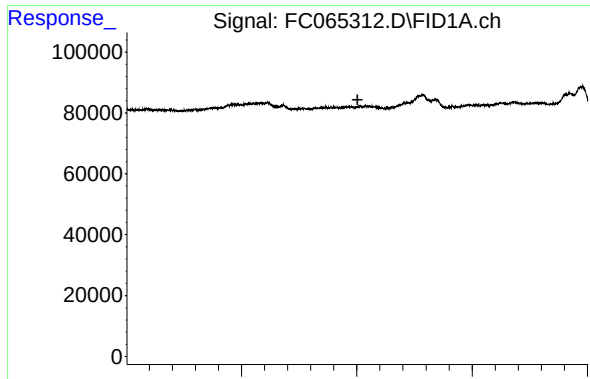

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.503 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

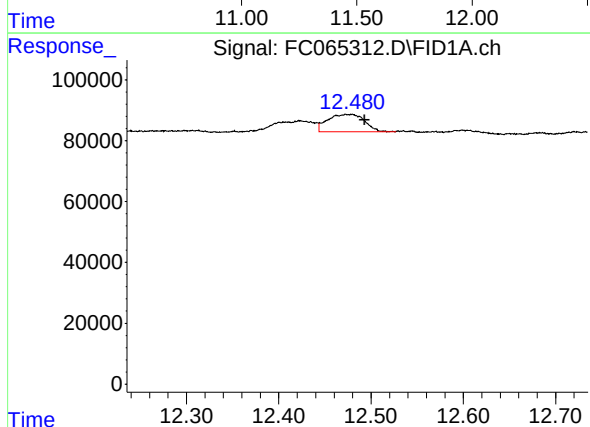


#10 n-Eicosane (C20)

R.T.: 12.480 min
Delta R.T.: -0.013 min
Response: 158908
Conc: 0.84 ug/ml

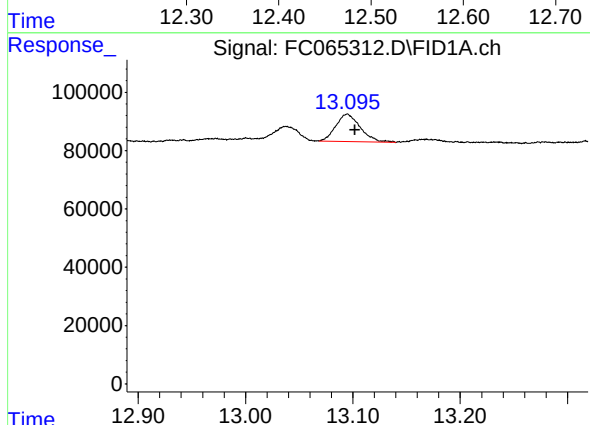


#11 n-Heneicosane (C21)

R.T.: 13.095 min
Delta R.T.: -0.007 min
Response: 148153
Conc: 0.80 ug/ml

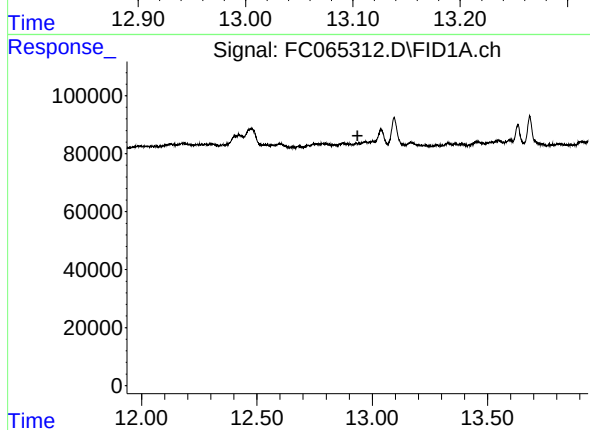

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 12.936 min
Response: 0
Conc: N.D.

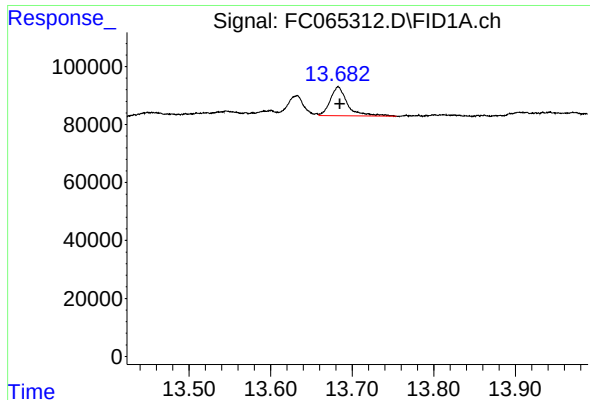

#13 n-Docosane (C22)


R.T.: 13.683 min
Delta R.T.: -0.002 min
Response: 147752
Conc: 0.82 ug/ml

Instrument :
FID_C
ClientSampleId :

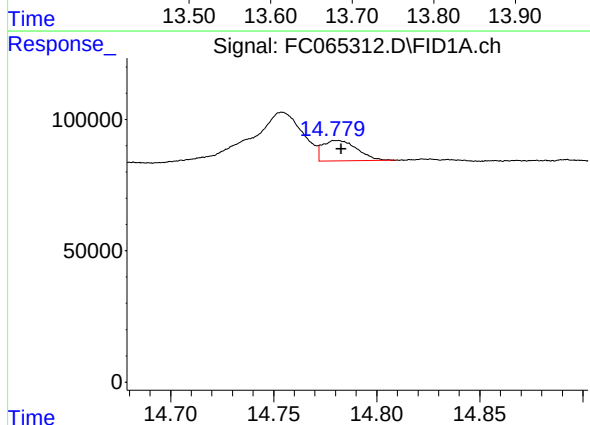


#14 n-Tetracosane (C24)

R.T.: 14.781 min
Delta R.T.: -0.002 min
Response: 90765
Conc: 0.52 ug/ml

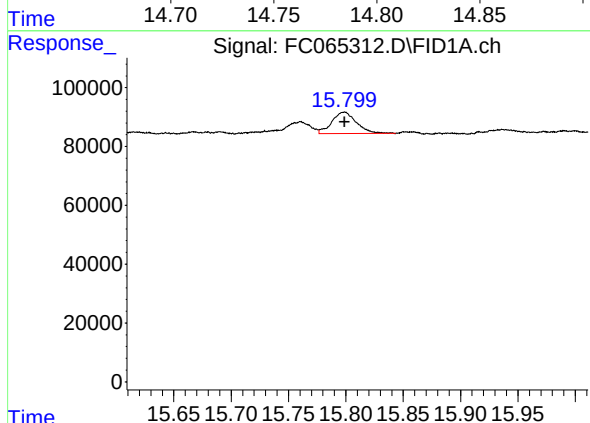


#15 n-Hexacosane (C26)

R.T.: 15.799 min
Delta R.T.: 0.000 min
Response: 110015
Conc: 0.66 ug/ml

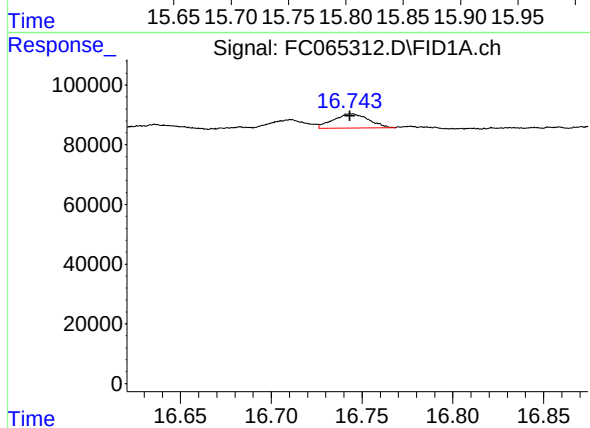

#16 n-Octacosane (C28)


R.T.: 16.744 min
Delta R.T.: 0.000 min
Response: 63727
Conc: 0.40 ug/ml

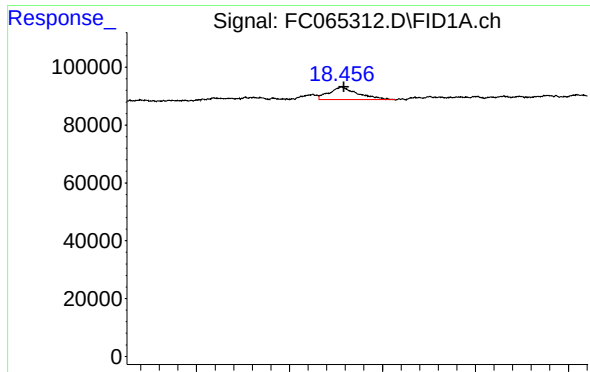

#18 n-Dotriacontane (C32)


R.T.: 18.456 min
Delta R.T.: -0.002 min
Response: 92020
Conc: 0.59 ug/ml

Instrument :
FID_C
ClientSampleId :

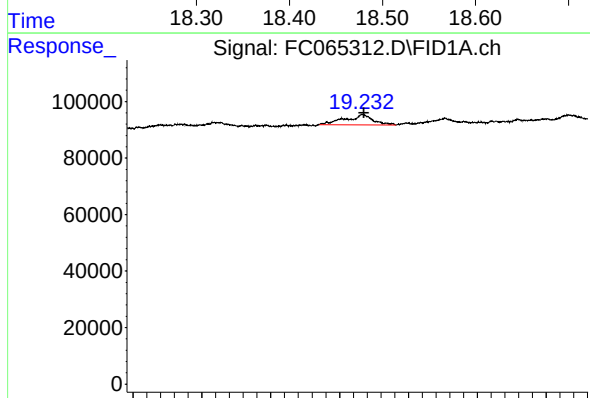

#19 n-Tetratriacontane (C34)

R.T.: 19.233 min
Delta R.T.: -0.002 min
Response: 102978
Conc: 0.67 ug/ml

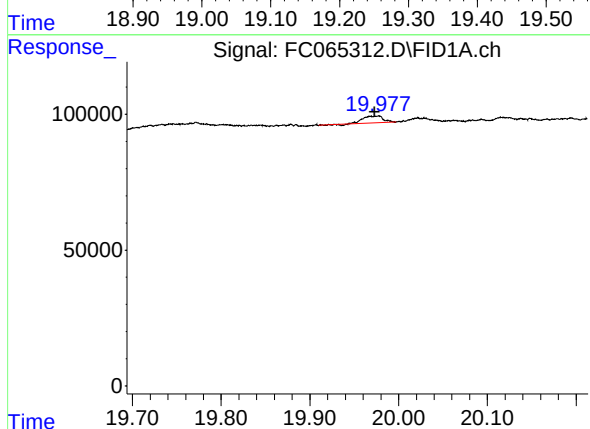

#20 n-Hexatriacontane (C36)

R.T.: 19.978 min
Delta R.T.: 0.005 min
Response: 40336
Conc: 0.26 ug/ml