

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC113023AL\
Data File : FC065322.D
Signal(s) : FID1A.ch
Acq On : 30 Nov 2023 04:19
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 30 23:26:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 112423.M
Quant Title : GC Extractables
QLast Update : Fri Nov 24 13:28:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T n-Tetracosane (C24)	14.758	78984	0.456 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC113023AL\
Data File : FC065322.D
Signal(s) : FID1A.ch
Acq On : 30 Nov 2023 04:19
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 30 23:26:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 112423.M
Quant Title : GC Extractables
QLast Update : Fri Nov 24 13:28:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

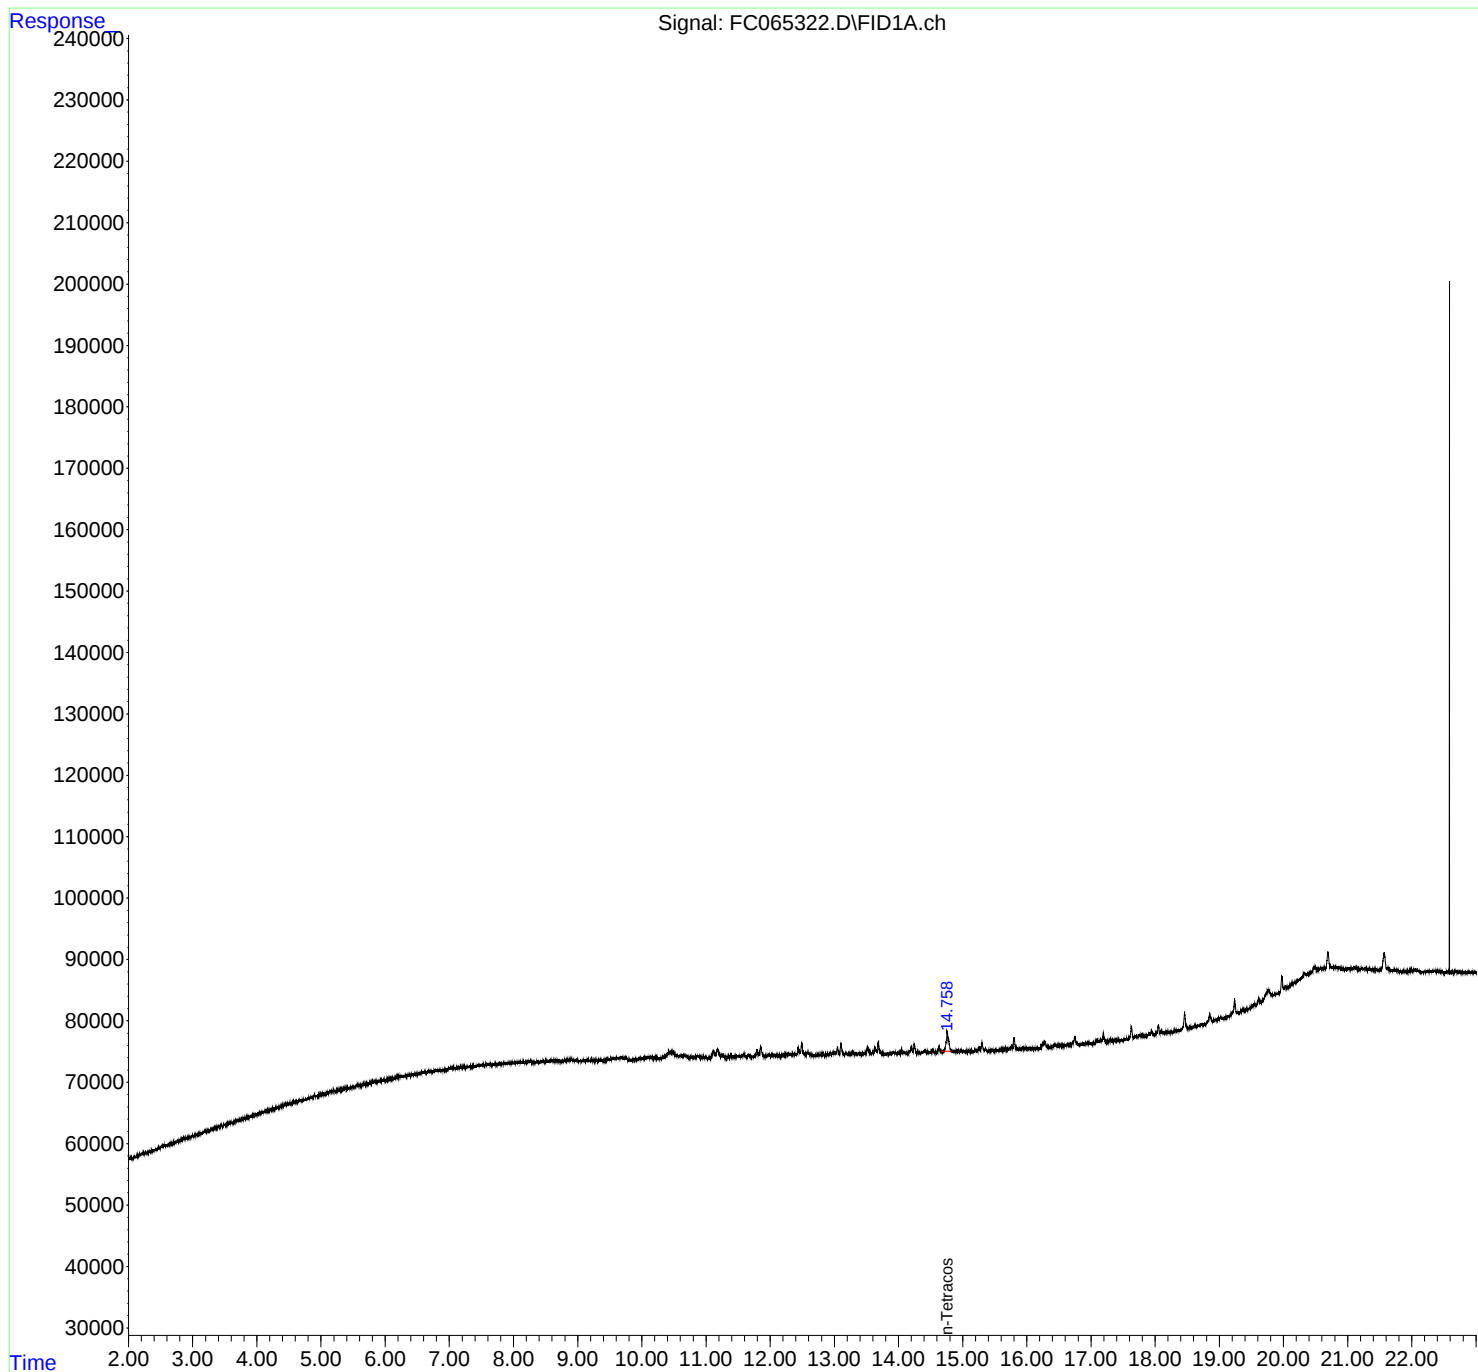


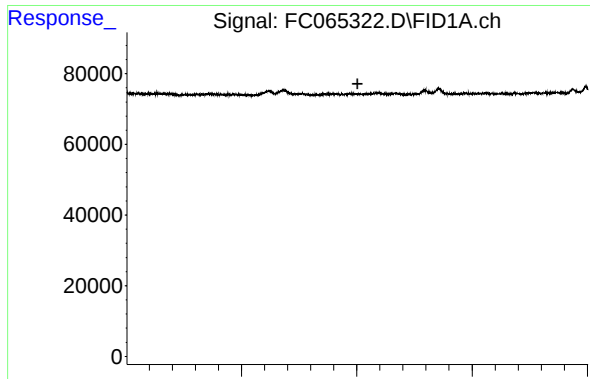

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.503 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

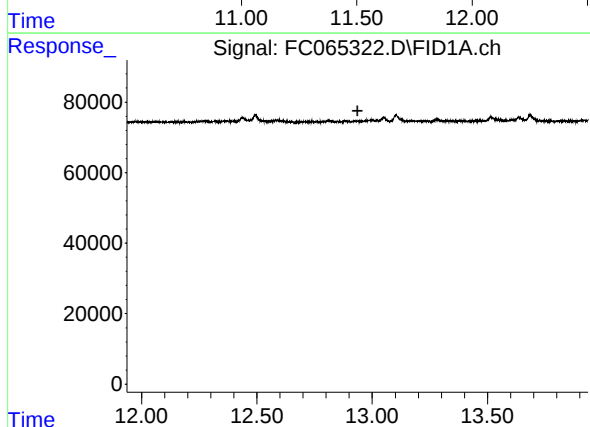

#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.936 min
Response: 0
Conc: N.D.

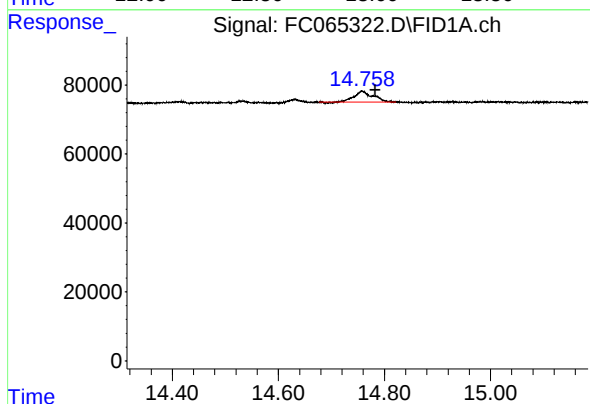

#14 n-Tetracosane (C24)

R.T.: 14.758 min
Delta R.T.: -0.025 min
Response: 78984
Conc: 0.46 ug/ml