

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC120221AL\
 Data File : FC057190.D
 Signal(s) : FID1A.CH
 Acq On : 03 Dec 2021 8:12
 Operator : AJ\MA
 Sample : M4873-11DL 5X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 A6-18-4.5DL

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 12/06/2021
 Supervised By :mohammad ahmed 12/06/2021

Integration File: sample.E
 Quant Time: Dec 03 11:51:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 111921.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 19 00:52:49 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.590	963047	8.299 ug/mlm
Spiked Amount	50.000	Recovery	= 16.60%
12) S 1-chlorooctadecane (S...	13.022	738741	8.115 ug/ml
Spiked Amount	50.000	Recovery	= 16.23%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC120221AL\
Data File : FC057190.D
Signal(s) : FID1A.CH
Acq On : 03 Dec 2021 8:12
Operator : AJ\MA
Sample : M4873-11DL 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
A6-18-4.5DL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/06/2021
Supervised By :mohammad ahmed 12/06/2021

Integration File: sample.E
Quant Time: Dec 03 11:51:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 111921.M
Quant Title : GC Extractables
QLast Update : Fri Nov 19 00:52:49 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

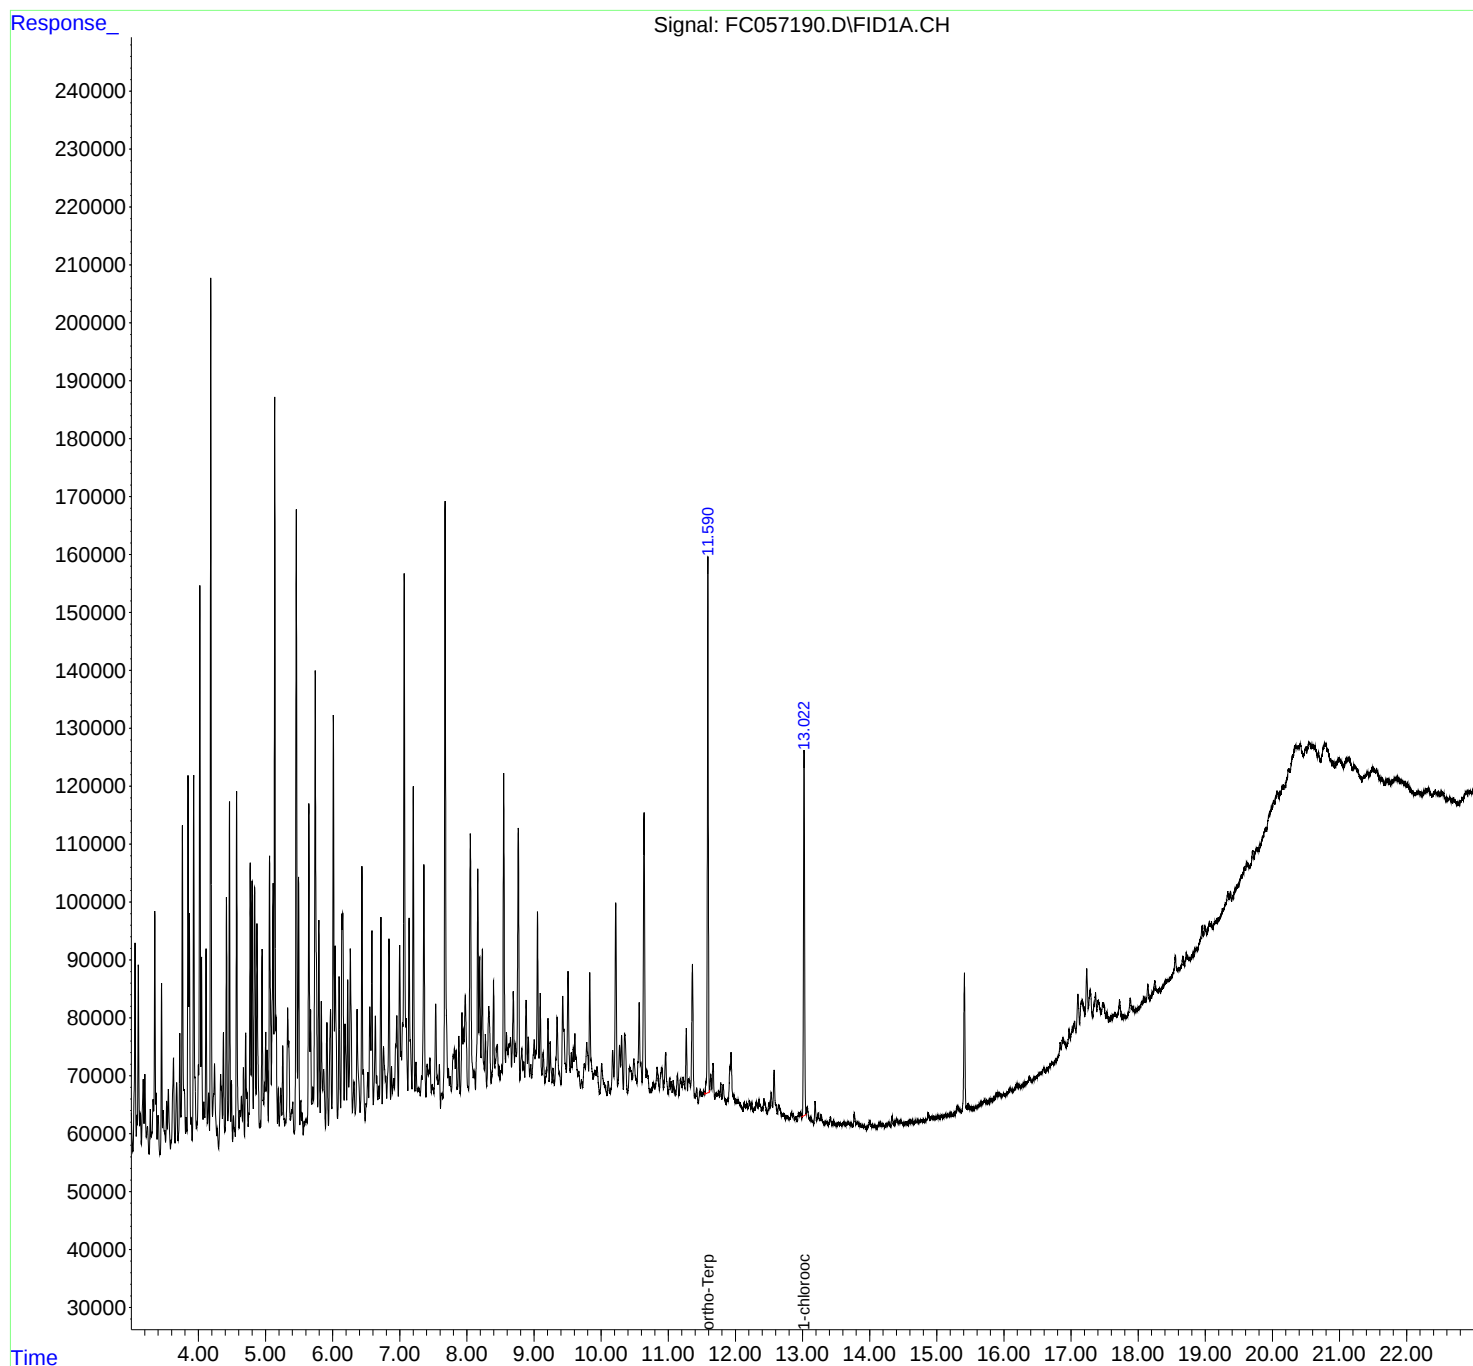

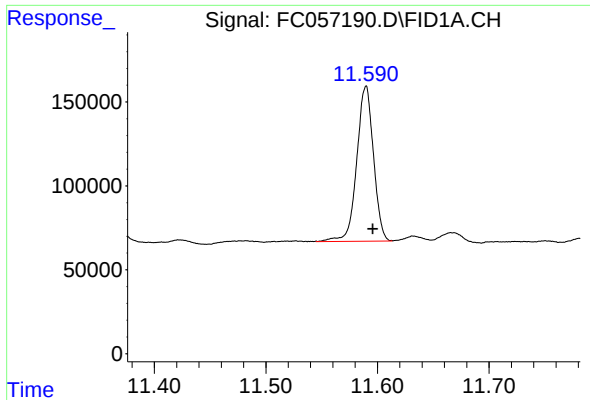


#9 ortho-Terphenyl (SURR)

R.T.: 11.590 min
Delta R.T.: -0.006 min
Response: 963047
Conc: 8.30 ug/ml

Instrument :
FID_C
ClientSampleId :
A6-18-4.5DL

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/06/2021
Supervised By :mohammad ahmed 12/06/2021

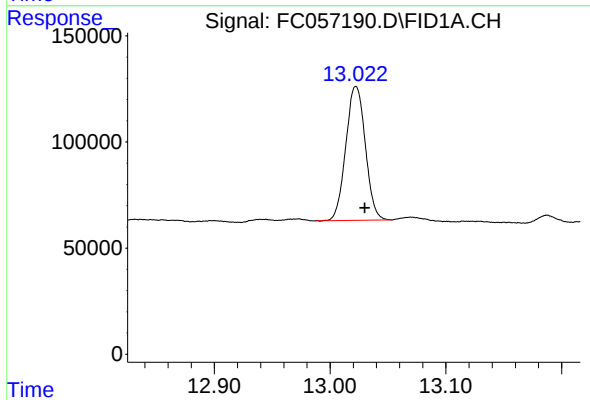

#12 1-chlorooctadecane (SURR)

R.T.: 13.022 min
Delta R.T.: -0.007 min
Response: 738741
Conc: 8.11 ug/ml