

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC120320AL\
 Data File : FC051096.D
 Signal(s) : FID1A.CH
 Acq On : 03 Dec 2020 15:34
 Operator : DD\AJ
 Sample : L4915-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 04 00:27:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 112720.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 30 10:42:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.592	3597507	29.238 ug/ml
Spiked Amount 50.000		Recovery =	58.48%
12) S 1-chlorooctadecane (S...	13.027	3044525	31.209 ug/ml
Spiked Amount 50.000		Recovery =	62.42%
Target Compounds			
10) T n-Eicosane (C20)	12.654f	1379624	11.876 ug/ml
14) T n-Tetracosane (C24)	14.876	784203	6.819 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC120320AL\
Data File : FC051096.D
Signal(s) : FID1A.CH
Acq On : 03 Dec 2020 15:34
Operator : DD\AJ
Sample : L4915-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 04 00:27:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 112720.M
Quant Title : GC Extractables
QLast Update : Mon Nov 30 10:42:25 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

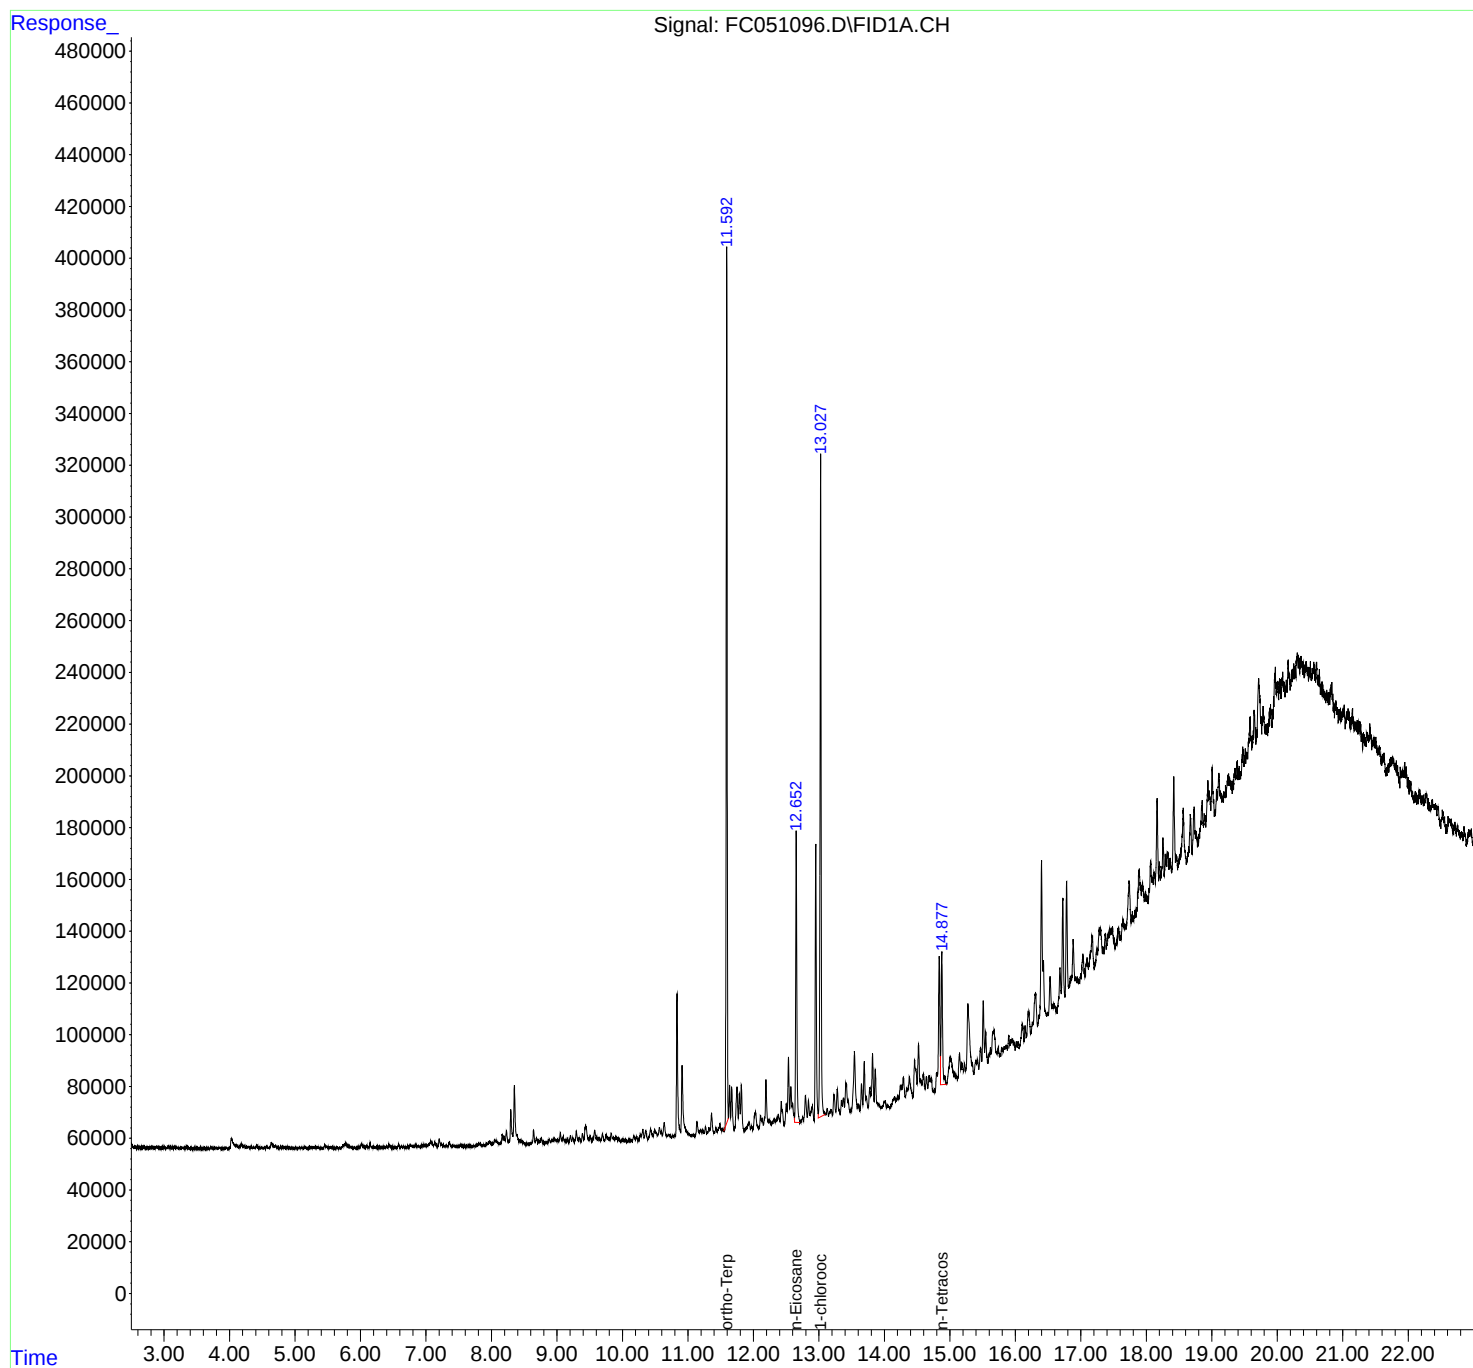


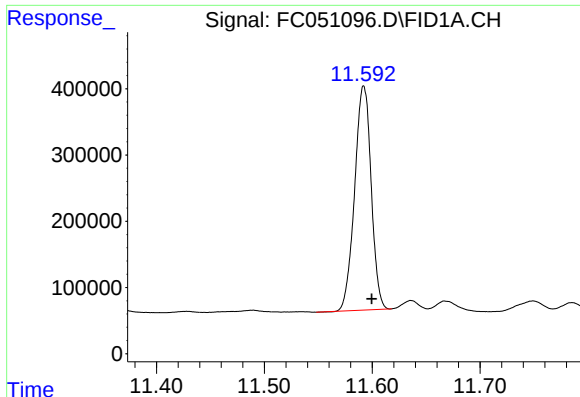

#9 ortho-Terphenyl (SURR)


R.T.: 11.592 min
Delta R.T.: -0.008 min
Response: 3597507
Conc: 29.24 ug/ml

Instrument :
FID_C
ClientSampleId :

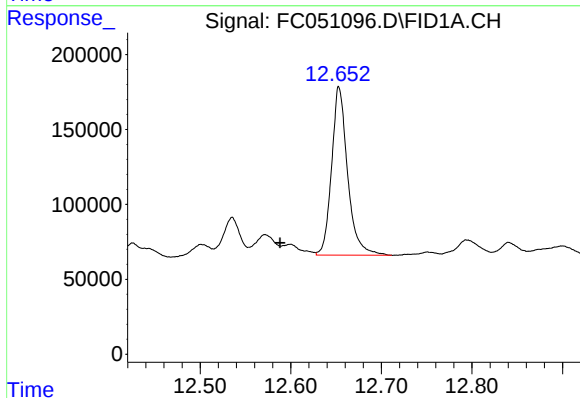


#10 n-Eicosane (C20)

R.T.: 12.654 min
Delta R.T.: 0.065 min
Response: 1379624
Conc: 11.88 ug/ml

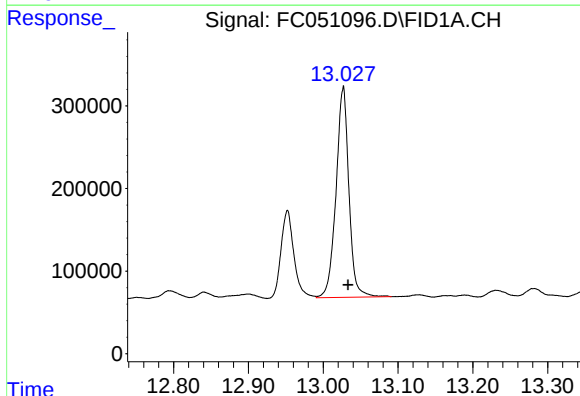

#12 1-chlorooctadecane (SURR)

R.T.: 13.027 min
Delta R.T.: -0.007 min
Response: 3044525
Conc: 31.21 ug/ml

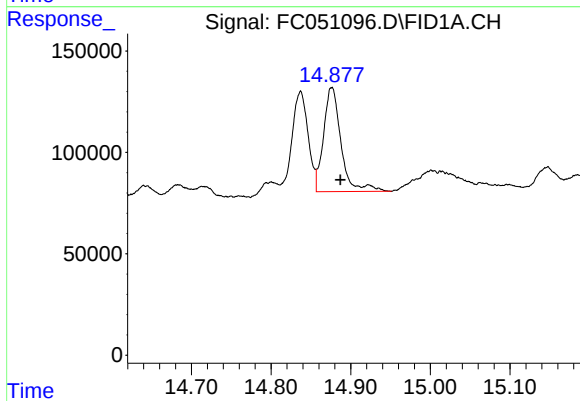

#14 n-Tetracosane (C24)

R.T.: 14.876 min
Delta R.T.: -0.011 min
Response: 784203
Conc: 6.82 ug/ml