

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC120623AL\
 Data File : FC065343.D
 Signal(s) : FID1A.ch
 Acq On : 06 Dec 2023 06:18
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 07 00:03:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 112423.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 24 13:28:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10) T	n-Eicosane (C20)	12.484	73679	0.389 ug/ml
11) T	n-Heneicosane (C21)	13.100	75490	0.409 ug/ml
13) T	n-Docosane (C22)	13.684	60812	0.337 ug/ml
14) T	n-Tetracosane (C24)	14.756	67225	0.388 ug/ml
15) T	n-Hexacosane (C26)	15.797	58399	0.351 ug/ml
17) T	n-Tricontane (C30)	17.626	68759	0.432 ug/ml
18) T	n-Dotriacontane (C32)	18.457	133852	0.851 ug/ml
19) T	n-Tetratriacontane (C34)	19.236	84732	0.549 ug/ml
20) T	n-Hexatriacontane (C36)	19.972	66944	0.437 ug/ml
21) T	n-Octatriacontane (C38)	20.692	63163	0.415 ug/ml
22) T	n-Tetracontane (C40)	21.565	14784	0.099 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC120623AL\
Data File : FC065343.D
Signal(s) : FID1A.ch
Acq On : 06 Dec 2023 06:18
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 07 00:03:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 112423.M
Quant Title : GC Extractables
QLast Update : Fri Nov 24 13:28:29 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

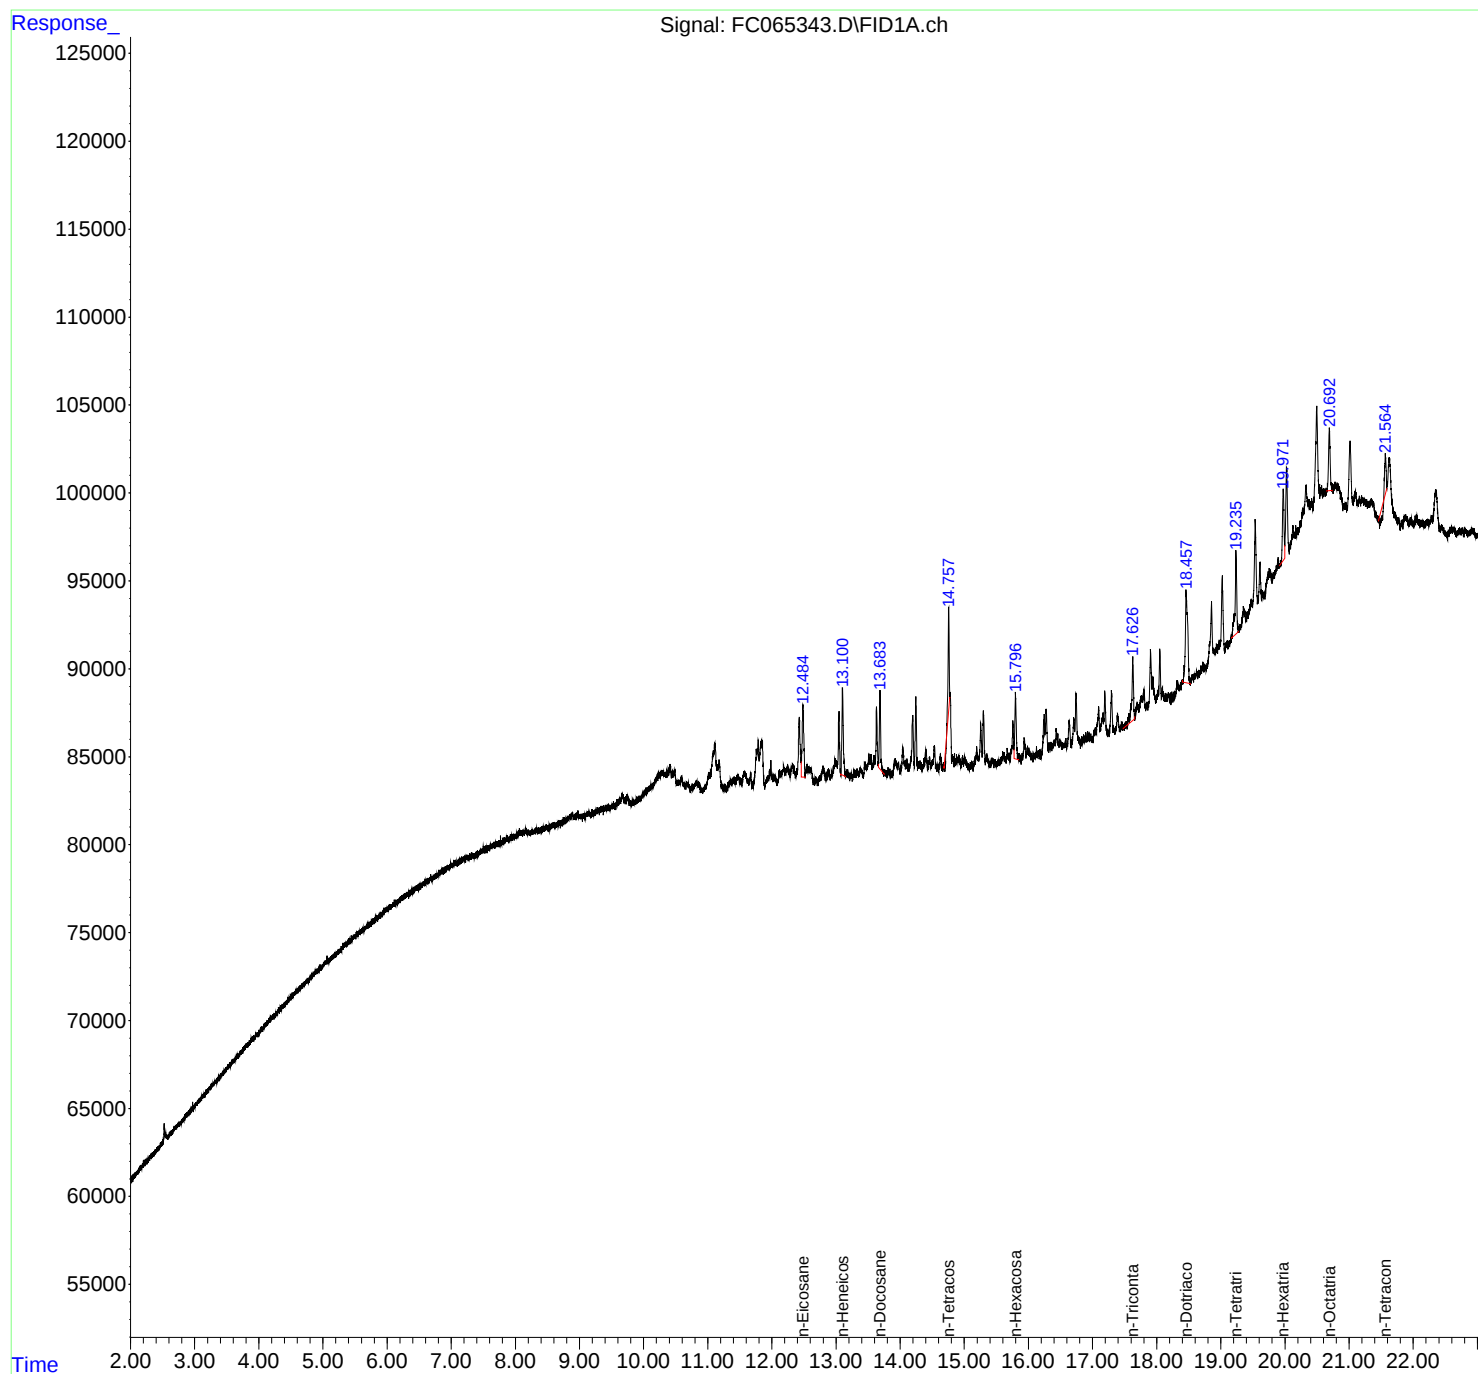

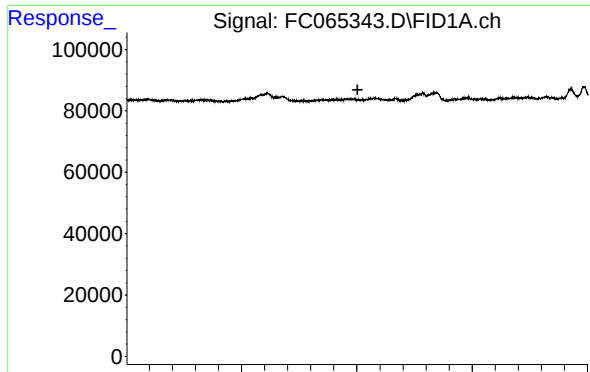


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.503 min
Response: 0
Conc: N.D.

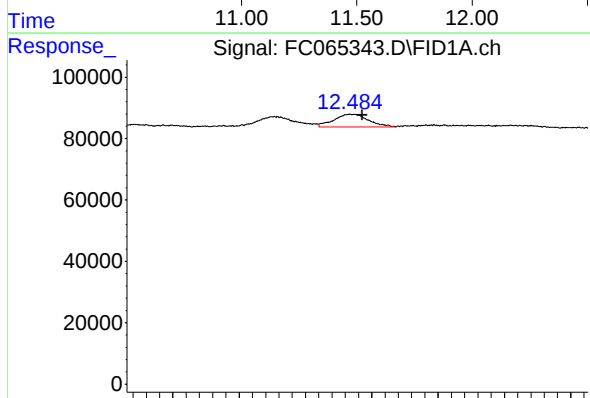


#10 n-Eicosane (C20)

R.T.: 12.484 min
Delta R.T.: -0.009 min
Response: 73679
Conc: 0.39 ug/ml

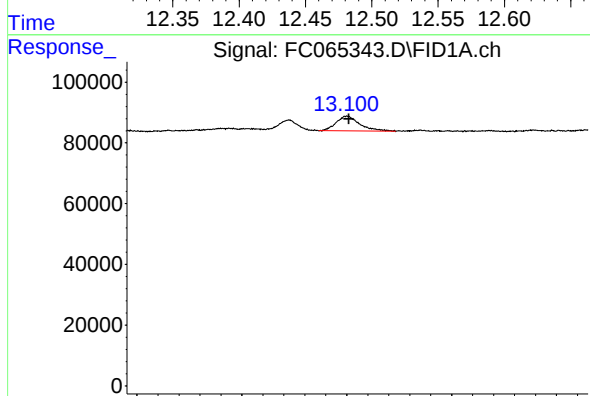


#11 n-Heneicosane (C21)

R.T.: 13.100 min
Delta R.T.: -0.002 min
Response: 75490
Conc: 0.41 ug/ml

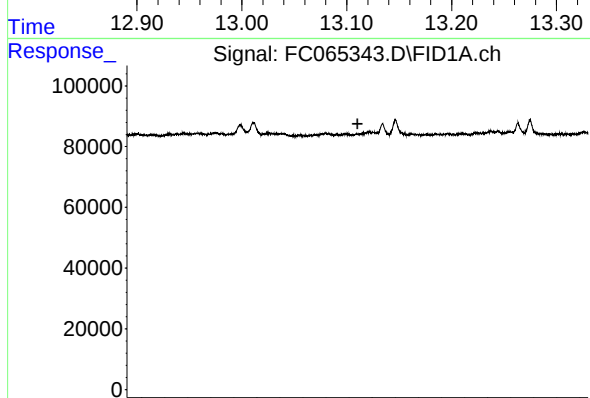


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.936 min
Response: 0
Conc: N.D.

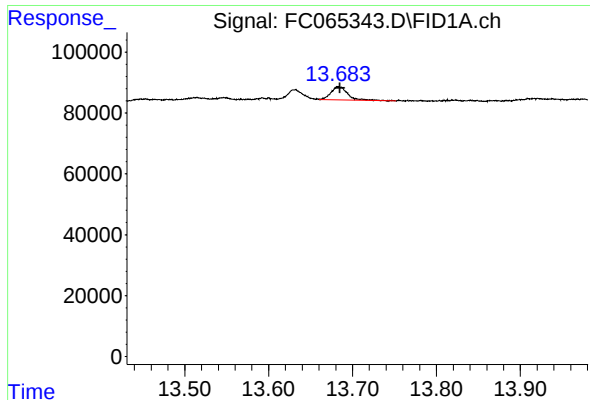


#13 n-Docosane (C22)

R.T.: 13.684 min
Delta R.T.: -0.001 min
Response: 60812
Conc: 0.34 ug/ml

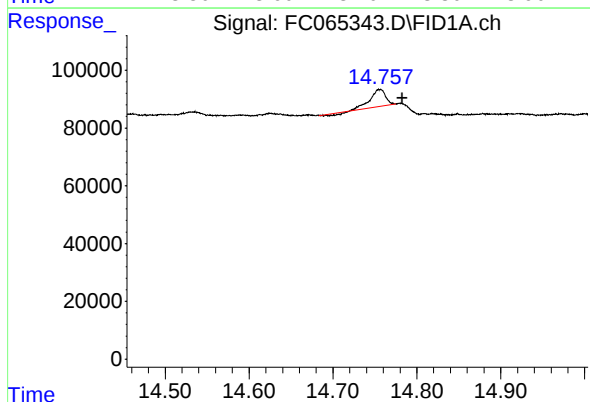


#14 n-Tetracosane (C24)

R.T.: 14.756 min
Delta R.T.: -0.027 min
Response: 67225
Conc: 0.39 ug/ml

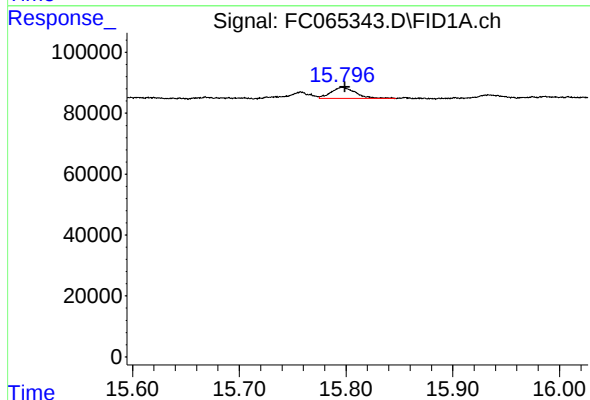


#15 n-Hexacosane (C26)

R.T.: 15.797 min
Delta R.T.: -0.002 min
Response: 58399
Conc: 0.35 ug/ml

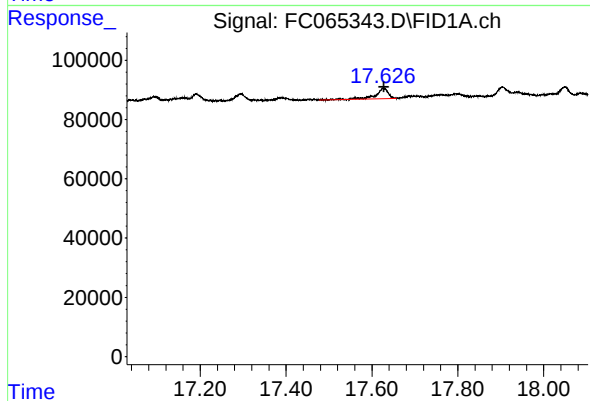


#17 n-Tricontane (C30)

R.T.: 17.626 min
Delta R.T.: -0.002 min
Response: 68759
Conc: 0.43 ug/ml

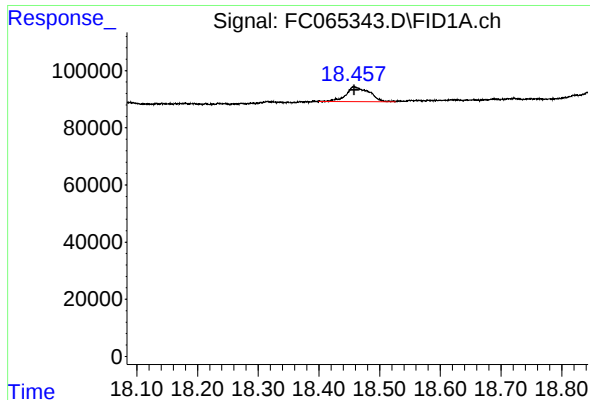


#18 n-Dotriacontane (C32)

R.T.: 18.457 min
Delta R.T.: -0.001 min
Response: 133852
Conc: 0.85 ug/ml

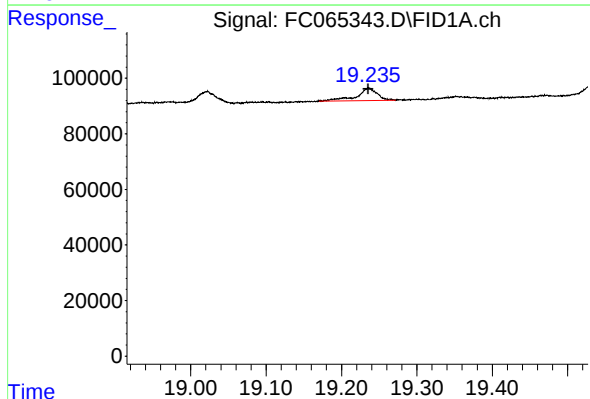


#19 n-Tetratriacontane (C34)

R.T.: 19.236 min
Delta R.T.: 0.000 min
Response: 84732
Conc: 0.55 ug/ml

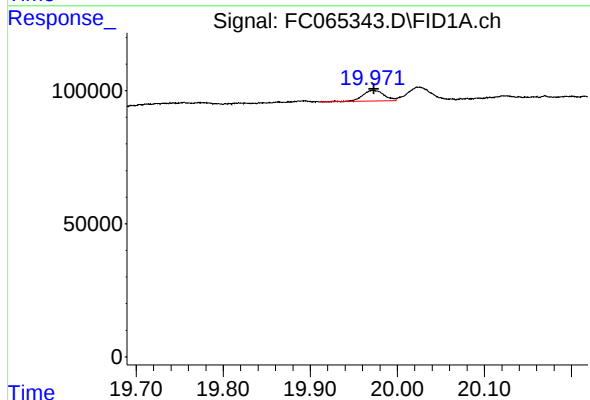


#20 n-Hexatriacontane (C36)

R.T.: 19.972 min
Delta R.T.: -0.001 min
Response: 66944
Conc: 0.44 ug/ml

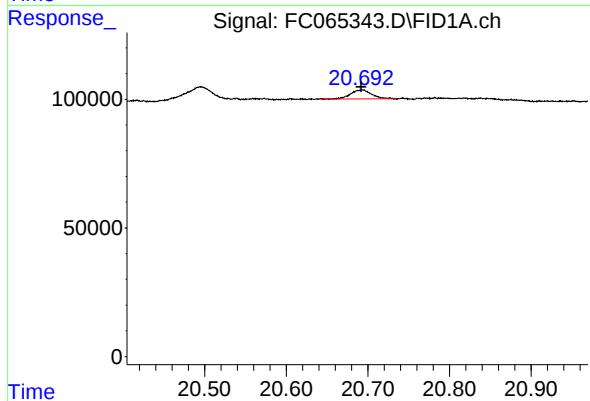

#21 n-Octatriacontane (C38)

R.T.: 20.692 min
Delta R.T.: 0.000 min
Response: 63163
Conc: 0.42 ug/ml

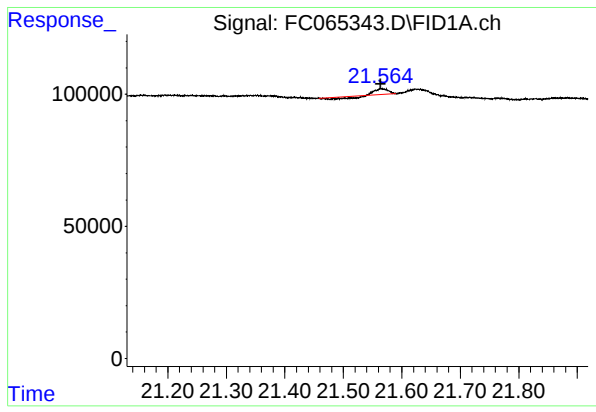

#22 n-Tetracontane (C40)

R.T.: 21.565 min
Delta R.T.: 0.001 min
Response: 14784
Conc: 0.10 ug/ml