

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC120723AL\
 Data File : FC065354.D
 Signal(s) : FID1A.ch
 Acq On : 07 Dec 2023 07:56
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 07 23:27:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 112423.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 24 13:28:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.486	170888	0.903 ug/ml
11) T n-Heneicosane (C21)	13.101	164797	0.892 ug/ml
13) T n-Docosane (C22)	13.686	164351	0.911 ug/ml
14) T n-Tetracosane (C24)	14.786	107266	0.619 ug/ml
15) T n-Hexacosane (C26)	15.802	96005	0.577 ug/ml
16) T n-Octacosane (C28)	16.747	88842	0.555 ug/ml
17) T n-Tricontane (C30)	17.629	72968	0.458 ug/ml
18) T n-Dotriacontane (C32)	18.460	96468	0.614 ug/ml
20) T n-Hexatriacontane (C36)	19.978	43625	0.285 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC120723AL\
Data File : FC065354.D
Signal(s) : FID1A.ch
Acq On : 07 Dec 2023 07:56
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 07 23:27:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 112423.M
Quant Title : GC Extractables
QLast Update : Fri Nov 24 13:28:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

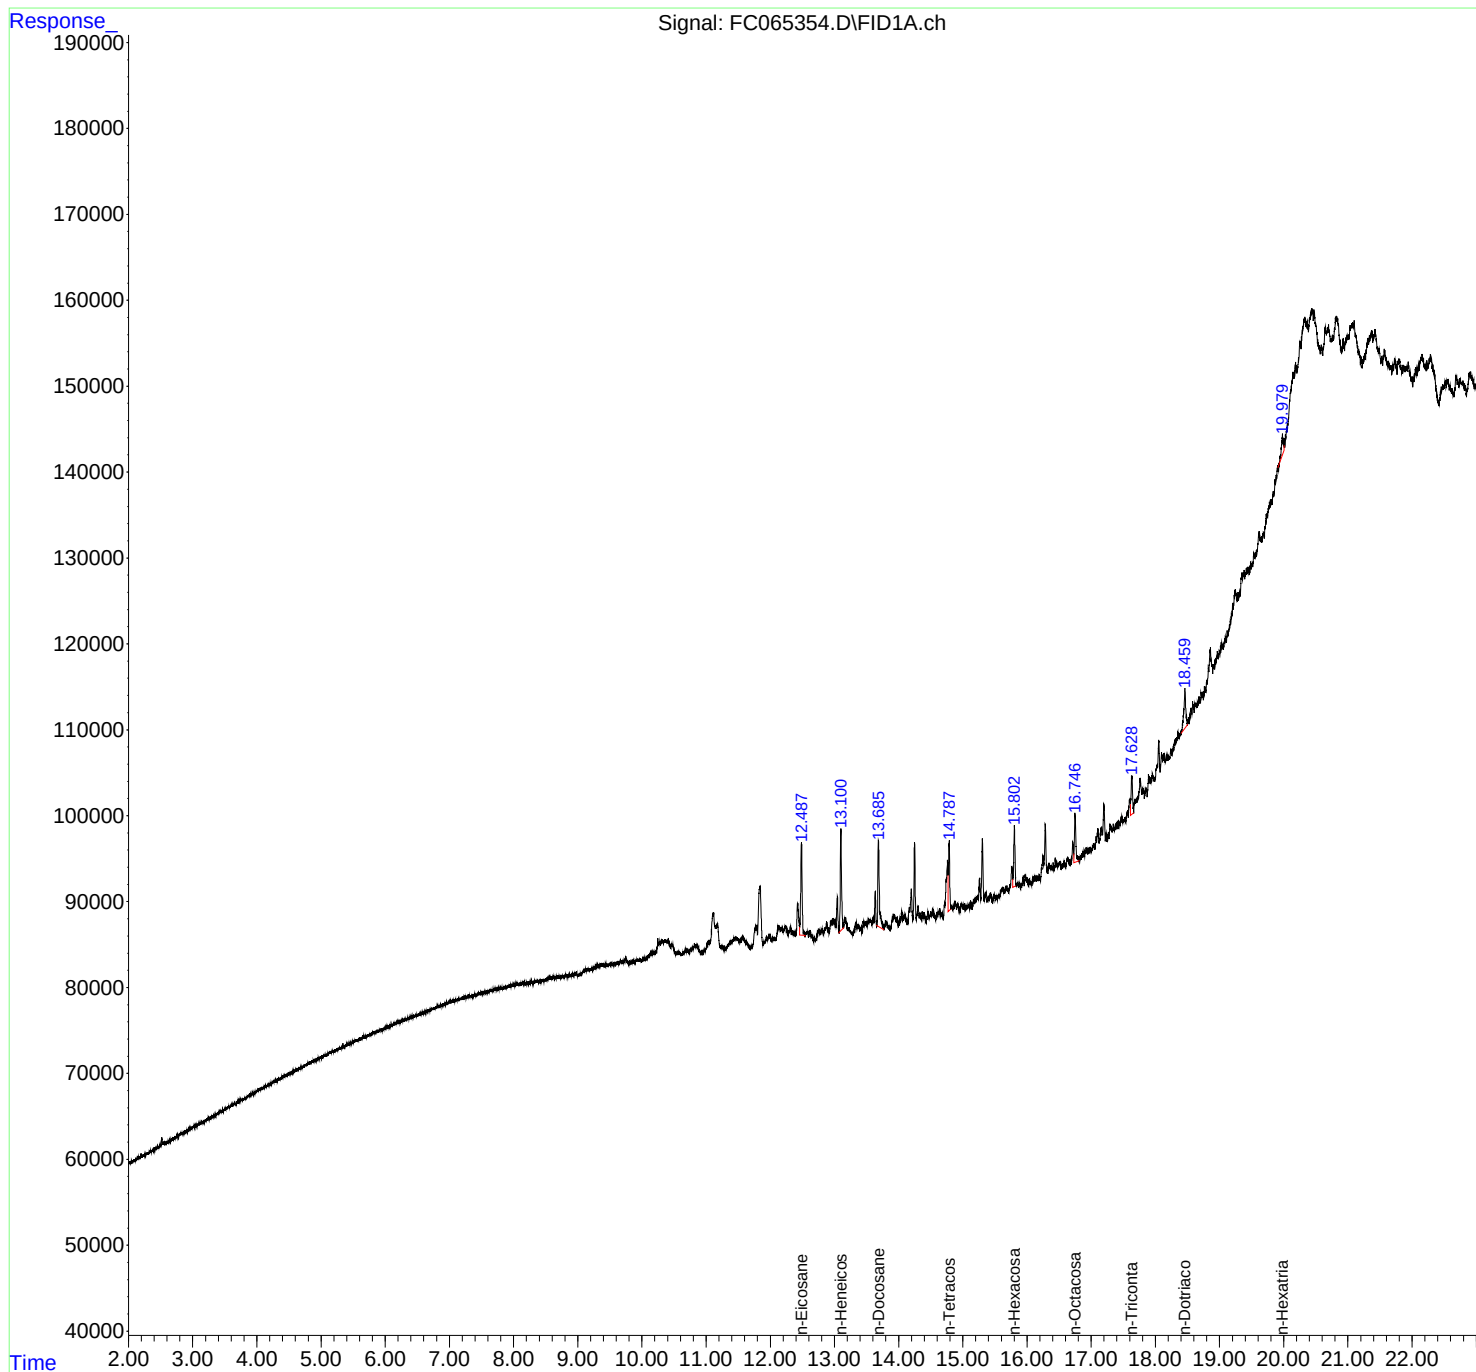


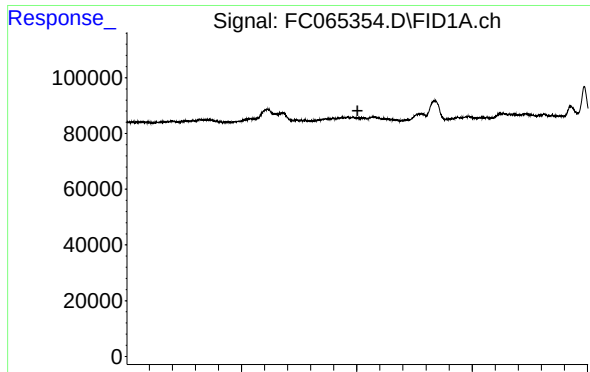

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.503 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

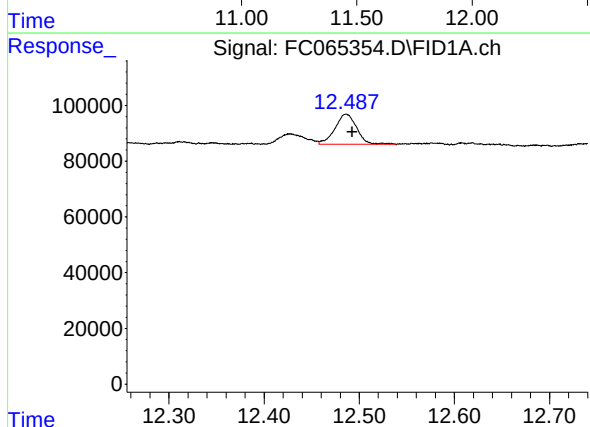


#10 n-Eicosane (C20)

R.T.: 12.486 min
Delta R.T.: -0.007 min
Response: 170888
Conc: 0.90 ug/ml

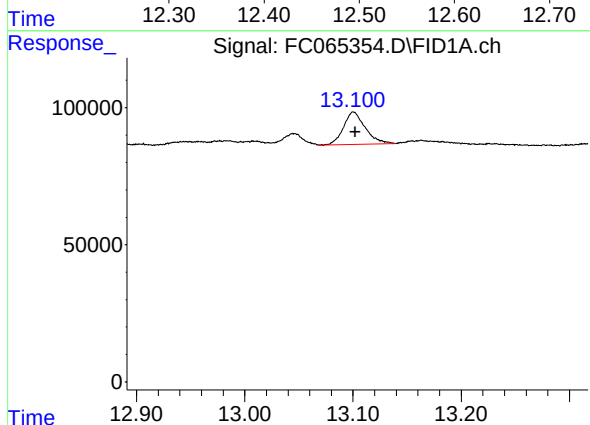


#11 n-Heneicosane (C21)

R.T.: 13.101 min
Delta R.T.: -0.001 min
Response: 164797
Conc: 0.89 ug/ml

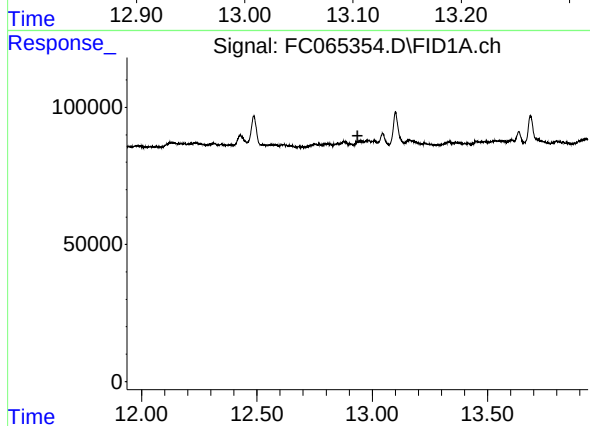

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 12.936 min
Response: 0
Conc: N.D.

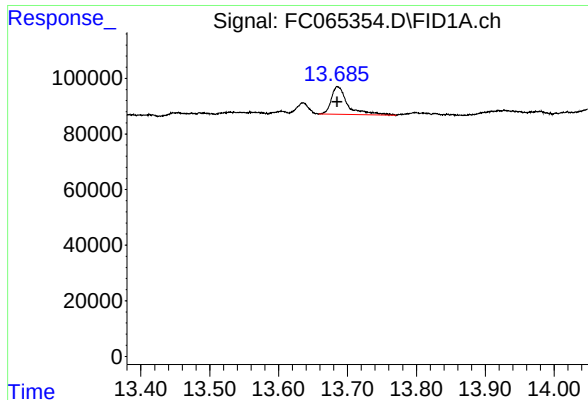

#13 n-Docosane (C22)


R.T.: 13.686 min
Delta R.T.: 0.000 min
Response: 164351
Conc: 0.91 ug/ml

Instrument :
FID_C
ClientSampleId :

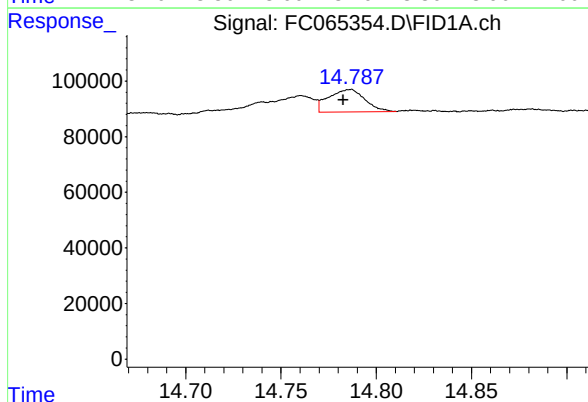


#14 n-Tetracosane (C24)

R.T.: 14.786 min
Delta R.T.: 0.003 min
Response: 107266
Conc: 0.62 ug/ml

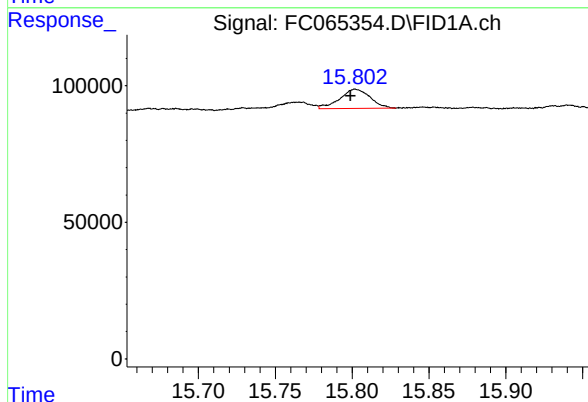


#15 n-Hexacosane (C26)

R.T.: 15.802 min
Delta R.T.: 0.003 min
Response: 96005
Conc: 0.58 ug/ml

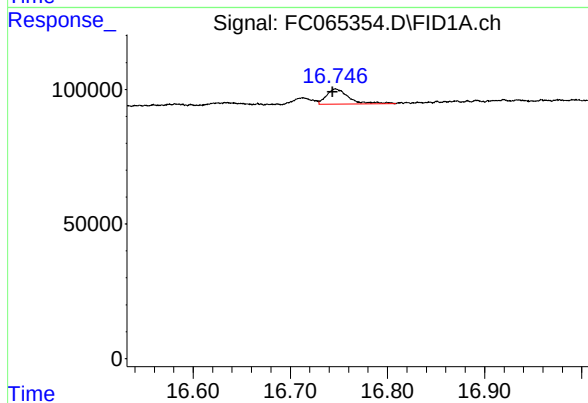

#16 n-Octacosane (C28)


R.T.: 16.747 min
Delta R.T.: 0.003 min
Response: 88842
Conc: 0.56 ug/ml

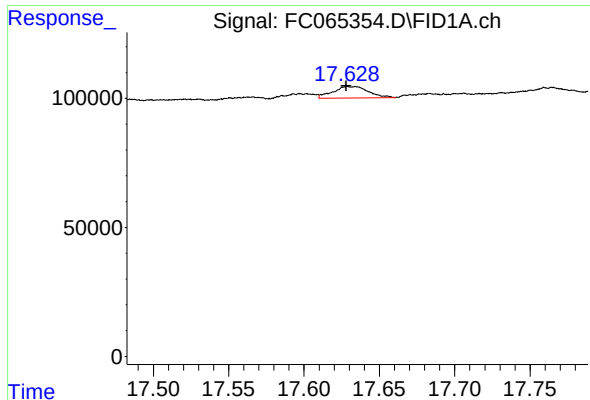

#17 n-Tricontane (C30)


R.T.: 17.629 min
Delta R.T.: 0.001 min
Response: 72968
Conc: 0.46 ug/ml

Instrument :
FID_C
ClientSampleId :

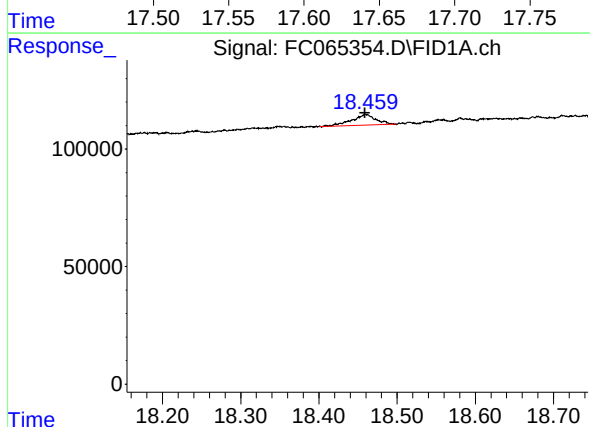

#18 n-Dotriacontane (C32)

R.T.: 18.460 min
Delta R.T.: 0.001 min
Response: 96468
Conc: 0.61 ug/ml

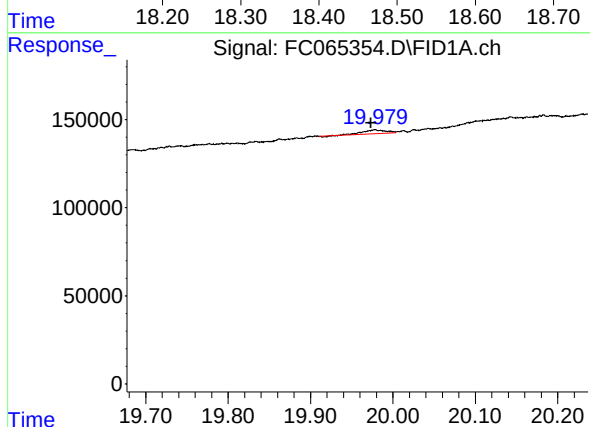

#20 n-Hexatriacontane (C36)

R.T.: 19.978 min
Delta R.T.: 0.005 min
Response: 43625
Conc: 0.28 ug/ml