

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121018AL\
 Data File : FC038105.D
 Signal(s) : FID1A.CH
 Acq On : 11 Dec 2018 3:41
 Operator : AJ\SJ
 Sample : J6319-13DL 5X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 067_DUP-1DL

Integration File: autoint1.e
 Quant Time: Dec 11 09:44:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 121018.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 10 17:11:09 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.280	426761	3.274 ug/ml
Spiked Amount 50.000		Recovery =	6.55%
12) S 1-chlorooctadecane (S...	12.723	347124	3.443 ug/ml
Spiked Amount 50.000		Recovery =	6.89%
Target Compounds			
1) T n-Nonane (C9)	3.132	435672	4.189 ug/ml
3) T A~Naphthalene (C11.7)	5.773	956125	8.139 ug/ml
4) T n-Dodecane (C12)	6.195	381792	3.536 ug/ml
5) T A~2-methylnaphthalene...	6.780	365504	3.111 ug/ml
6) T n-Tetradecane (C14)	8.023	46370	0.415 ug/ml
10) T n-Eicosane (C20)	12.320	102828	0.856 ug/ml
14) T n-Tetracosane (C24)	14.533	54584	0.475 ug/ml
17) T n-Tricontane (C30)	17.418	26609	0.242 ug/ml
18) T n-Dotriacontane (C32)	18.275	91260	0.891 ug/ml
19) T n-Tetratriacontane (C34)	19.028	35402	0.402 ug/ml
22) T n-Tetracontane (C40)	21.315	405745	4.643 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121018AL\
Data File : FC038105.D
Signal(s) : FID1A.CH
Acq On : 11 Dec 2018 3:41
Operator : AJ\SJ
Sample : J6319-13DL 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_C
ClientSampled :
067_DUP-1DL

Integration File: autoint1.e
Quant Time: Dec 11 09:44:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 121018.M
Quant Title : GC Extractables
QLast Update : Mon Dec 10 17:11:09 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

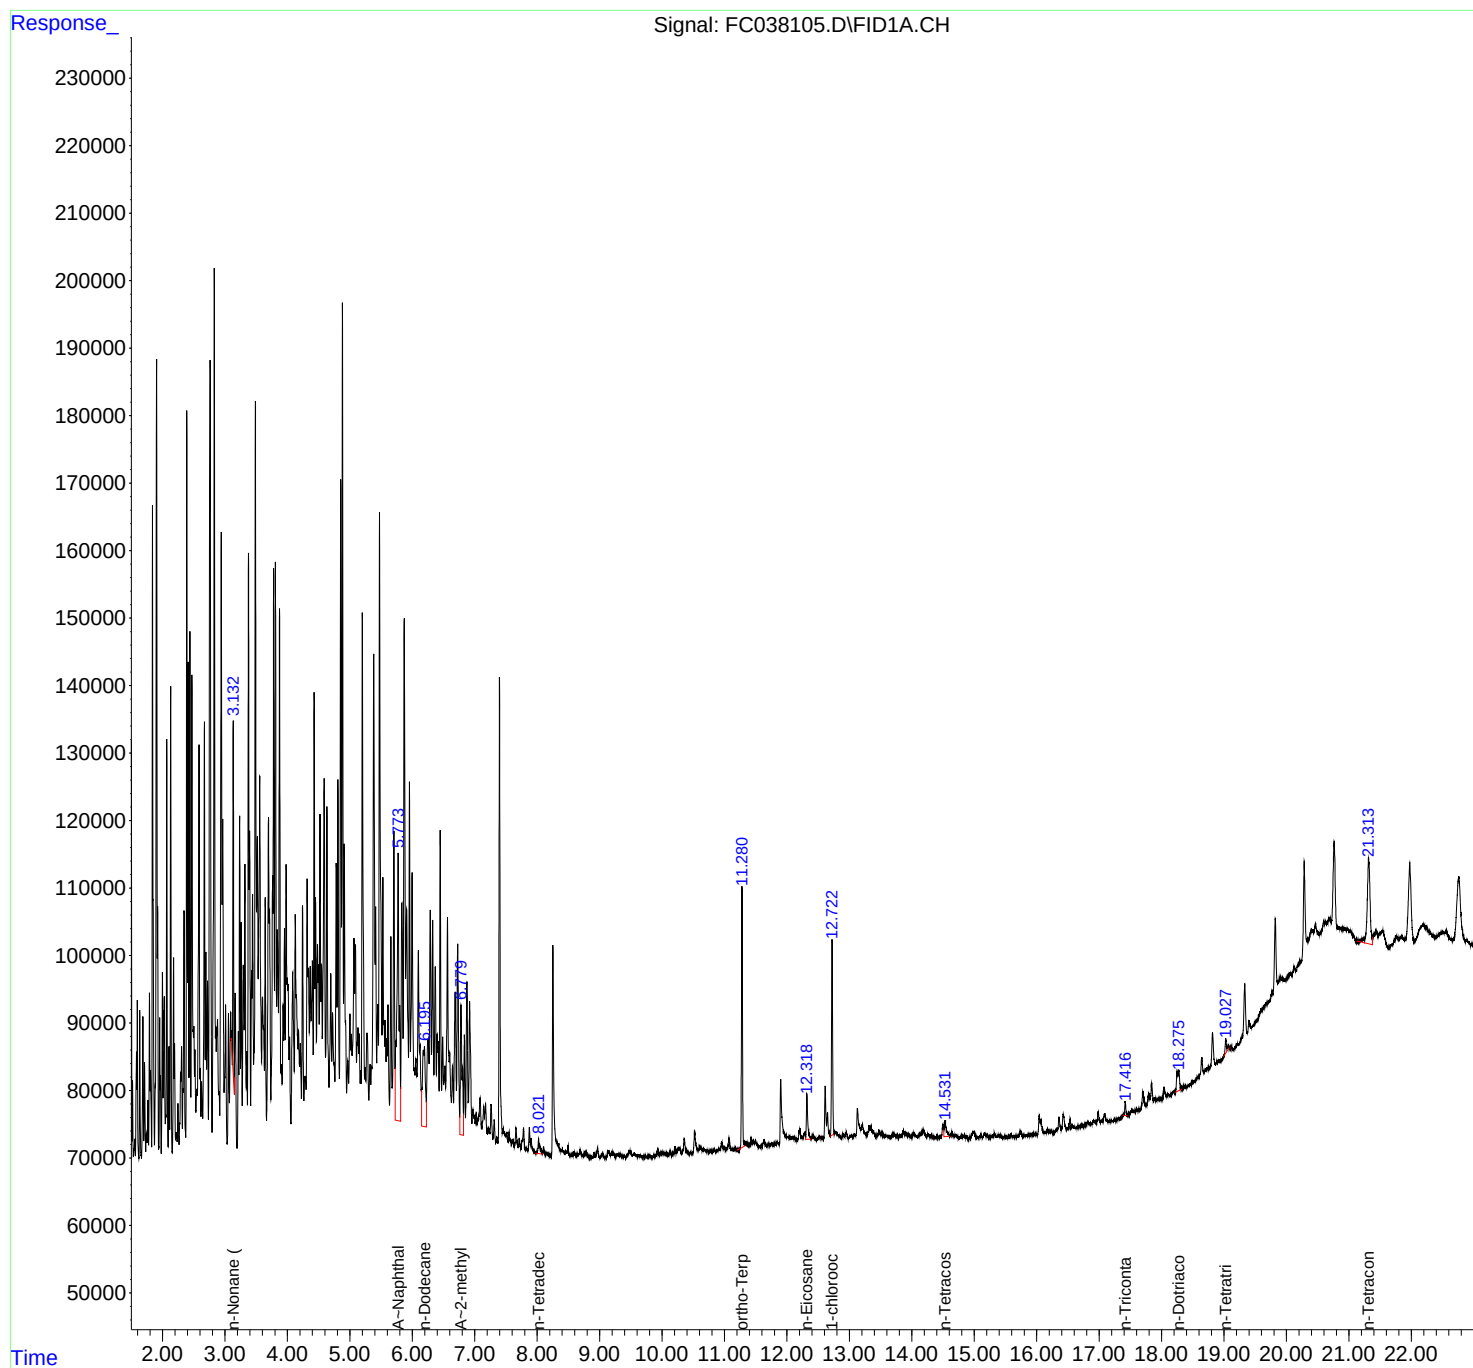


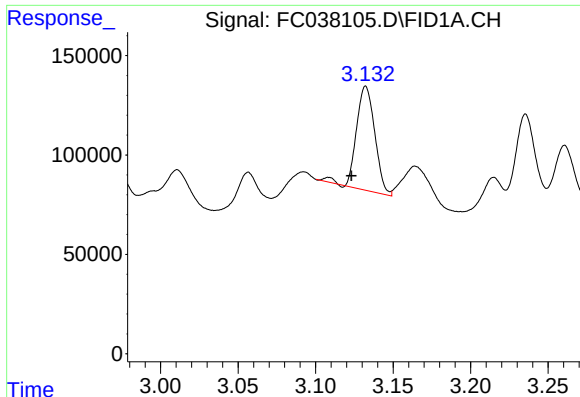

#1 n-Nonane (C9)


R.T.: 3.132 min
Delta R.T.: 0.009 min
Response: 435672
Conc: 4.19 ug/ml

Instrument :
FID_C
ClientSampleId :
067_DUP-1DL

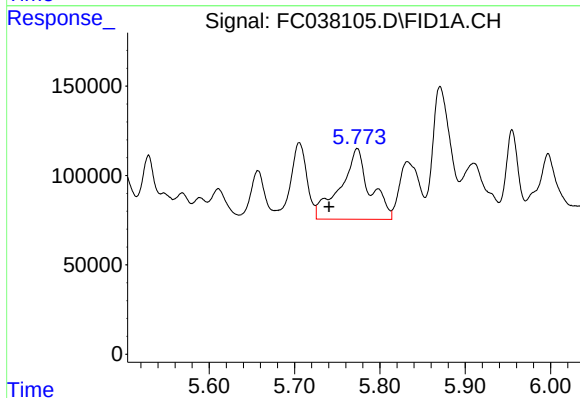


#3 A~Naphthalene (C11.7)

R.T.: 5.773 min
Delta R.T.: 0.033 min
Response: 956125
Conc: 8.14 ug/ml

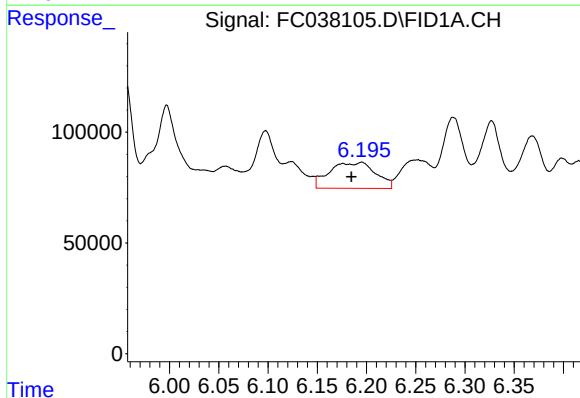


#4 n-Dodecane (C12)

R.T.: 6.195 min
Delta R.T.: 0.010 min
Response: 381792
Conc: 3.54 ug/ml

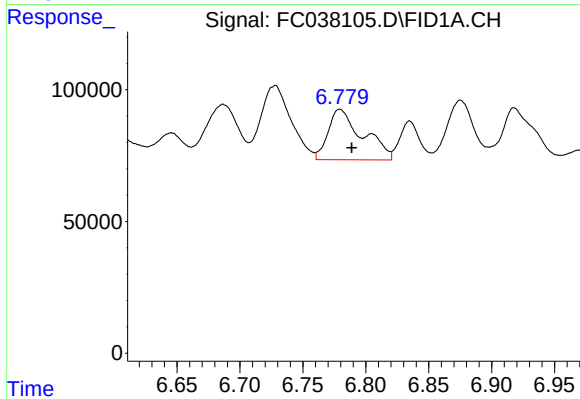

#5 A~2-methylnaphthalene (C12.89)


R.T.: 6.780 min
Delta R.T.: -0.009 min
Response: 365504
Conc: 3.11 ug/ml

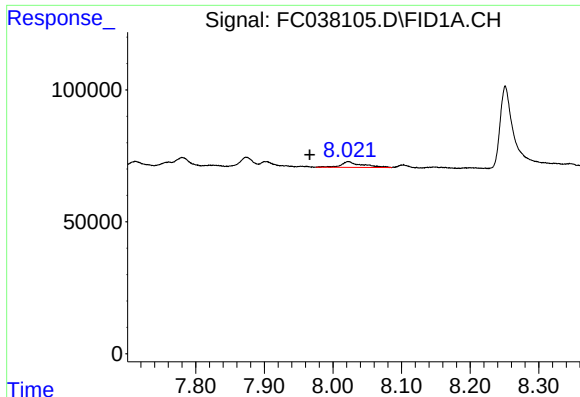

#6 n-Tetradecane (C14)


R.T.: 8.023 min
Delta R.T.: 0.056 min
Response: 46370
Conc: 0.42 ug/ml

Instrument :
FID_C
ClientSampleId :
067_DUP-1DL

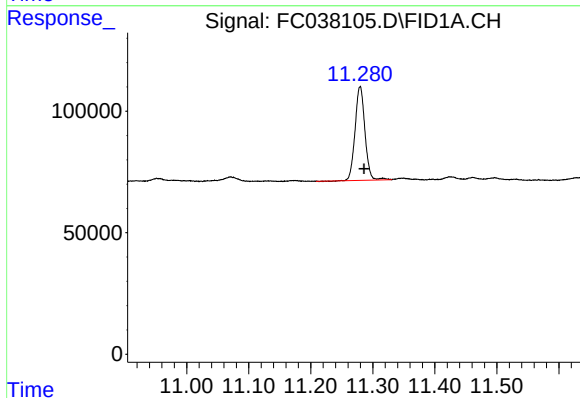


#9 ortho-Terphenyl (SURR)

R.T.: 11.280 min
Delta R.T.: -0.006 min
Response: 426761
Conc: 3.27 ug/ml

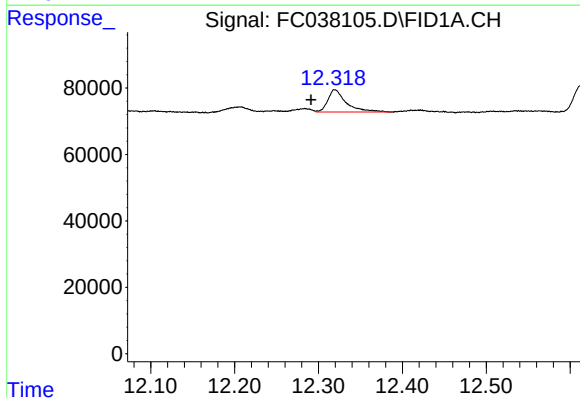


#10 n-Eicosane (C20)

R.T.: 12.320 min
Delta R.T.: 0.029 min
Response: 102828
Conc: 0.86 ug/ml

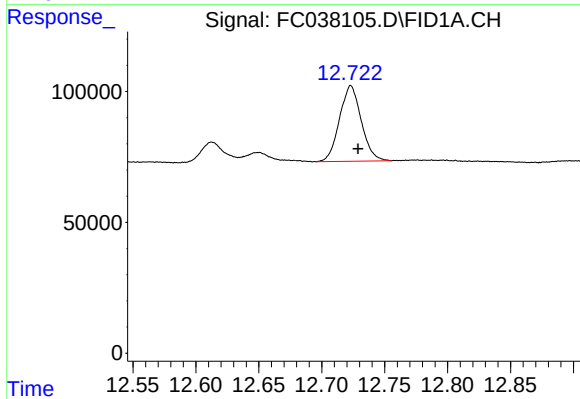

#12 1-chlorooctadecane (SURR)


R.T.: 12.723 min
Delta R.T.: -0.006 min
Response: 347124
Conc: 3.44 ug/ml

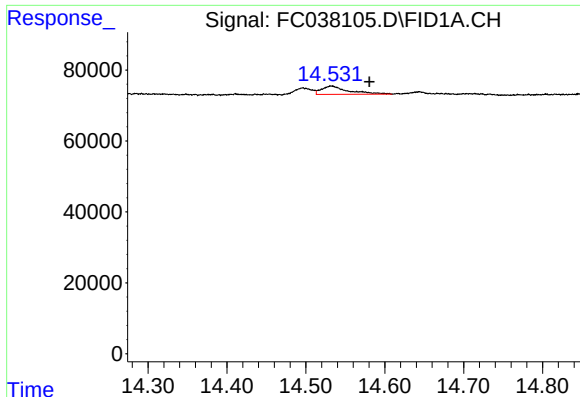

#14 n-Tetracosane (C24)


R.T.: 14.533 min
Delta R.T.: -0.048 min
Response: 54584
Conc: 0.48 ug/ml

Instrument :
FID_C
ClientSampleId :
067_DUP-1DL

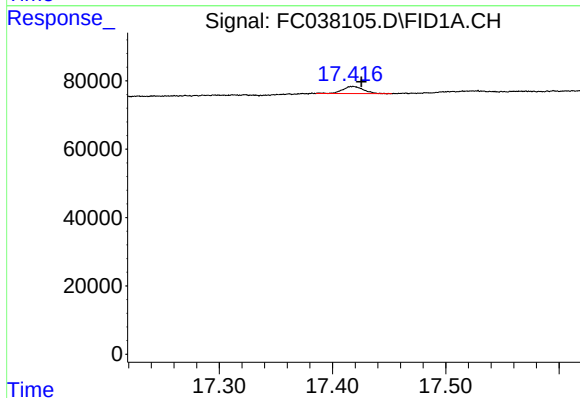


#17 n-Tricontane (C30)

R.T.: 17.418 min
Delta R.T.: -0.007 min
Response: 26609
Conc: 0.24 ug/ml

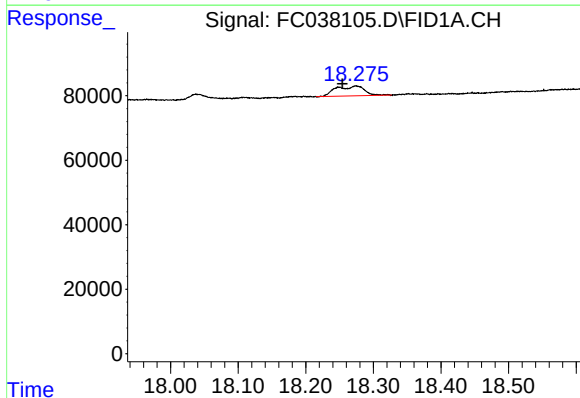


#18 n-Dotriacontane (C32)

R.T.: 18.275 min
Delta R.T.: 0.020 min
Response: 91260
Conc: 0.89 ug/ml

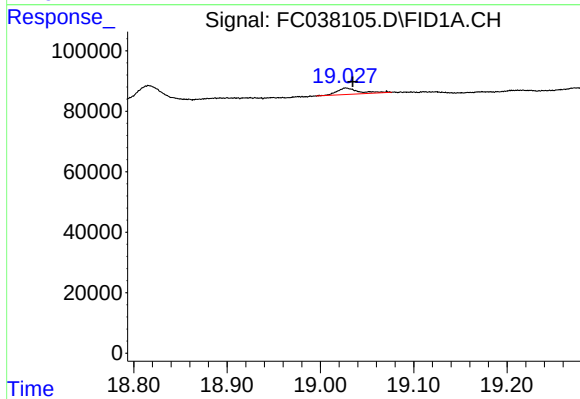

#19 n-Tetratriacontane (C34)

R.T.: 19.028 min
Delta R.T.: -0.007 min
Response: 35402
Conc: 0.40 ug/ml

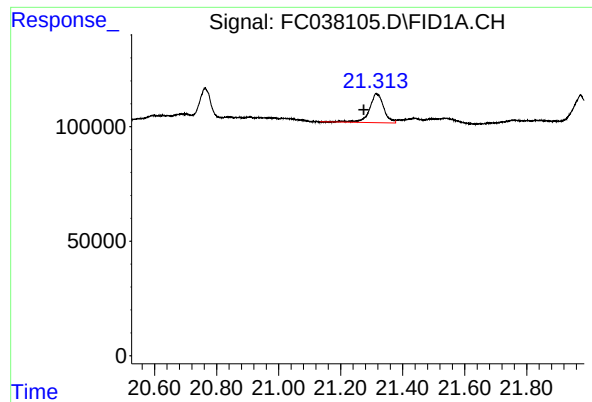

#22 n-Tetracontane (C40)

R.T.: 21.315 min
Delta R.T.: 0.041 min
Response: 405745
Conc: 4.64 ug/ml

Instrument :
FID_C
ClientSampleId :
067_DUP-1DL