

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121018AL\
 Data File : FC038109.D
 Signal(s) : FID1A.CH
 Acq On : 11 Dec 2018 6:06
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 11 09:44:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 121018.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 10 17:11:09 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
17) T n-Tricontane (C30)	17.423	37868	0.345 ug/ml
18) T n-Dotriacontane (C32)	18.252	76463	0.747 ug/ml
19) T n-Tetratriacontane (C34)	19.031	38000	0.431 ug/ml
20) T n-Hexatriacontane (C36)	19.769	21595	0.276 ug/ml
22) T n-Tetracontane (C40)	21.317	59856	0.685 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121018AL\
Data File : FC038109.D
Signal(s) : FID1A.CH
Acq On : 11 Dec 2018 6:06
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 09:44:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 121018.M
Quant Title : GC Extractables
QLast Update : Mon Dec 10 17:11:09 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

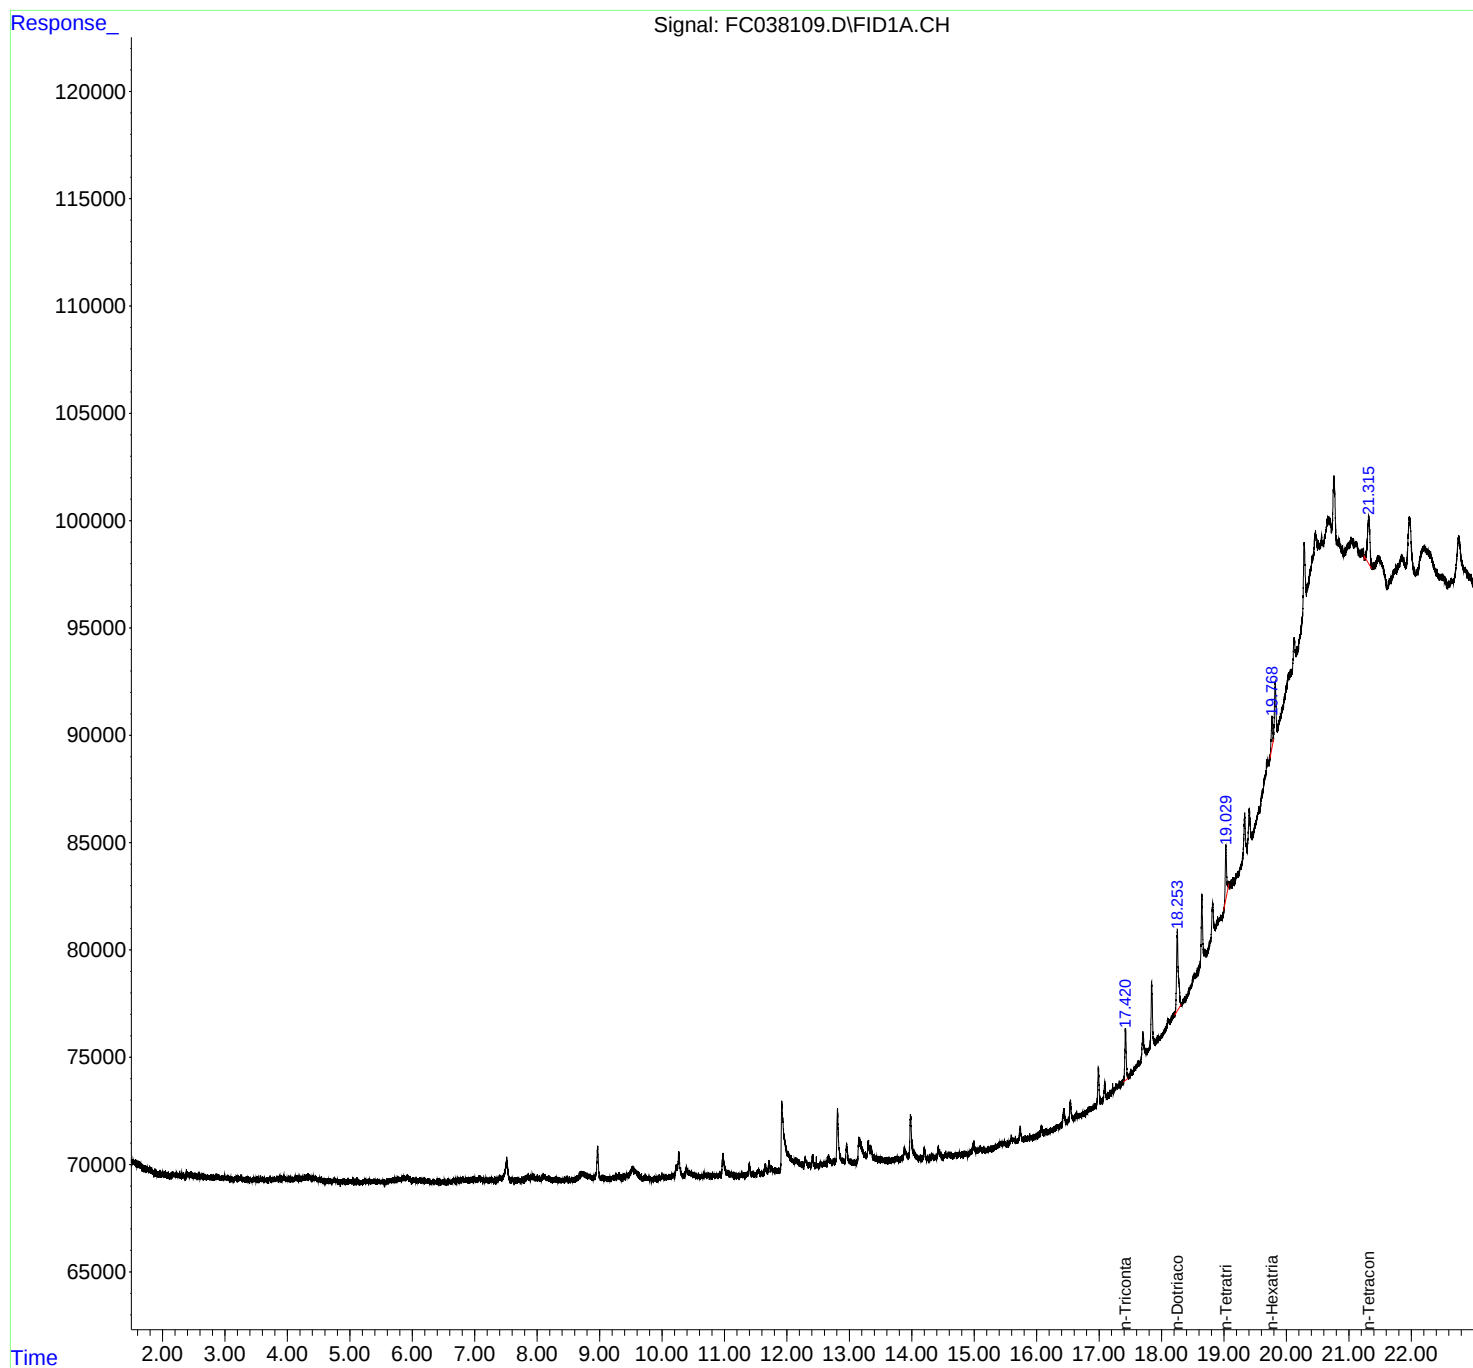


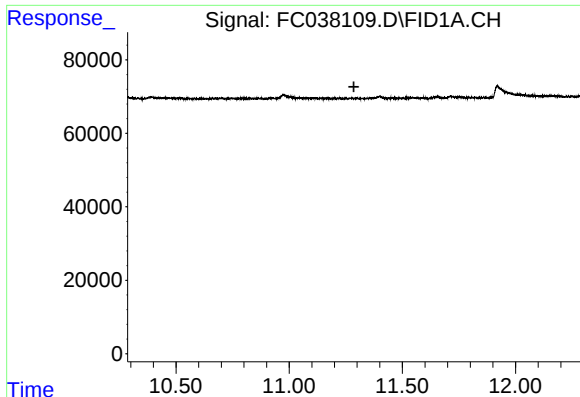

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.286 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

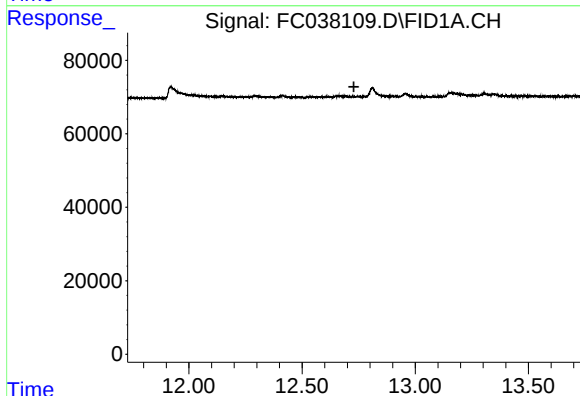


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.729 min
Response: 0
Conc: N.D.

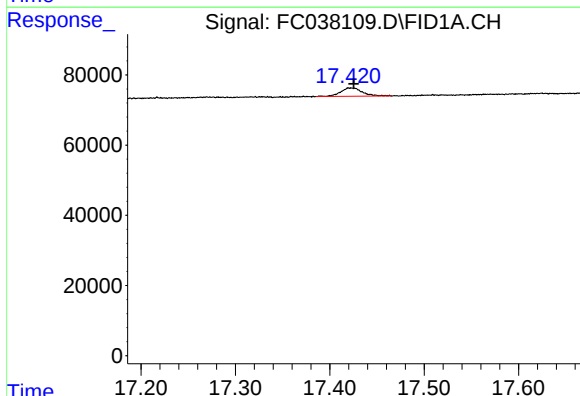


#17 n-Tricontane (C30)

R.T.: 17.423 min
Delta R.T.: -0.003 min
Response: 37868
Conc: 0.35 ug/ml

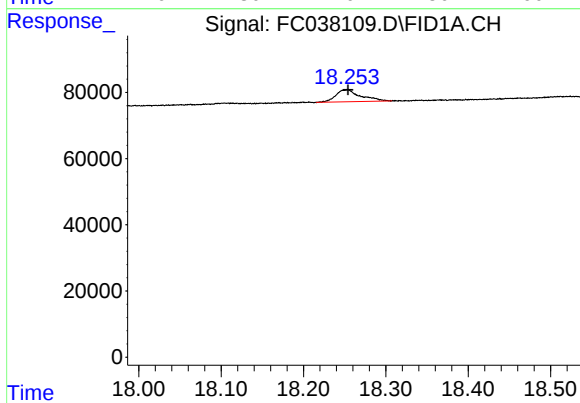

#18 n-Dotriacontane (C32)


R.T.: 18.252 min
Delta R.T.: -0.002 min
Response: 76463
Conc: 0.75 ug/ml

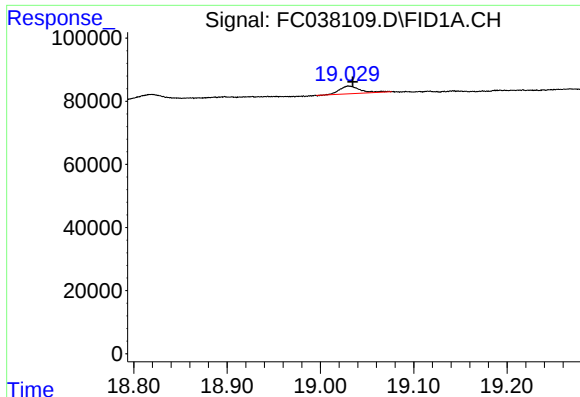

#19 n-Tetratriacontane (C34)


R.T.: 19.031 min
Delta R.T.: -0.004 min
Response: 38000
Conc: 0.43 ug/ml

Instrument :
FID_C
ClientSampleId :

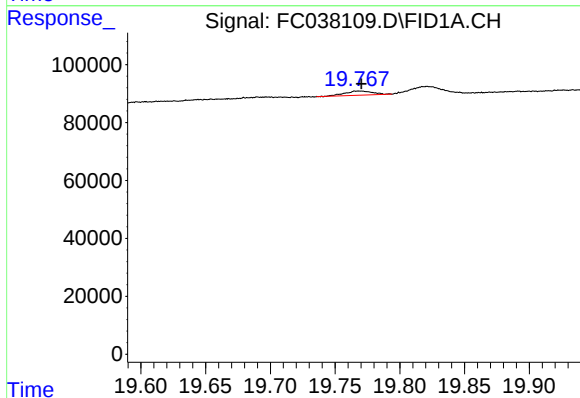

#20 n-Hexatriacontane (C36)

R.T.: 19.769 min
Delta R.T.: -0.001 min
Response: 21595
Conc: 0.28 ug/ml

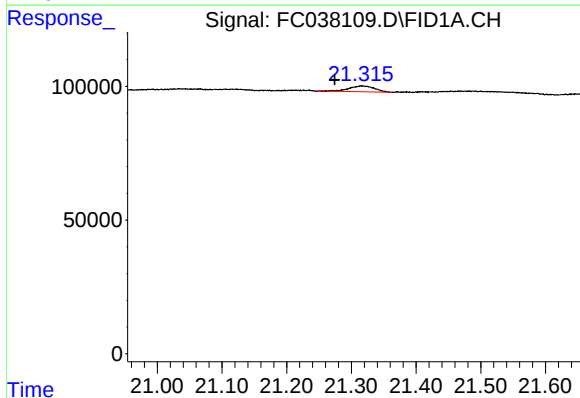

#22 n-Tetracontane (C40)

R.T.: 21.317 min
Delta R.T.: 0.042 min
Response: 59856
Conc: 0.68 ug/ml