

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121018AL\
 Data File : FC038112.D
 Signal(s) : FID1A.CH
 Acq On : 11 Dec 2018 9:07
 Operator : AJ\SJ
 Sample : J6319-16
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 11 09:44:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 121018.M
 Quant Title : GC Extractables
 QLast Update : Mon Dec 10 17:11:09 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.282	5302381	40.673 ug/ml
Spiked Amount 50.000		Recovery =	81.35%
12) S 1-chlorooctadecane (S...	12.724	1610255	15.971 ug/ml
Spiked Amount 50.000		Recovery =	31.94%
Target Compounds			
17) T n-Tricontane (C30)	17.420	32204	0.293 ug/ml
18) T n-Dotriacontane (C32)	18.251	67454	0.659 ug/ml
19) T n-Tetratriacontane (C34)	19.030	28794	0.327 ug/ml
22) T n-Tetracontane (C40)	21.319	82796	0.947 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121018AL\
Data File : FC038112.D
Signal(s) : FID1A.CH
Acq On : 11 Dec 2018 9:07
Operator : AJ\SJ
Sample : J6319-16
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 11 09:44:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 121018.M
Quant Title : GC Extractables
QLast Update : Mon Dec 10 17:11:09 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

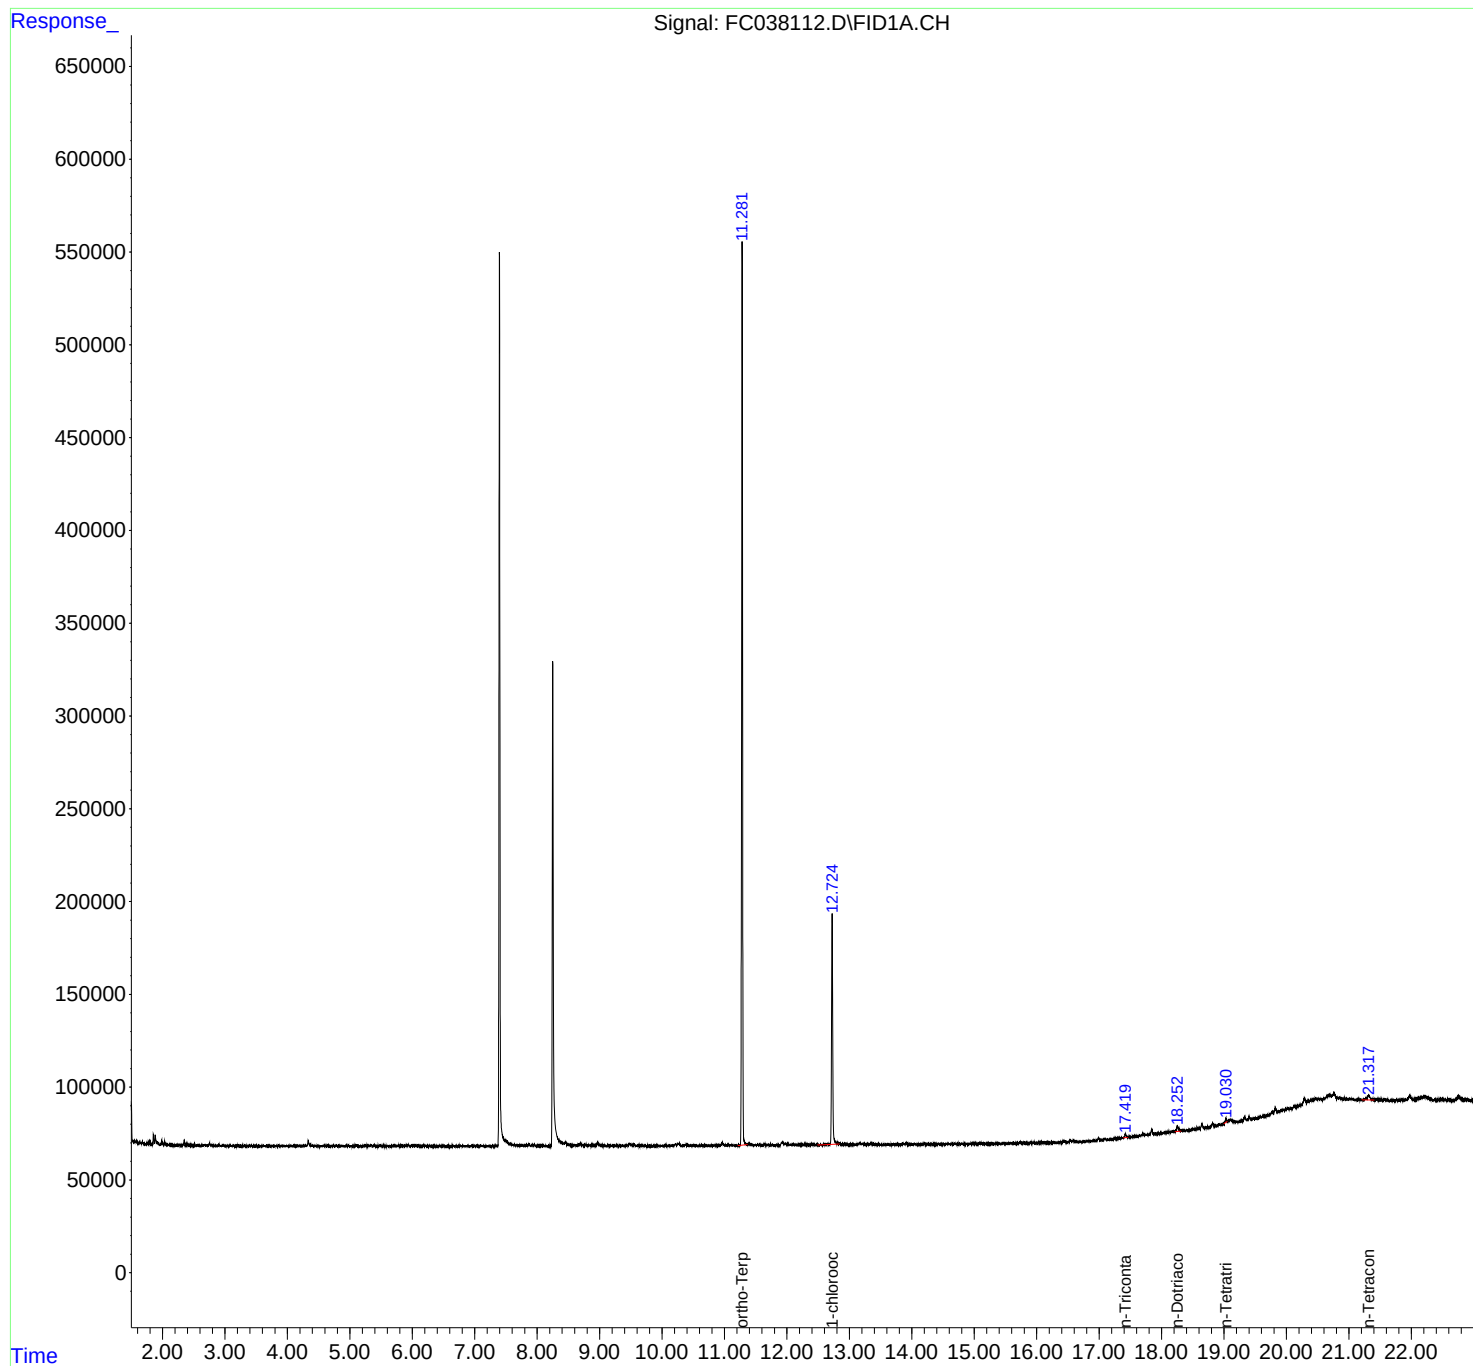


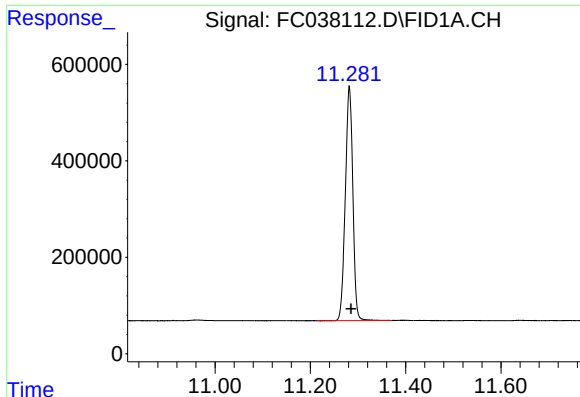

#9 ortho-Terphenyl (SURR)


R.T.: 11.282 min
Delta R.T.: -0.004 min
Response: 5302381
Conc: 40.67 ug/ml

Instrument :
FID_C
ClientSampleId :

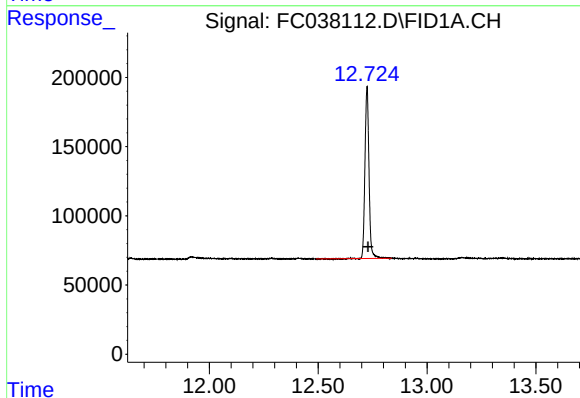


#12 1-chlorooctadecane (SURR)

R.T.: 12.724 min
Delta R.T.: -0.005 min
Response: 1610255
Conc: 15.97 ug/ml

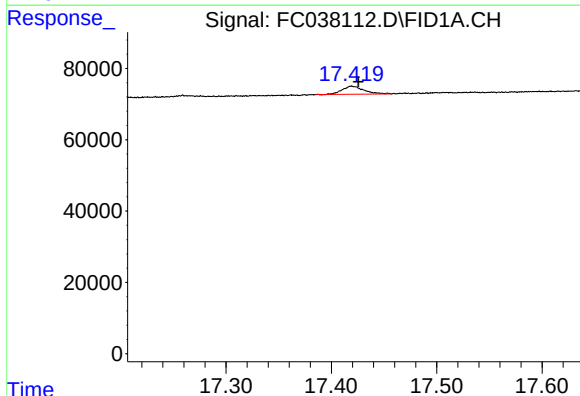


#17 n-Tricontane (C30)

R.T.: 17.420 min
Delta R.T.: -0.006 min
Response: 32204
Conc: 0.29 ug/ml

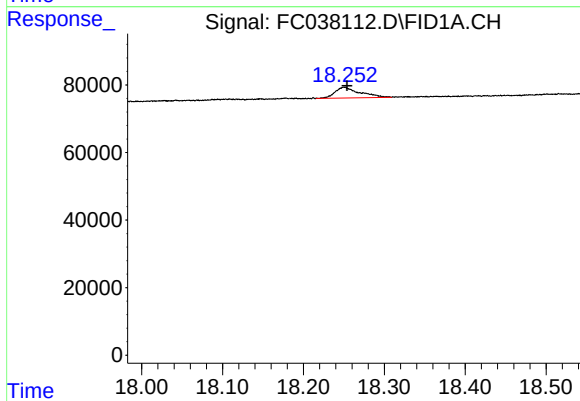

#18 n-Dotriacontane (C32)


R.T.: 18.251 min
Delta R.T.: -0.004 min
Response: 67454
Conc: 0.66 ug/ml

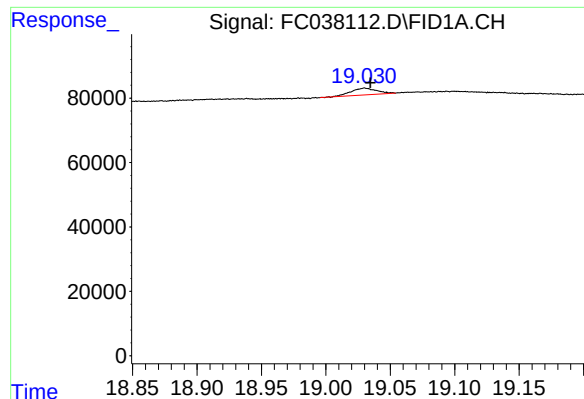

#19 n-Tetratriacontane (C34)

R.T.: 19.030 min
Delta R.T.: -0.004 min
Response: 28794
Conc: 0.33 ug/ml

Instrument :
FID_C
ClientSampleId :

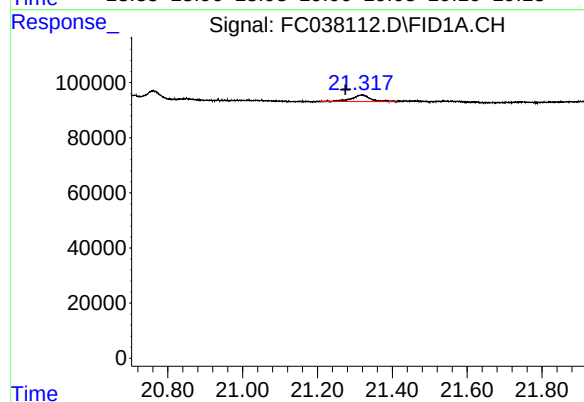

#22 n-Tetracontane (C40)

R.T.: 21.319 min
Delta R.T.: 0.045 min
Response: 82796
Conc: 0.95 ug/ml