

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121218AL\
 Data File : FC038136.D
 Signal(s) : FID1A.CH
 Acq On : 12 Dec 2018 00:17
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 12 05:42:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 121018.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 11 15:29:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
16) T n-Octacosane (C28)	16.572	98033	0.872 ug/ml
17) T n-Tricontane (C30)	17.428	217848	1.985 ug/ml
18) T n-Dotriacontane (C32)	18.252	509131	4.971 ug/ml
19) T n-Tetratriacontane (C34)	19.045	657179	7.457 ug/ml
20) T n-Hexatriacontane (C36)	19.785	617076	7.877 ug/ml
21) T n-Octatriacontane (C38)	20.481	1649370	21.315 ug/ml
22) T n-Tetracontane (C40)	21.306	2491561	28.513 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121218AL\
Data File : FC038136.D
Signal(s) : FID1A.CH
Acq On : 12 Dec 2018 00:17
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampled :

Integration File: autoint1.e
Quant Time: Dec 12 05:42:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 121018.M
Quant Title : GC Extractables
QLast Update : Tue Dec 11 15:29:14 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

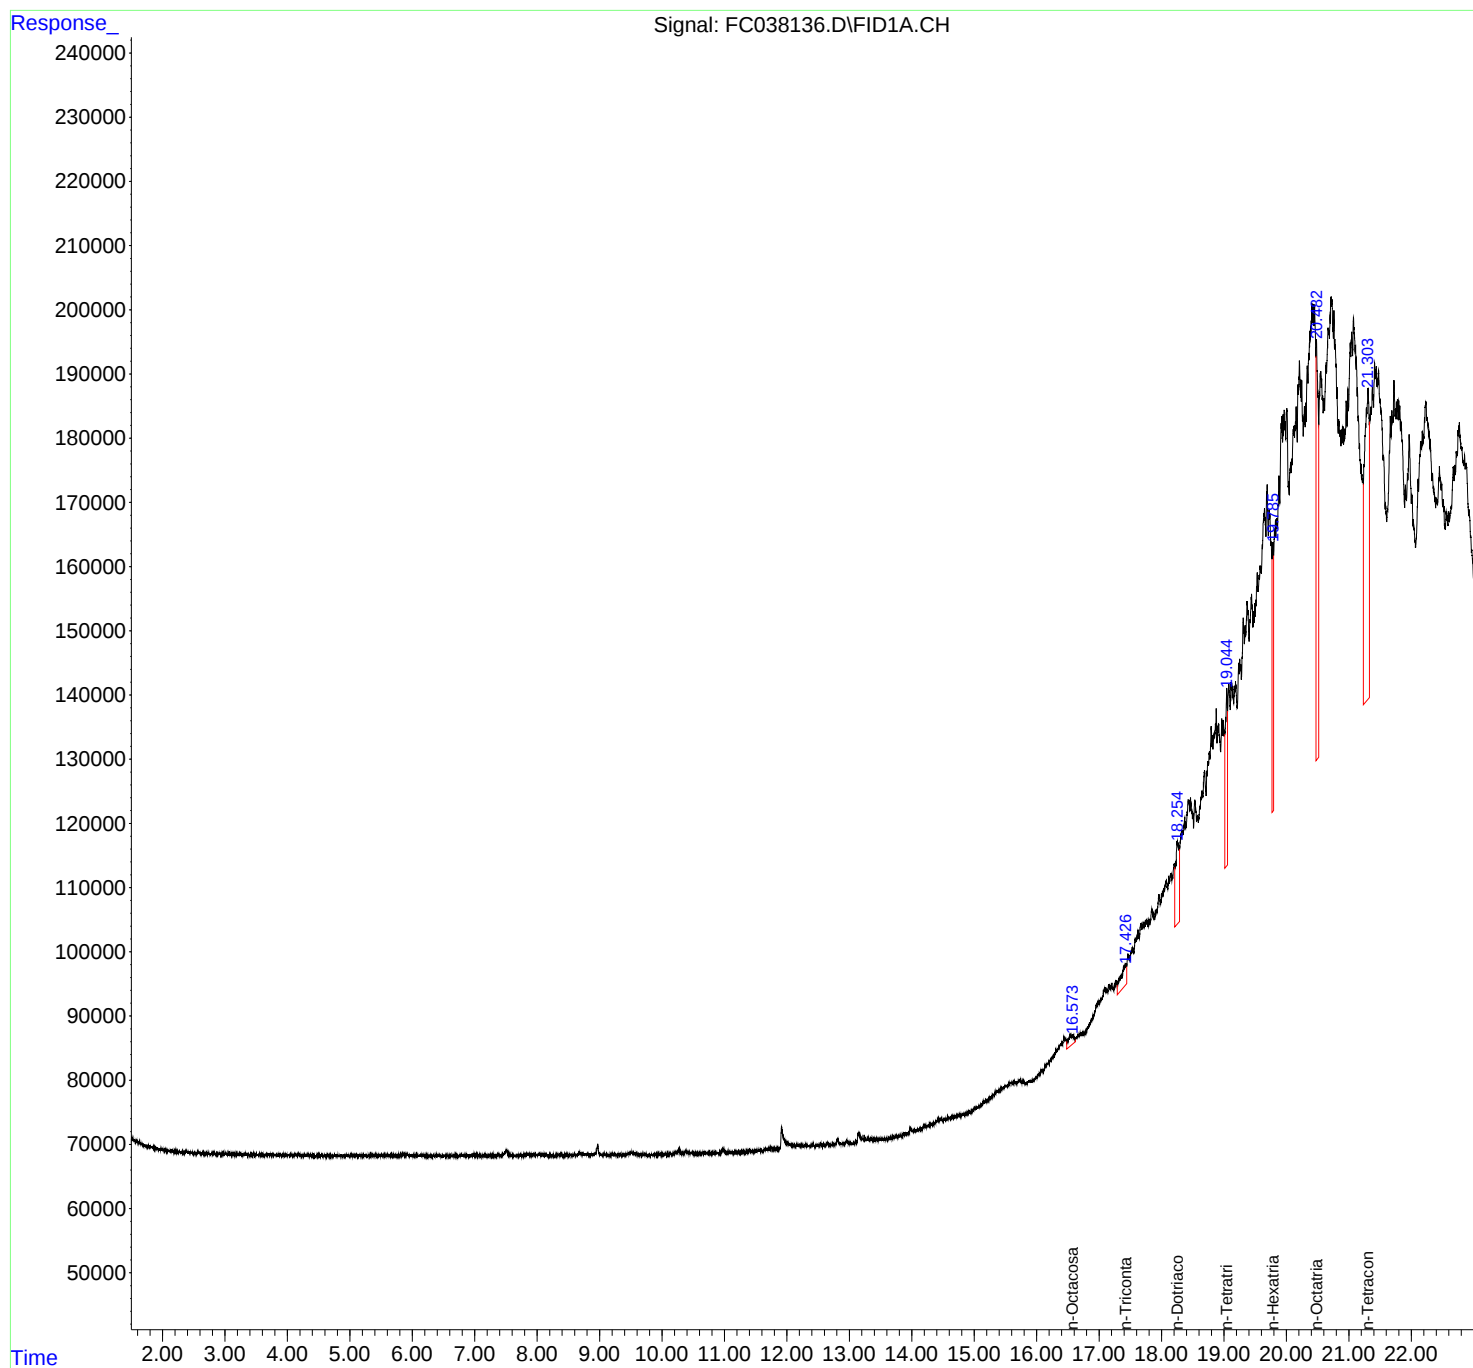


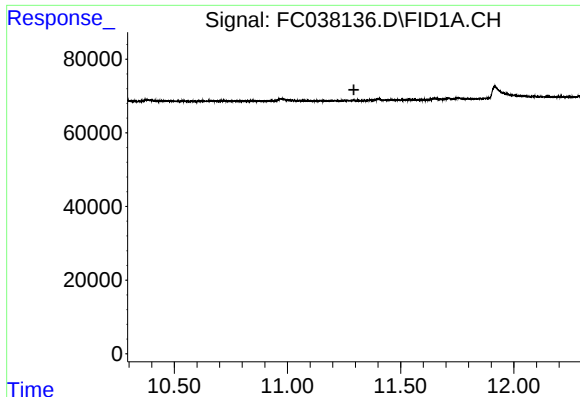

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.294 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

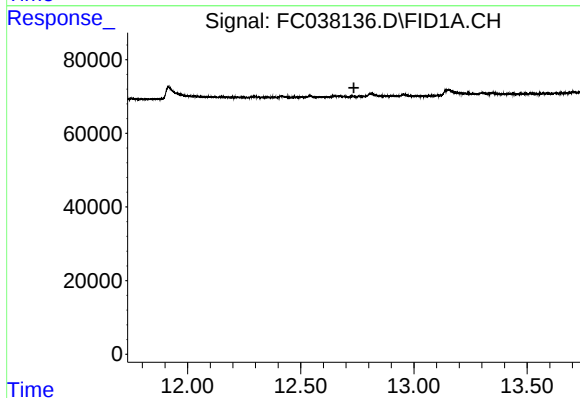


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 12.735 min
Response: 0
Conc: N.D.

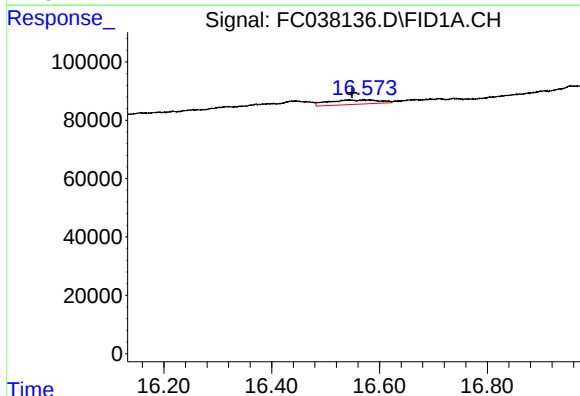


#16 n-Octacosane (C28)

R.T.: 16.572 min
Delta R.T.: 0.023 min
Response: 98033
Conc: 0.87 ug/ml

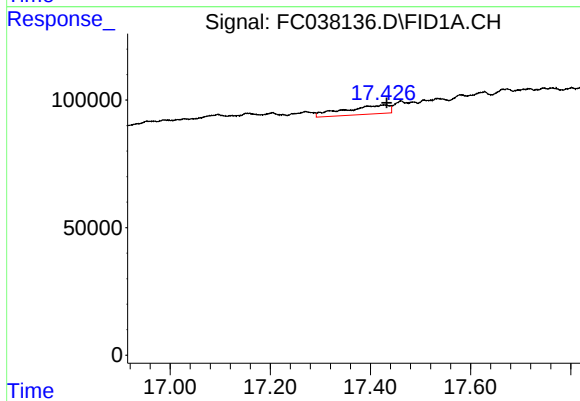

#17 n-Tricontane (C30)


R.T.: 17.428 min
Delta R.T.: -0.005 min
Response: 217848
Conc: 1.98 ug/ml

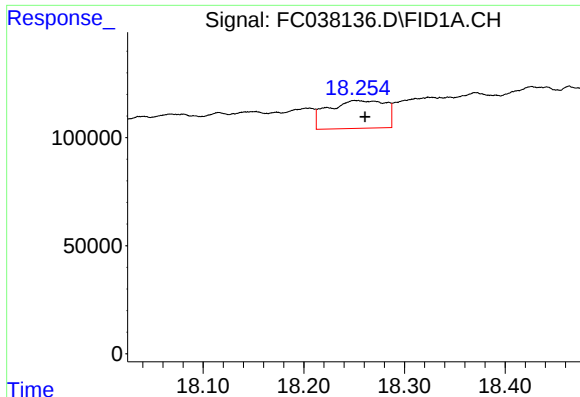

#18 n-Dotriacontane (C32)


R.T.: 18.252 min
Delta R.T.: -0.009 min
Response: 509131
Conc: 4.97 ug/ml

Instrument :
FID_C
ClientSampleId :

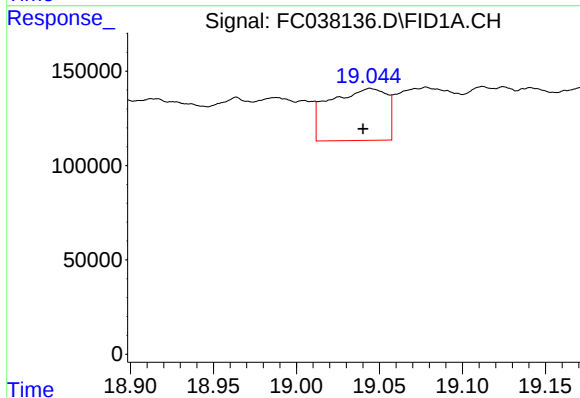


#19 n-Tetratriacontane (C34)

R.T.: 19.045 min
Delta R.T.: 0.005 min
Response: 657179
Conc: 7.46 ug/ml

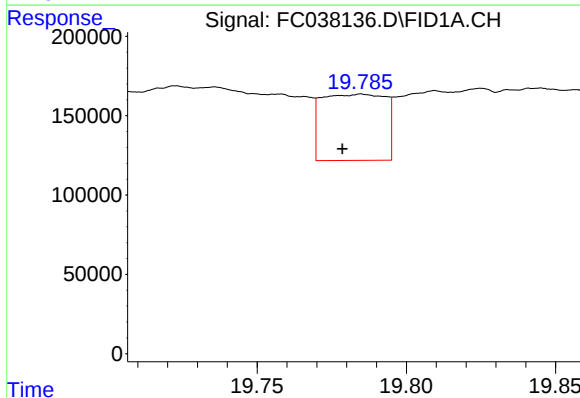


#20 n-Hexatriacontane (C36)

R.T.: 19.785 min
Delta R.T.: 0.006 min
Response: 617076
Conc: 7.88 ug/ml

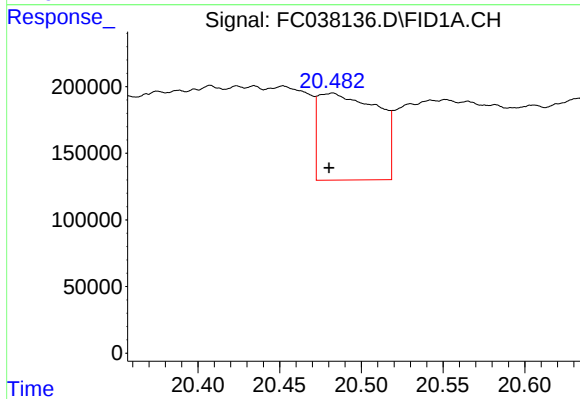

#21 n-Octatriacontane (C38)

R.T.: 20.481 min
Delta R.T.: 0.001 min
Response: 1649370
Conc: 21.31 ug/ml

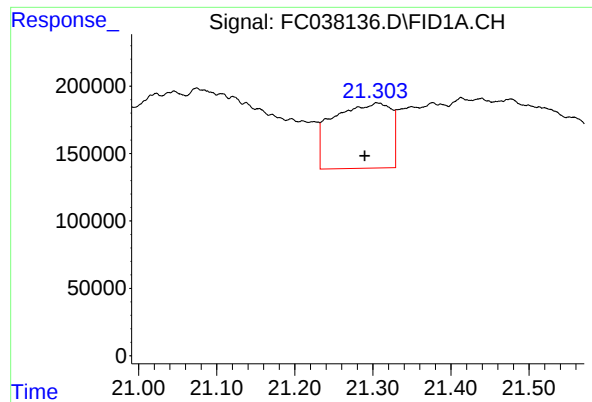

#22 n-Tetracontane (C40)

R.T.: 21.306 min
Delta R.T.: 0.017 min
Response: 2491561
Conc: 28.51 ug/ml

Instrument :
FID_C
ClientSampleId :