

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC121322AL\  
 Data File : FC062411.D  
 Signal(s) : FID1A.ch  
 Acq On : 13 Dec 2022 10:20  
 Operator : YP/AJ  
 Sample : N5994-01  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 FID\_C  
 ClientSampleId :  
 AOC6-B1

Integration File: autoint1.e  
 Quant Time: Dec 13 16:38:33 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 120722.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Dec 08 01:05:24 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.569 | 4012153    | 28.443 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 56.89%       |
| 12) S 1-chlorooctadecane (S... | 13.009 | 2596132    | 24.358 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 48.72%       |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC121322AL\  
Data File : FC062411.D  
Signal(s) : FID1A.ch  
Acq On : 13 Dec 2022 10:20  
Operator : YP/AJ  
Sample : N5994-01  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_C  
ClientSampleId :  
AOC6-B1

Integration File: autoint1.e  
Quant Time: Dec 13 16:38:33 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 120722.M  
Quant Title : GC Extractables  
QLast Update : Thu Dec 08 01:05:24 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

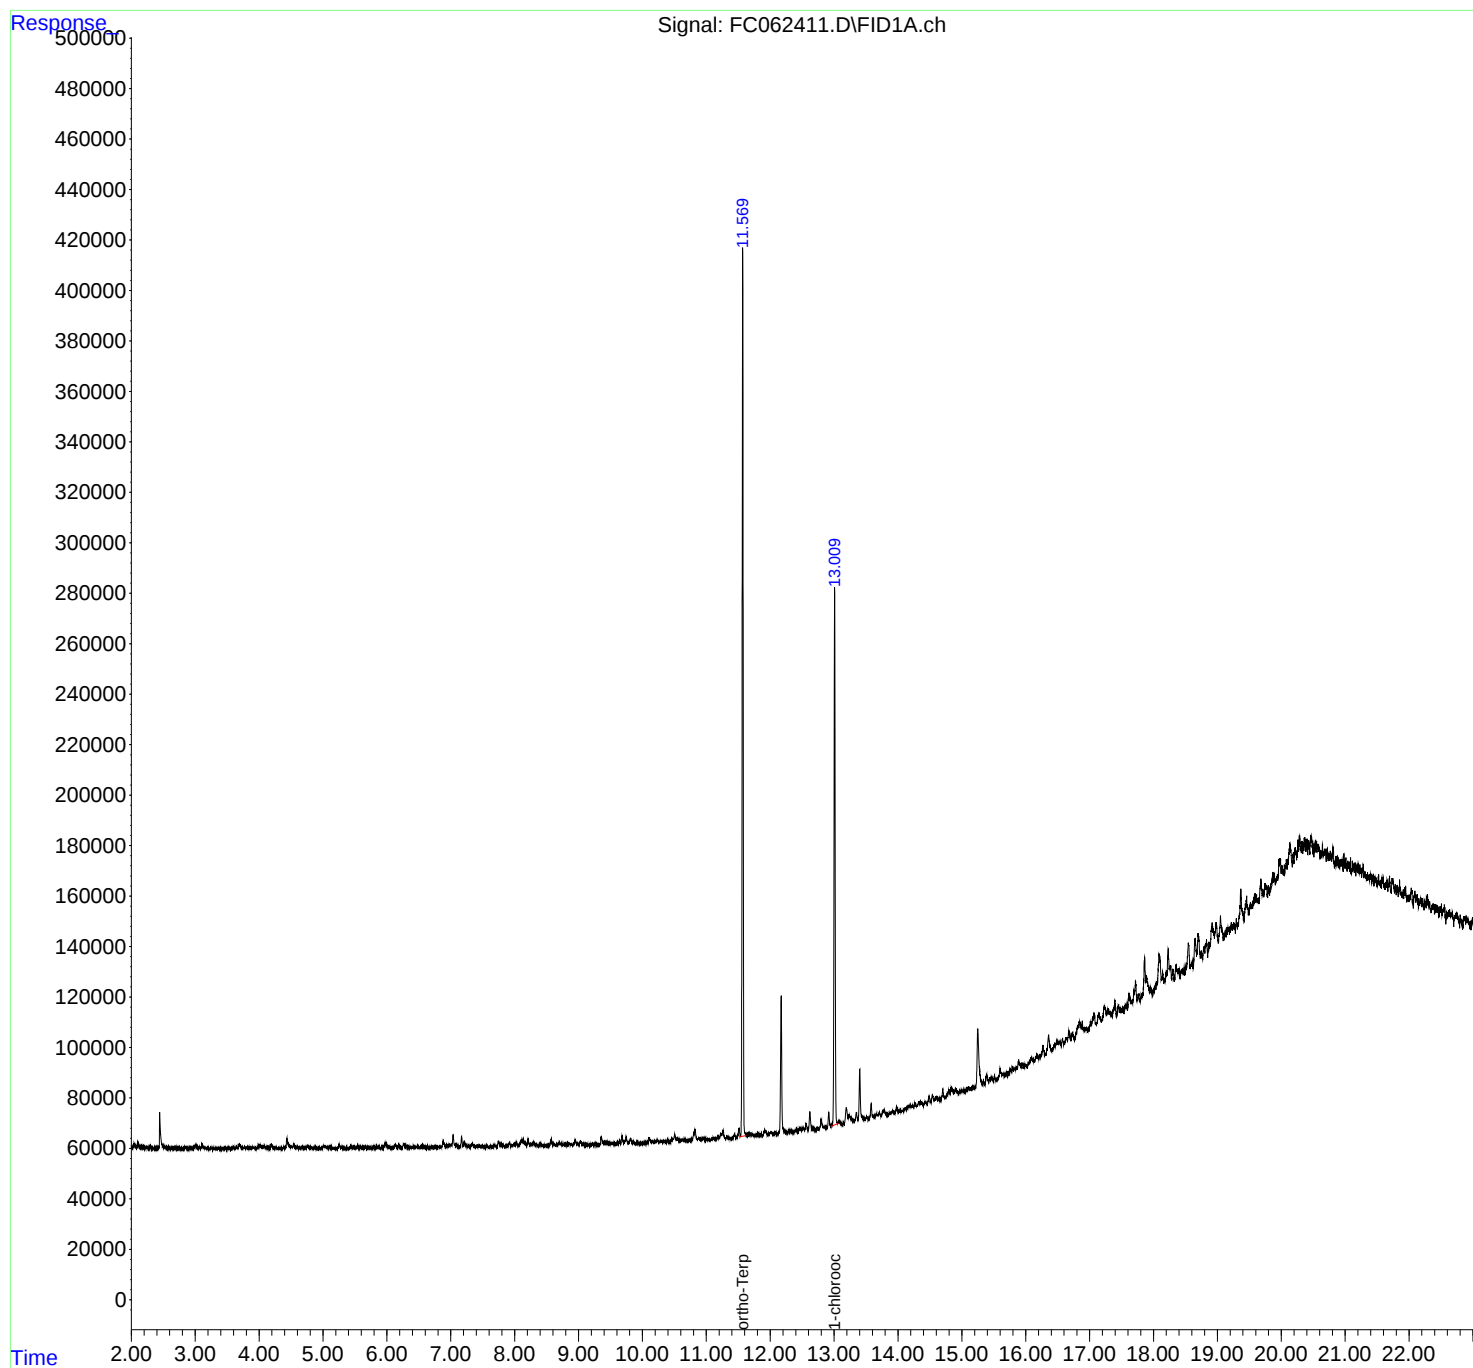


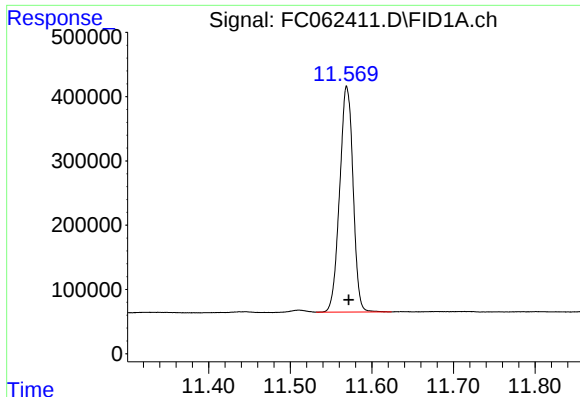

#9 ortho-Terphenyl (SURR)

R.T.: 11.569 min  
Delta R.T.: -0.002 min  
Response: 4012153  
Conc: 28.44 ug/ml

Instrument :  
FID\_C  
ClientSampleId :  
AOC6-B1

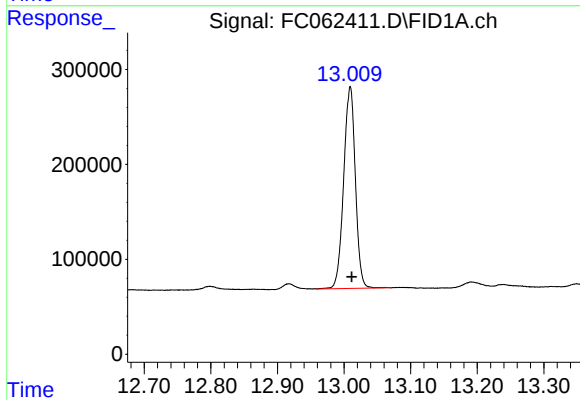

#12 1-chlorooctadecane (SURR)

R.T.: 13.009 min  
Delta R.T.: -0.002 min  
Response: 2596132  
Conc: 24.36 ug/ml