

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121521AL\
 Data File : FC057509.D
 Signal(s) : FID1A.CH
 Acq On : 16 Dec 2021 1:15
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 16 05:40:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 20:43:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

17) T	n-Tricontane (C30)	16.979	76289	0.558 ug/ml
18) T	n-Dotriacontane (C32)	17.845	68580	0.511 ug/ml
19) T	n-Tetratriacontane (C34)	18.595f	139410	1.069 ug/ml
20) T	n-Hexatriacontane (C36)	19.400	180534	1.520 ug/ml
21) T	n-Octatriacontane (C38)	20.063	36771	0.335 ug/ml
22) T	n-Tetracontane (C40)	21.031	281558	2.820 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121521AL\
Data File : FC057509.D
Signal(s) : FID1A.CH
Acq On : 16 Dec 2021 1:15
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 05:40:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 20:43:13 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

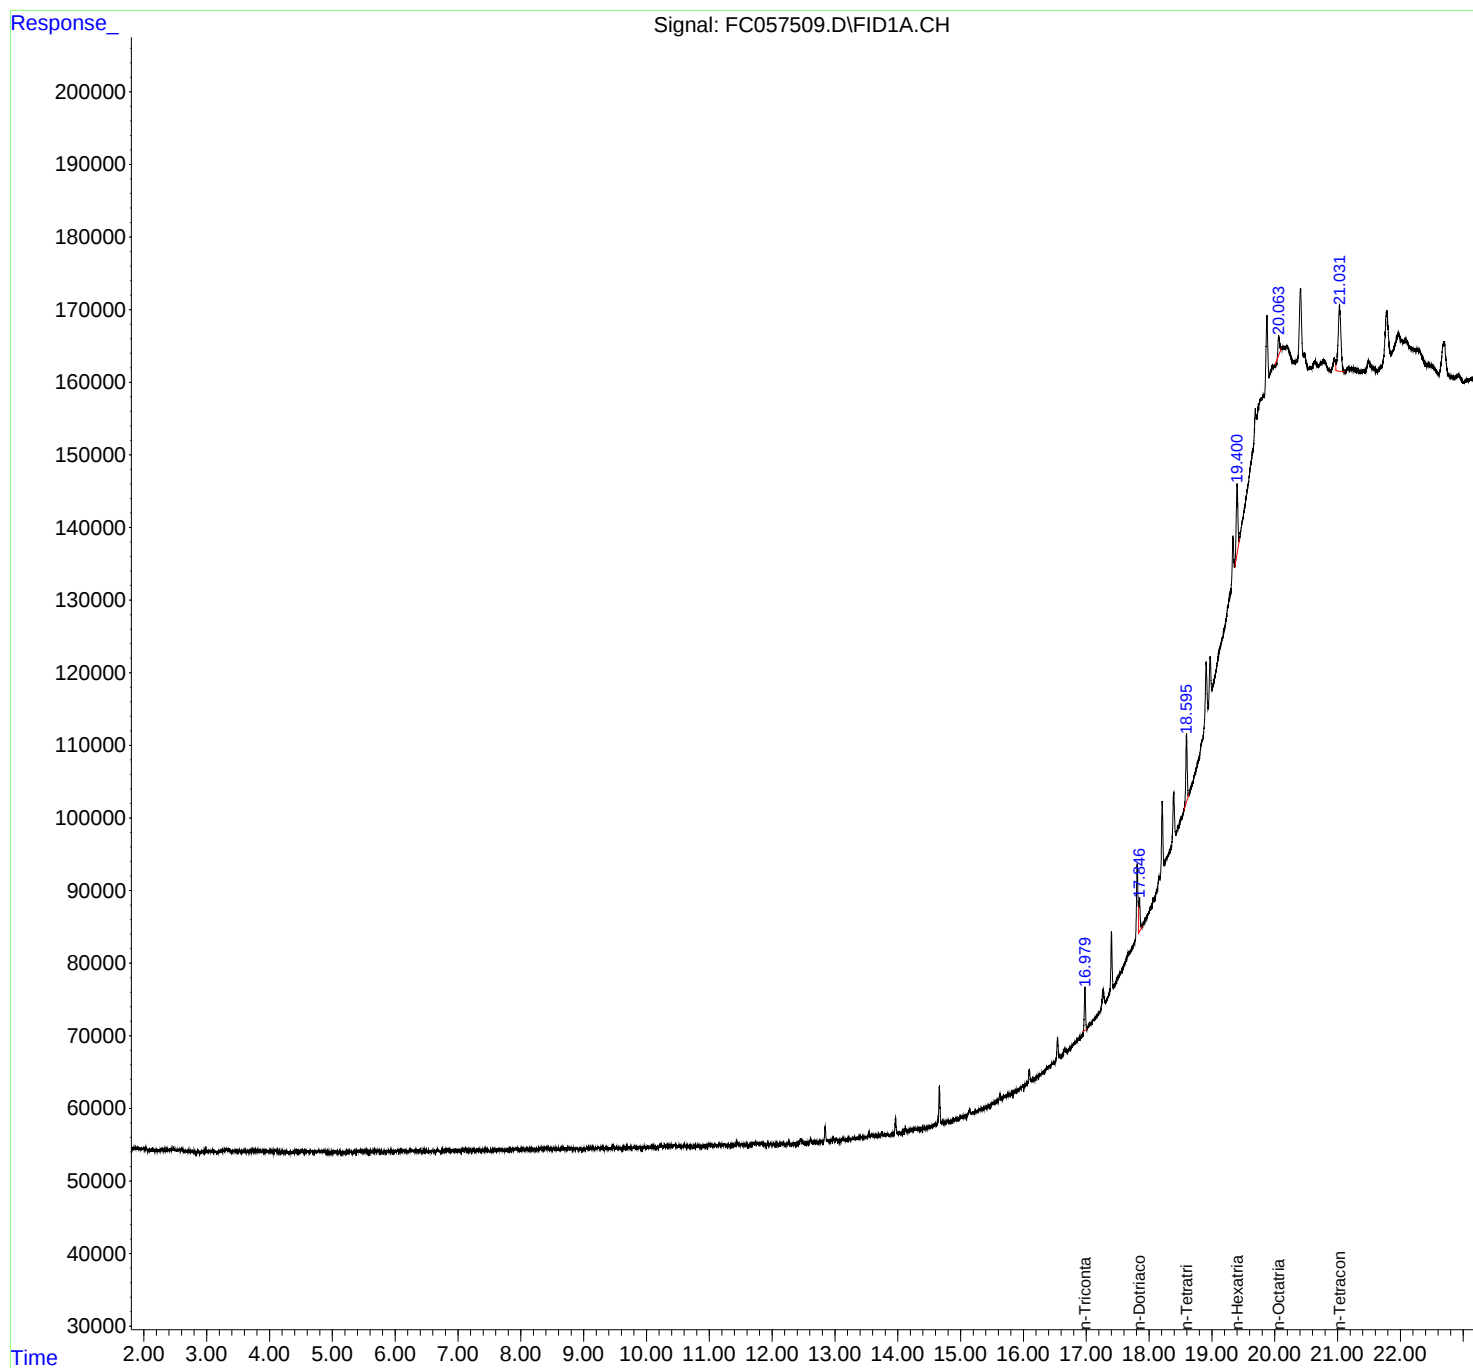


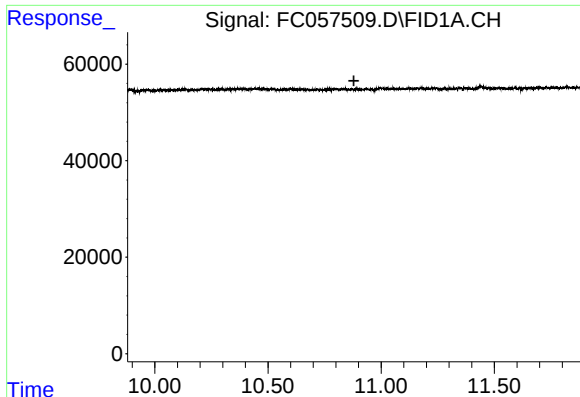

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.880 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

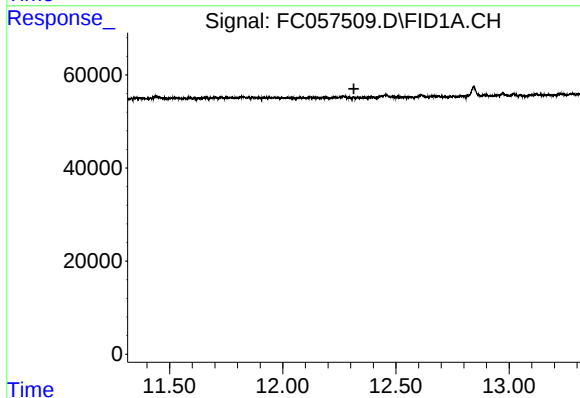


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.314 min
Response: 0
Conc: N.D.

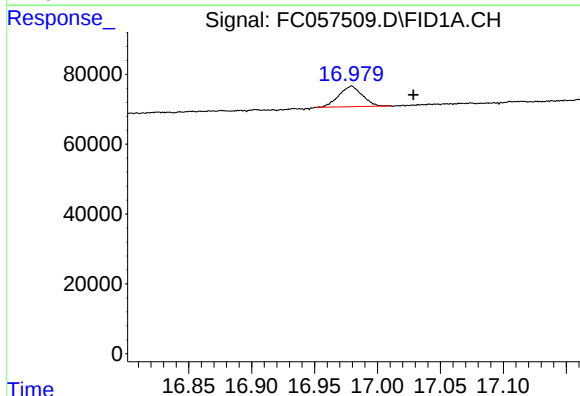


#17 n-Tricontane (C30)

R.T.: 16.979 min
Delta R.T.: -0.050 min
Response: 76289
Conc: 0.56 ug/ml

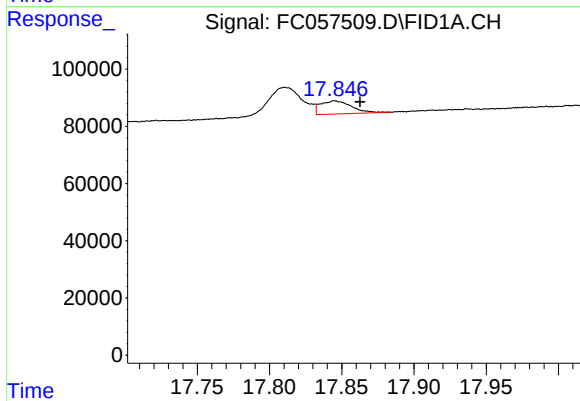

#18 n-Dotriacontane (C32)


R.T.: 17.845 min
Delta R.T.: -0.017 min
Response: 68580
Conc: 0.51 ug/ml

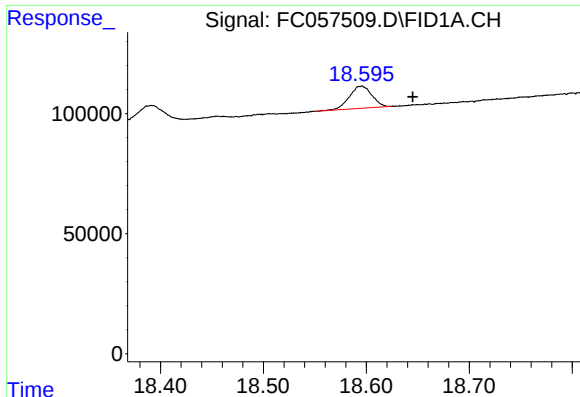

#19 n-Tetratriacontane (C34)


R.T.: 18.595 min
Delta R.T.: -0.050 min
Response: 139410
Conc: 1.07 ug/ml

Instrument :
FID_C
ClientSampleId :

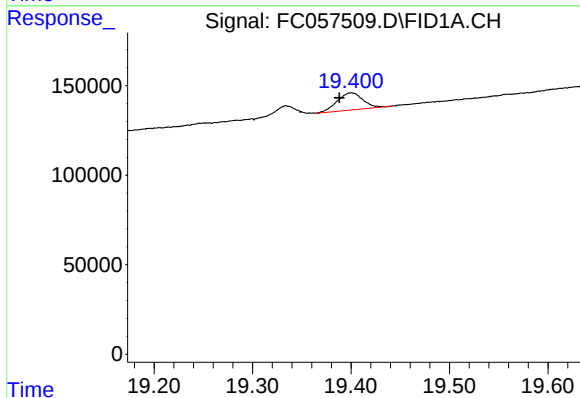


#20 n-Hexatriacontane (C36)

R.T.: 19.400 min
Delta R.T.: 0.012 min
Response: 180534
Conc: 1.52 ug/ml

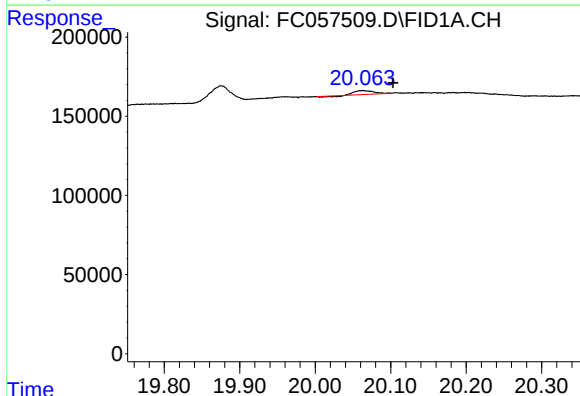

#21 n-Octatriacontane (C38)

R.T.: 20.063 min
Delta R.T.: -0.040 min
Response: 36771
Conc: 0.33 ug/ml

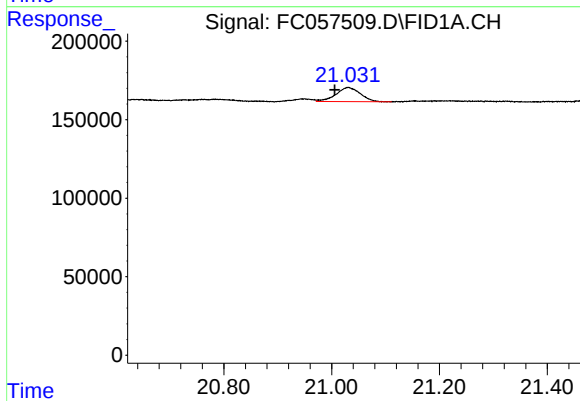

#22 n-Tetracontane (C40)

R.T.: 21.031 min
Delta R.T.: 0.024 min
Response: 281558
Conc: 2.82 ug/ml