

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121522AL\
 Data File : FC062447.D
 Signal(s) : FID1A.ch
 Acq On : 15 Dec 2022 17:39
 Operator : YP/AJ
 Sample : N6065-01D
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 16 03:09:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 120722.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 08 01:05:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.574	5644367	40.013 ug/ml
Spiked Amount 50.000		Recovery =	80.03%
12) S 1-chlorooctadecane (S...	13.013	4491197	42.138 ug/ml
Spiked Amount 50.000		Recovery =	84.28%
Target Compounds			
17) T n-Tricontane (C30)	17.720	71179	0.637 ug/ml
18) T n-Dotriacontane (C32)	18.553	90297	0.813 ug/ml
19) T n-Tetratriacontane (C34)	19.335	49766	0.460 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121522AL\
Data File : FC062447.D
Signal(s) : FID1A.ch
Acq On : 15 Dec 2022 17:39
Operator : YP/AJ
Sample : N6065-01D
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 03:09:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 120722.M
Quant Title : GC Extractables
QLast Update : Thu Dec 08 01:05:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

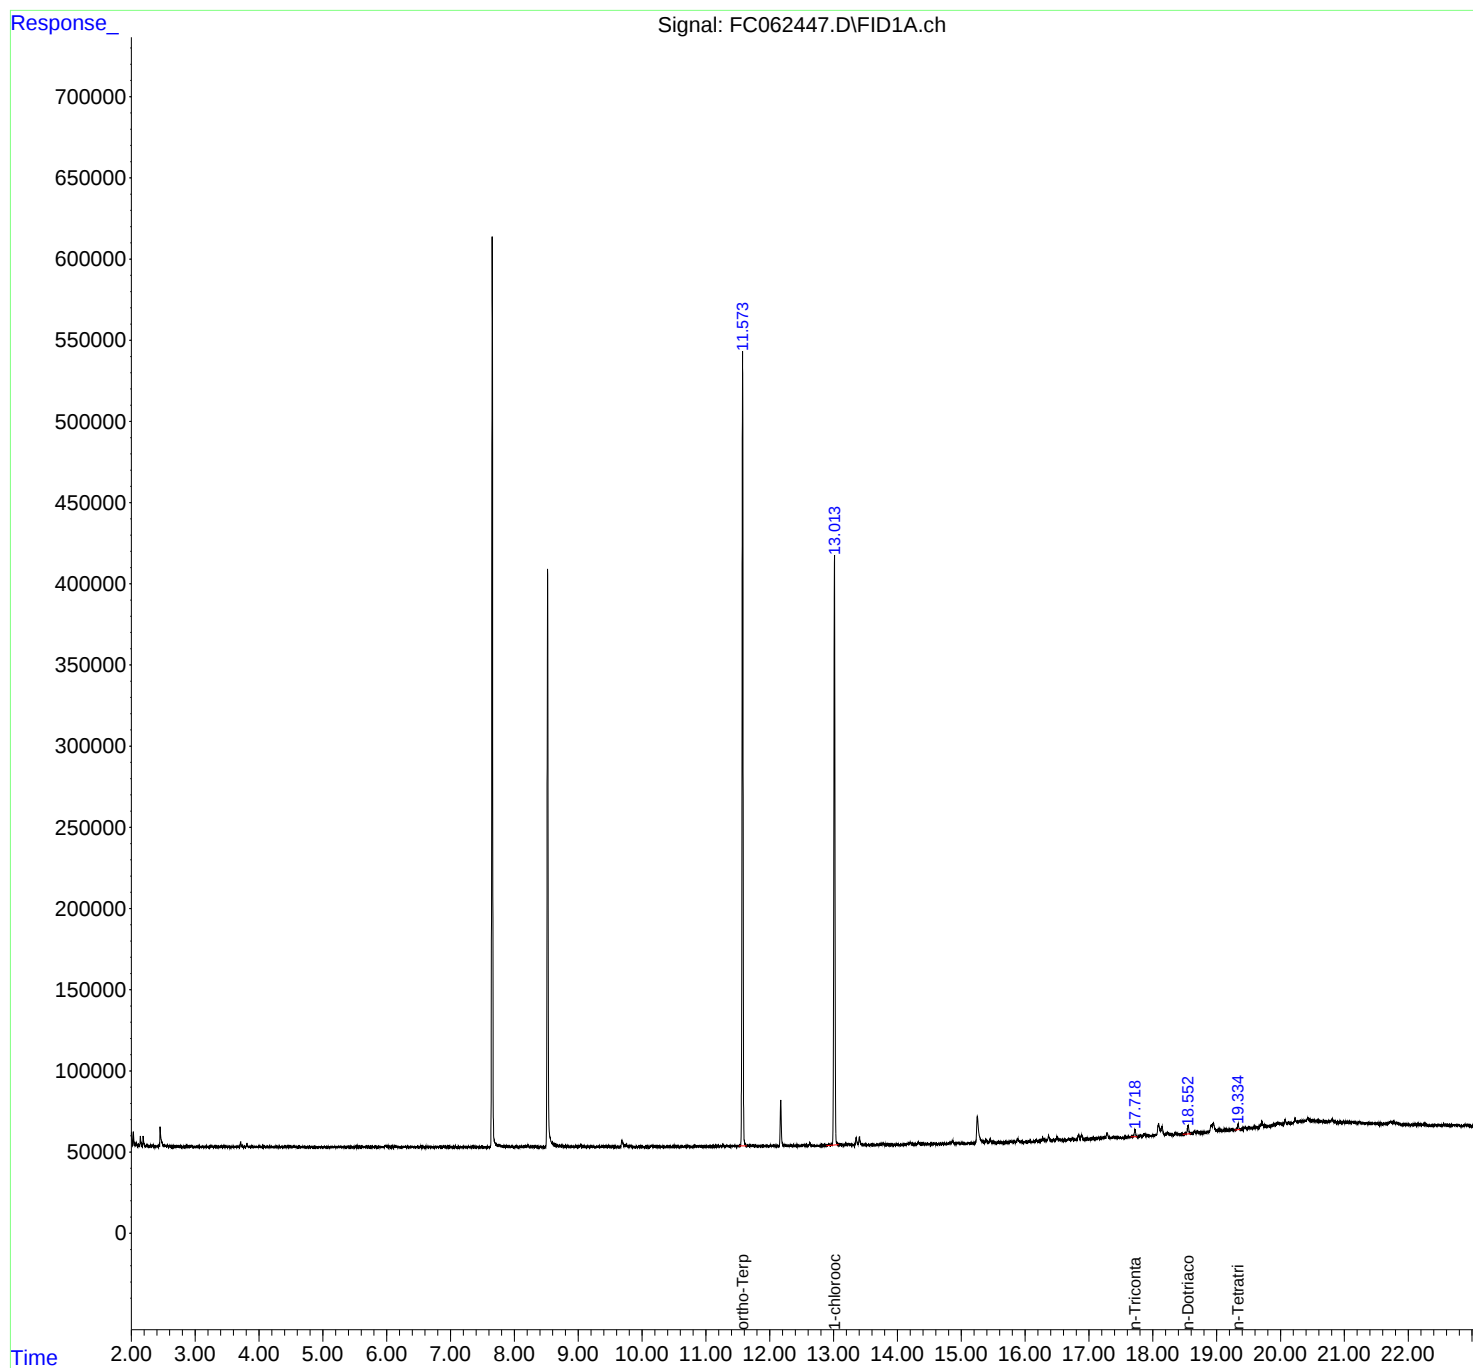


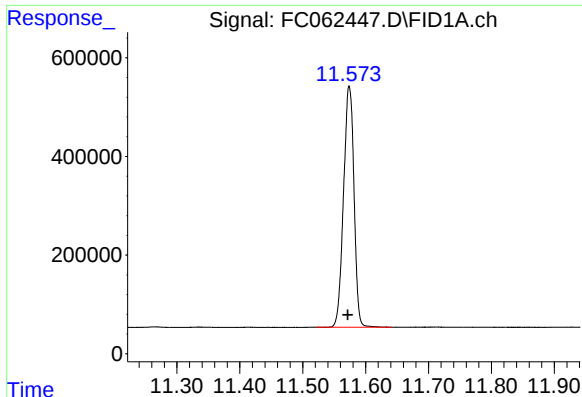

#9 ortho-Terphenyl (SURR)


R.T.: 11.574 min
Delta R.T.: 0.003 min
Response: 5644367
Conc: 40.01 ug/ml

Instrument :
FID_C
ClientSampleId :

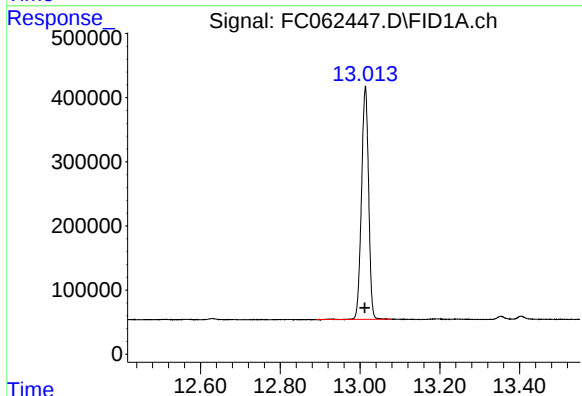


#12 1-chlorooctadecane (SURR)

R.T.: 13.013 min
Delta R.T.: 0.002 min
Response: 4491197
Conc: 42.14 ug/ml

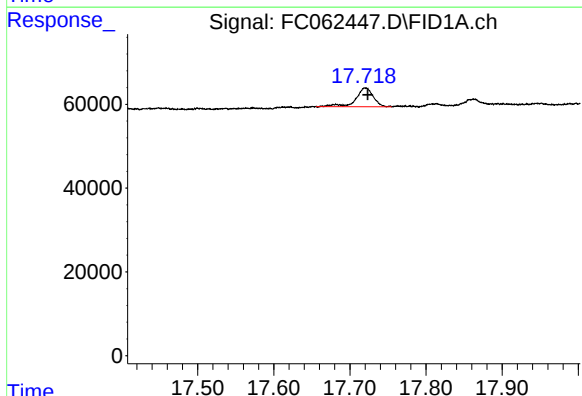


#17 n-Tricontane (C30)

R.T.: 17.720 min
Delta R.T.: -0.003 min
Response: 71179
Conc: 0.64 ug/ml

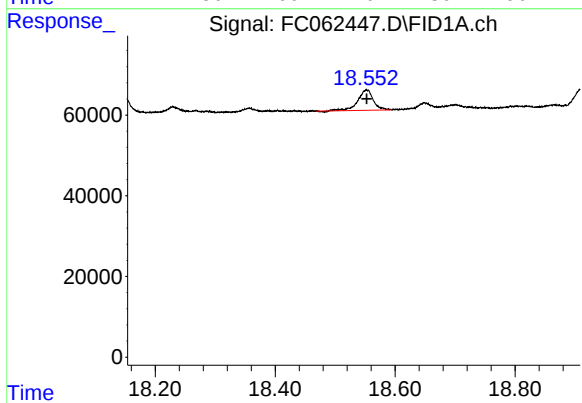

#18 n-Dotriacontane (C32)

R.T.: 18.553 min
Delta R.T.: 0.000 min
Response: 90297
Conc: 0.81 ug/ml

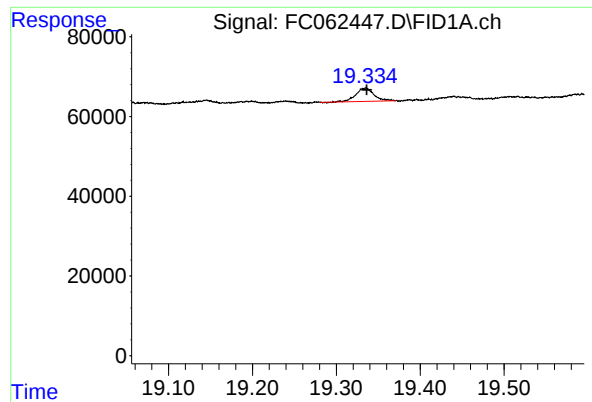

#19 n-Tetratriacontane (C34)

R.T.: 19.335 min
Delta R.T.: 0.000 min
Response: 49766
Conc: 0.46 ug/ml

Instrument :

FID_C

ClientSampleId :