

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121523AL\
 Data File : FC065484.D
 Signal(s) : FID1A.ch
 Acq On : 15 Dec 2023 18:45
 Operator : YP/AJ
 Sample : 05791-11DL 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 15 22:33:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 112423.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 24 13:28:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.933	1780482	10.753 ug/ml
Spiked Amount 50.000		Recovery =	21.51%
Target Compounds			
17) T n-Tricontane (C30)	17.624	26305	0.165 ug/ml
18) T n-Dotriacontane (C32)	18.443	136063	0.866 ug/ml
19) T n-Tetratriacontane (C34)	19.248	55909	0.362 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121523AL\
Data File : FC065484.D
Signal(s) : FID1A.ch
Acq On : 15 Dec 2023 18:45
Operator : YP/AJ
Sample : 05791-11DL 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 15 22:33:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 112423.M
Quant Title : GC Extractables
QLast Update : Fri Nov 24 13:28:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

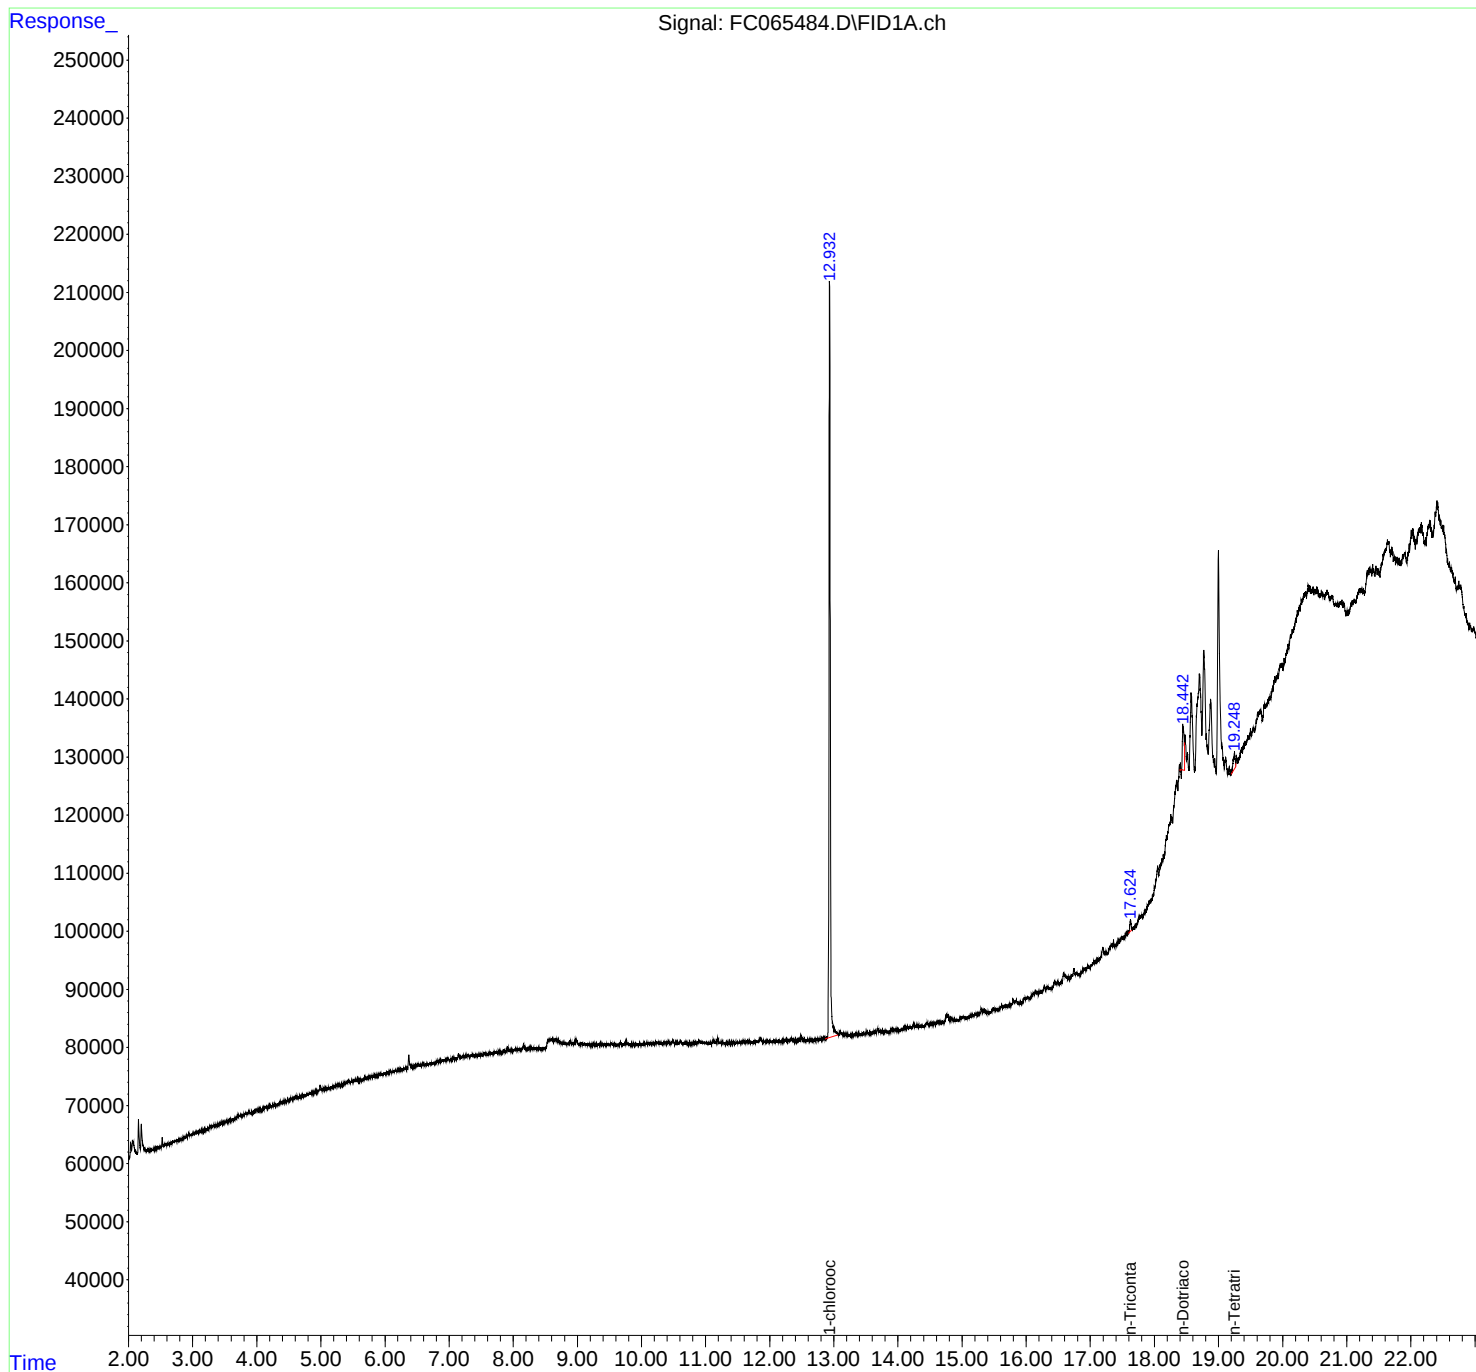


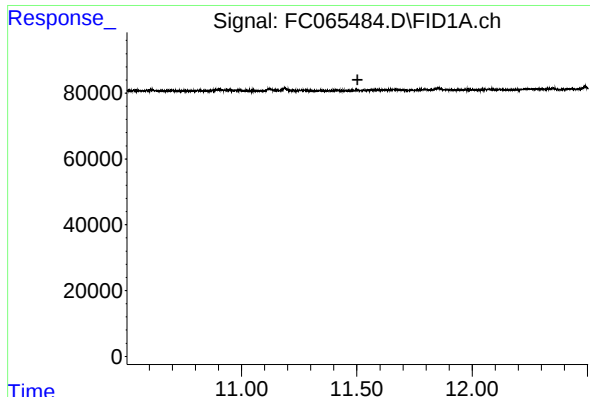

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.503 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

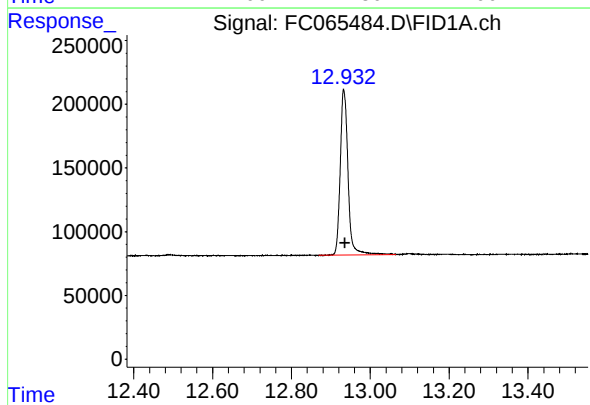


#12 1-chlorooctadecane (SURR)

R.T.: 12.933 min
Delta R.T.: -0.003 min
Response: 1780482
Conc: 10.75 ug/ml

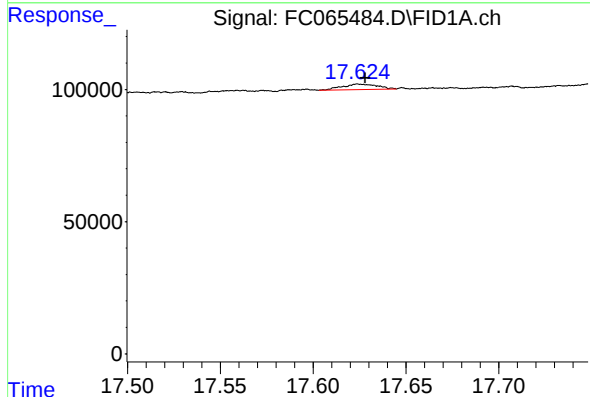


#17 n-Tricontane (C30)

R.T.: 17.624 min
Delta R.T.: -0.004 min
Response: 26305
Conc: 0.17 ug/ml

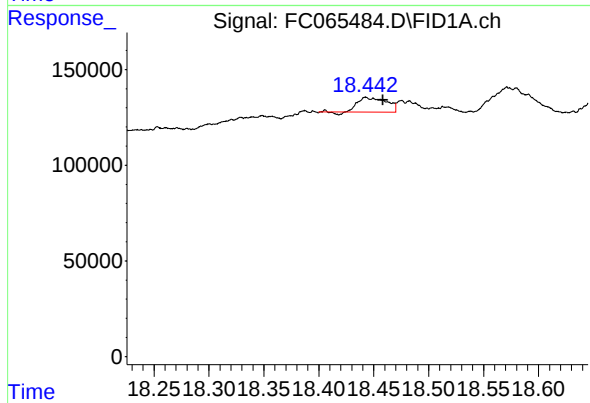

#18 n-Dotriacontane (C32)

R.T.: 18.443 min
Delta R.T.: -0.016 min
Response: 136063
Conc: 0.87 ug/ml

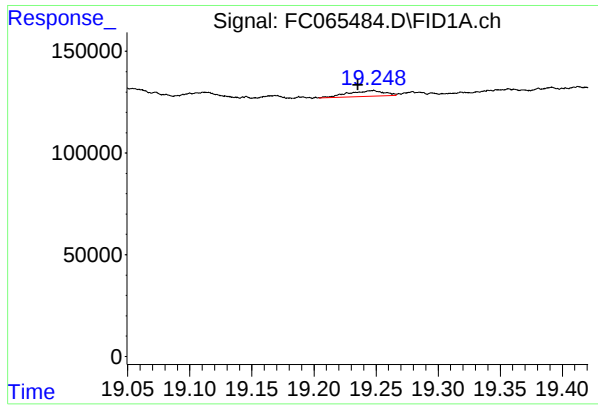

#19 n-Tetratriacontane (C34)

R.T.: 19.248 min
Delta R.T.: 0.012 min
Response: 55909
Conc: 0.36 ug/ml

Instrument :

FID_C

ClientSampleId :