

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121523AL\
 Data File : FC065486.D
 Signal(s) : FID1A.ch
 Acq On : 15 Dec 2023 20:03
 Operator : YP/AJ
 Sample : 05791-10DL2 250X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 15 22:33:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 112423.M
 Quant Title : GC Extractables
 QLast Update : Fri Nov 24 13:28:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) T n-Tetracosane (C24)	14.784	88264	0.509 ug/ml
15) T n-Hexacosane (C26)	15.836	797245	4.788 ug/ml
16) T n-Octacosane (C28)	16.739	539350	3.372 ug/ml
17) T n-Tricontane (C30)	17.628	164517	1.033 ug/ml
18) T n-Dotriacontane (C32)	18.439	276222	1.757 ug/ml
19) T n-Tetratriacontane (C34)	19.218	100773	0.653 ug/ml
20) T n-Hexatriacontane (C36)	19.979	241718	1.577 ug/ml
21) T n-Octatriacontane (C38)	20.623f	90338	0.594 ug/ml
22) T n-Tetracontane (C40)	21.568	408590	2.726 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121523AL\
Data File : FC065486.D
Signal(s) : FID1A.ch
Acq On : 15 Dec 2023 20:03
Operator : YP/AJ
Sample : 05791-10DL2 250X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 15 22:33:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 112423.M
Quant Title : GC Extractables
QLast Update : Fri Nov 24 13:28:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

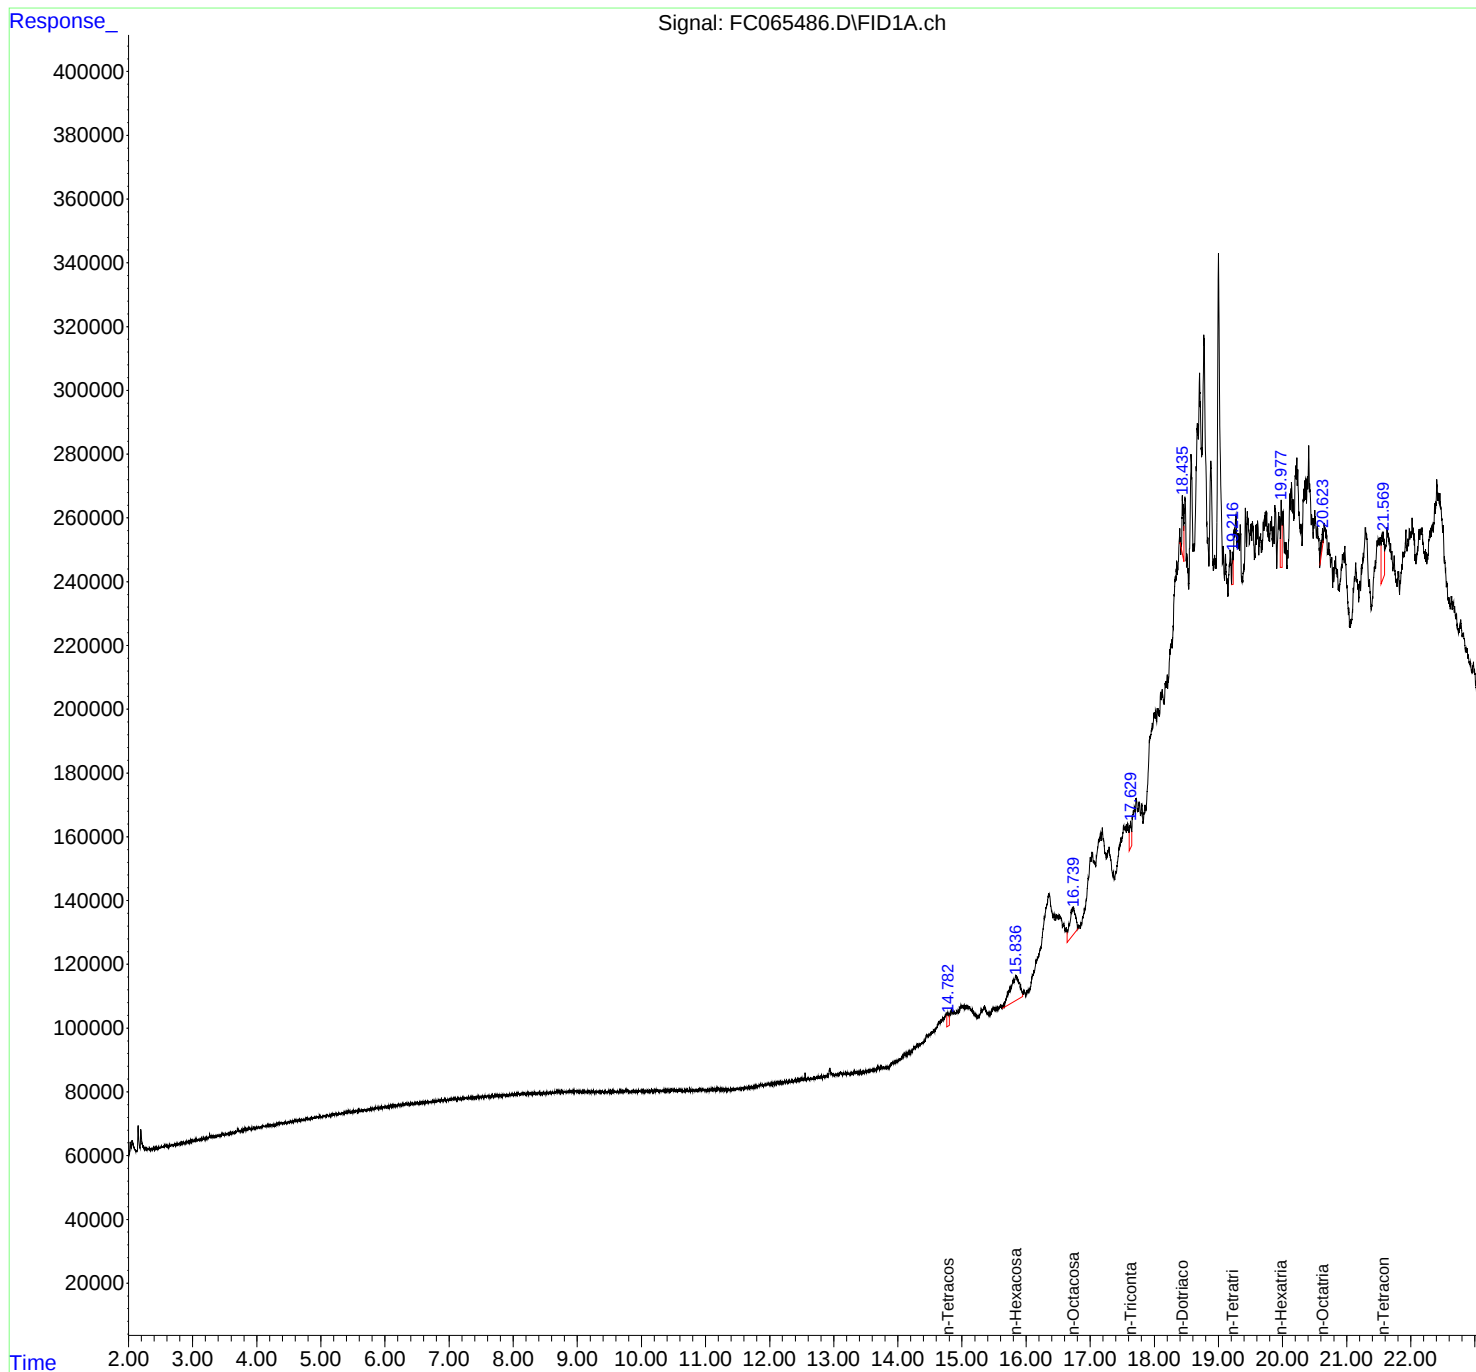


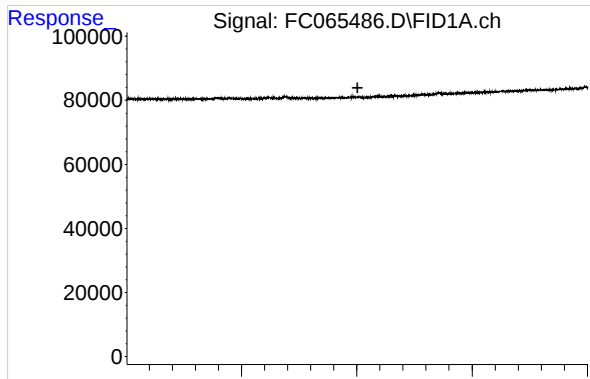

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.503 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

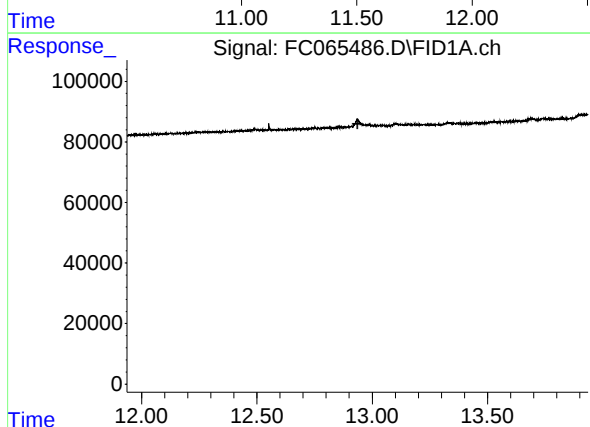


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.936 min
Response: 0
Conc: N.D.

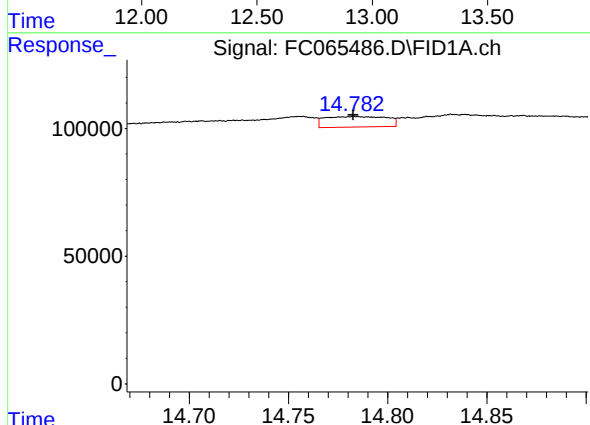


#14 n-Tetracosane (C24)

R.T.: 14.784 min
Delta R.T.: 0.000 min
Response: 88264
Conc: 0.51 ug/ml

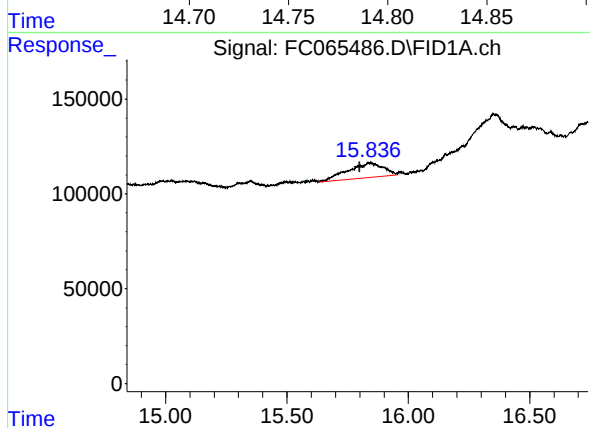

#15 n-Hexacosane (C26)


R.T.: 15.836 min
Delta R.T.: 0.037 min
Response: 797245
Conc: 4.79 ug/ml

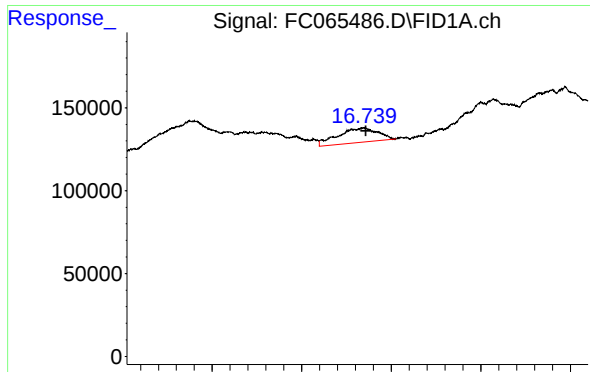

#16 n-Octacosane (C28)


R.T.: 16.739 min
Delta R.T.: -0.005 min
Response: 539350
Conc: 3.37 ug/ml

Instrument :
FID_C
ClientSampleId :

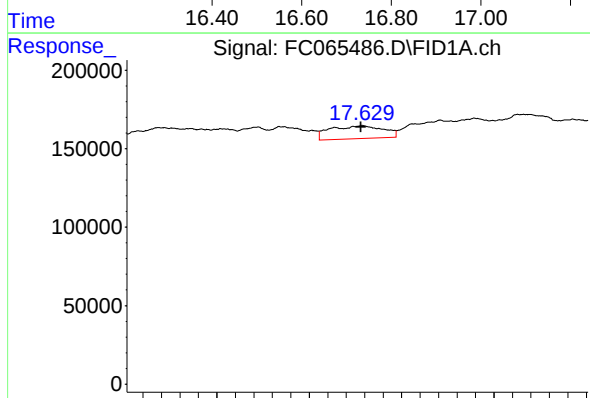


#17 n-Tricontane (C30)

R.T.: 17.628 min
Delta R.T.: 0.000 min
Response: 164517
Conc: 1.03 ug/ml

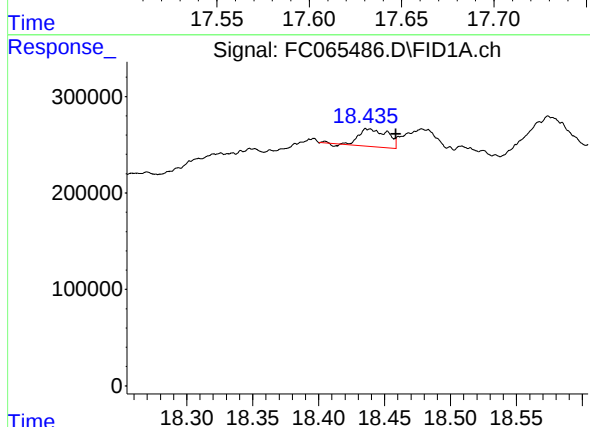


#18 n-Dotriacontane (C32)

R.T.: 18.439 min
Delta R.T.: -0.020 min
Response: 276222
Conc: 1.76 ug/ml

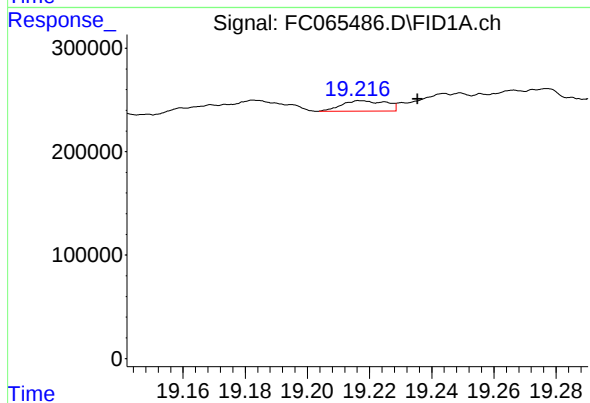

#19 n-Tetratriacontane (C34)


R.T.: 19.218 min
Delta R.T.: -0.017 min
Response: 100773
Conc: 0.65 ug/ml

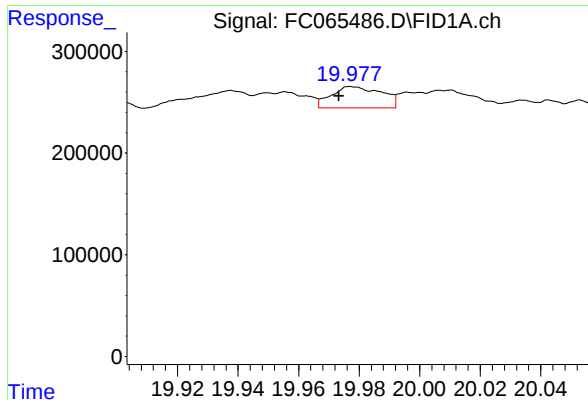

#20 n-Hexatriacontane (C36)


R.T.: 19.979 min
Delta R.T.: 0.005 min
Response: 241718
Conc: 1.58 ug/ml

Instrument :
FID_C
ClientSampleId :

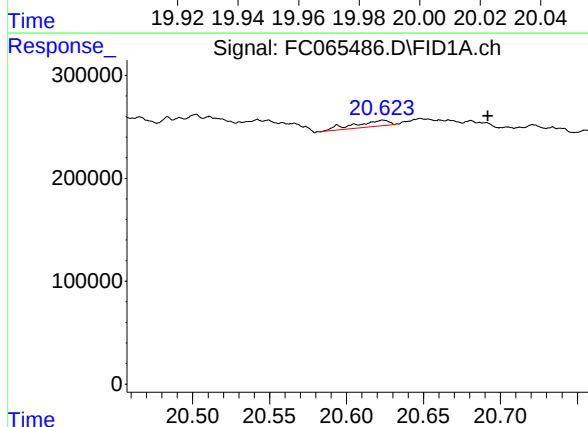

#21 n-Octatriacontane (C38)

R.T.: 20.623 min
Delta R.T.: -0.069 min
Response: 90338
Conc: 0.59 ug/ml

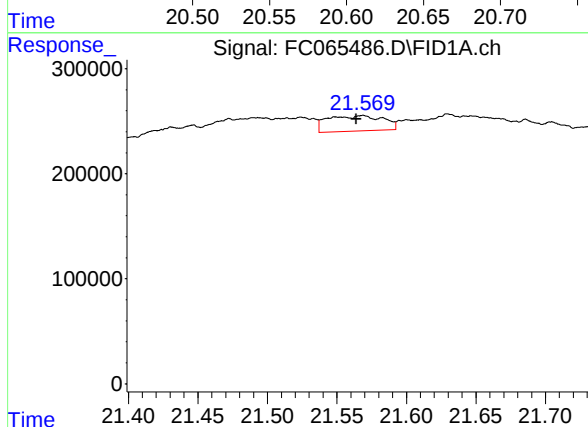

#22 n-Tetracontane (C40)

R.T.: 21.568 min
Delta R.T.: 0.004 min
Response: 408590
Conc: 2.73 ug/ml