

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121523AL\
Data File : FC065488.D
Signal(s) : FID1A.ch
Acq On : 15 Dec 2023 22:01
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 02:38:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 112423.M
Quant Title : GC Extractables
QLast Update : Fri Nov 24 13:28:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.627	146637	0.921 ug/ml
19) T	n-Tetratriacontane (C34)	19.288f	70857	0.459 ug/ml
20) T	n-Hexatriacontane (C36)	20.001	676560	4.414 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121523AL\
Data File : FC065488.D
Signal(s) : FID1A.ch
Acq On : 15 Dec 2023 22:01
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 02:38:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 112423.M
Quant Title : GC Extractables
QLast Update : Fri Nov 24 13:28:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

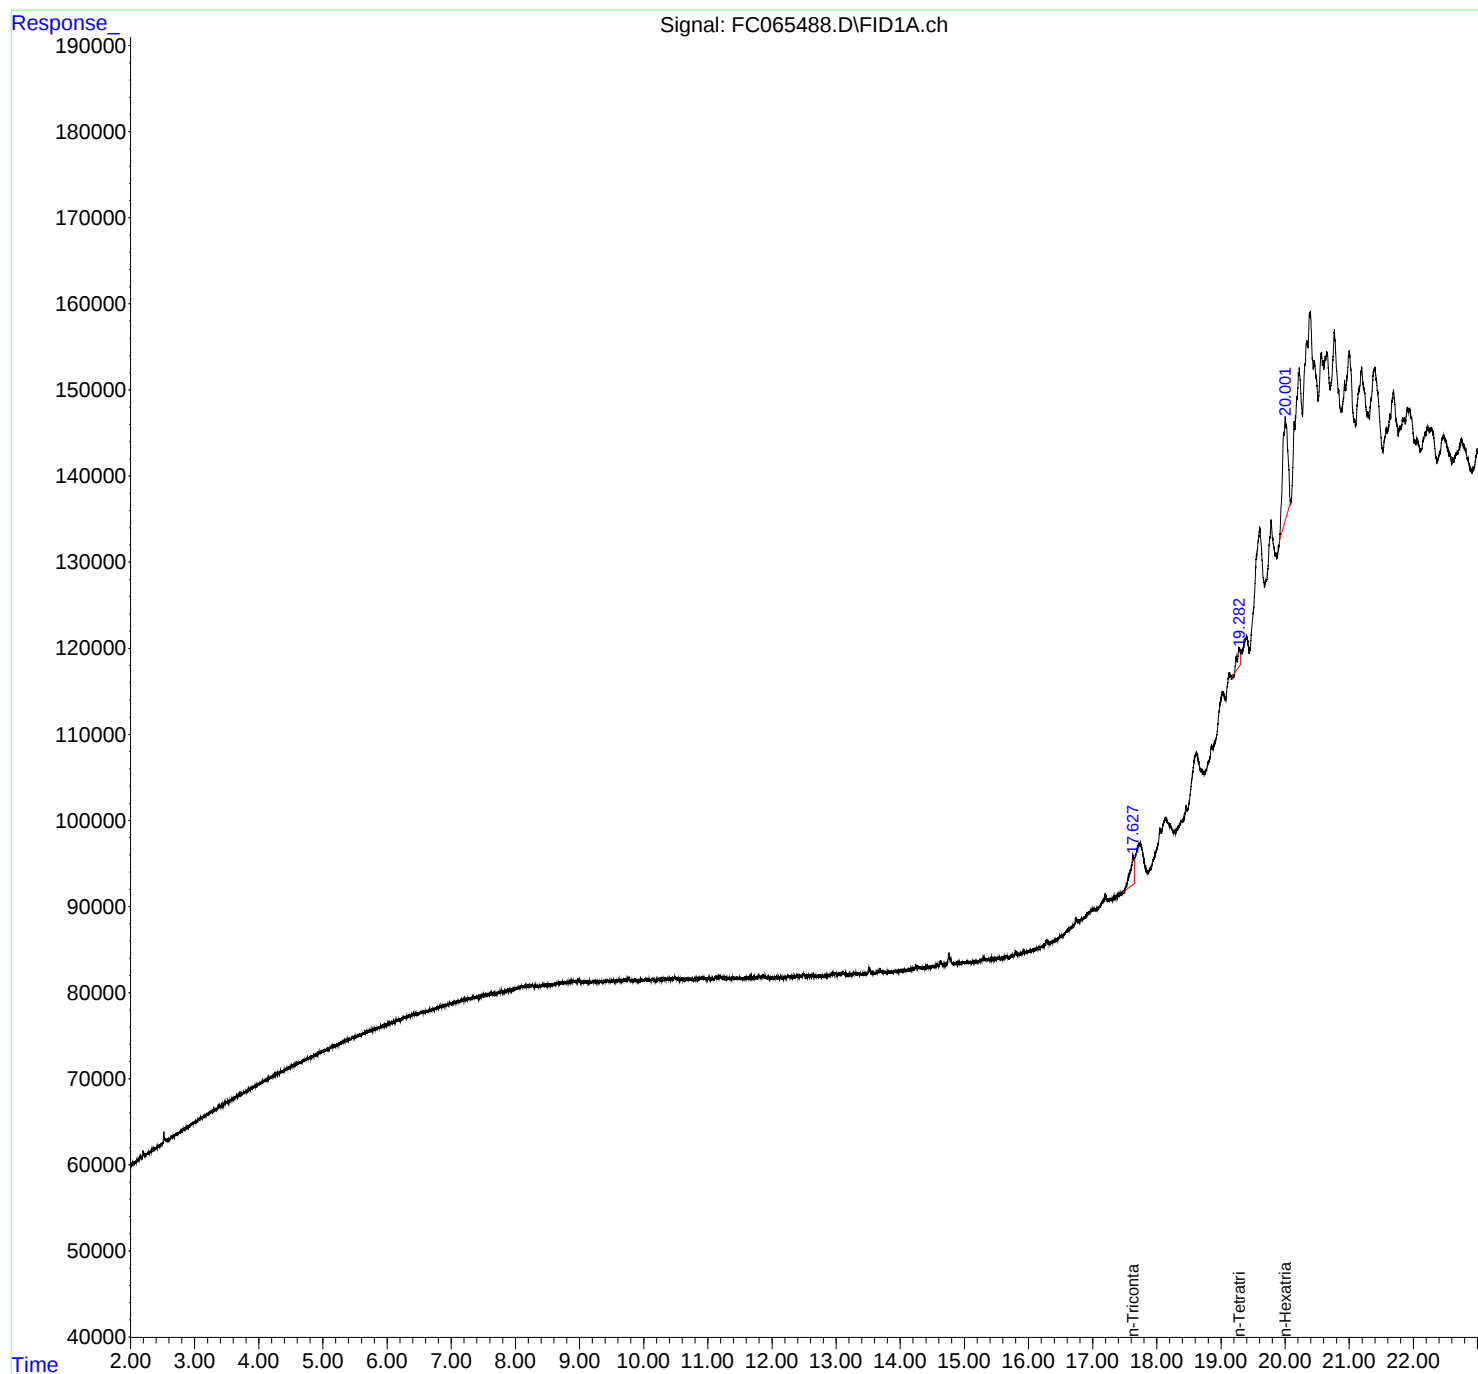


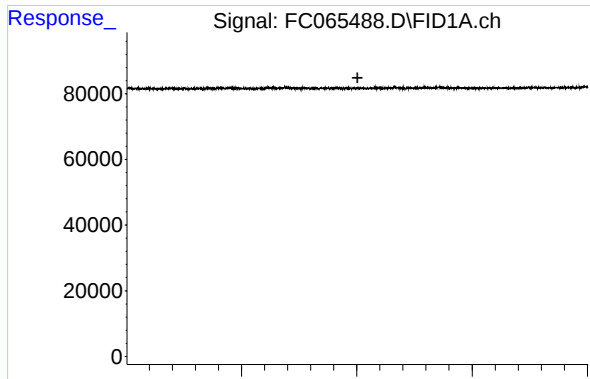

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.503 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

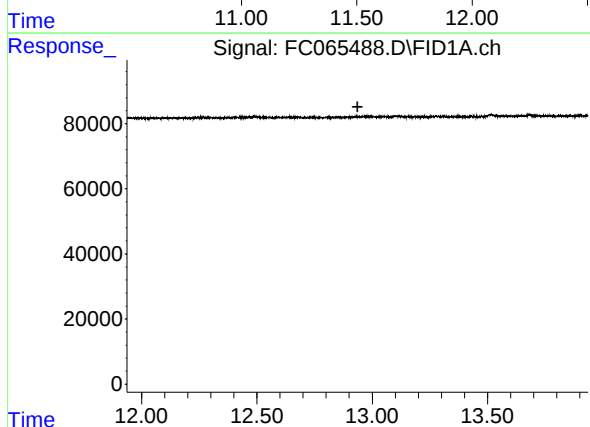


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.936 min
Response: 0
Conc: N.D.

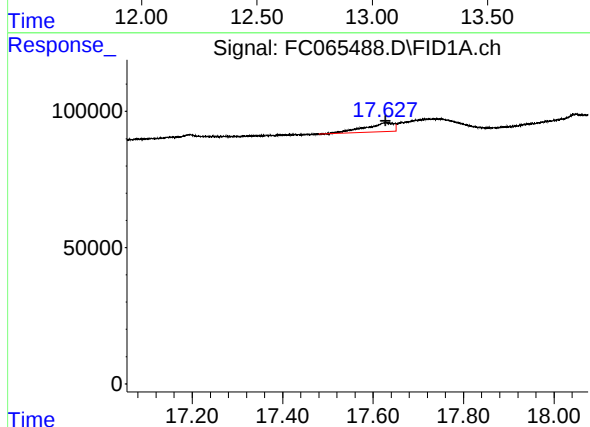


#17 n-Tricontane (C30)

R.T.: 17.627 min
Delta R.T.: 0.000 min
Response: 146637
Conc: 0.92 ug/ml

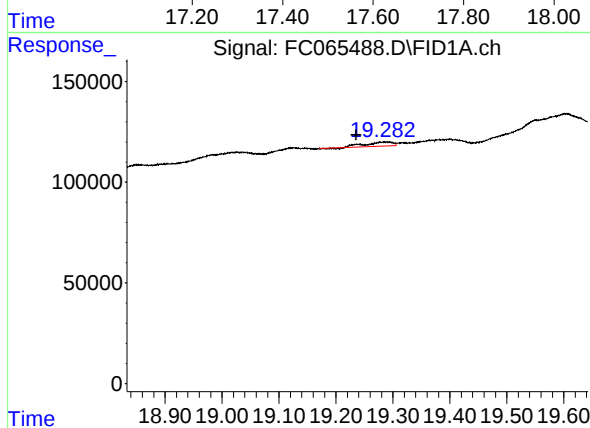

#19 n-Tetratriacontane (C34)

R.T.: 19.288 min
Delta R.T.: 0.053 min
Response: 70857
Conc: 0.46 ug/ml

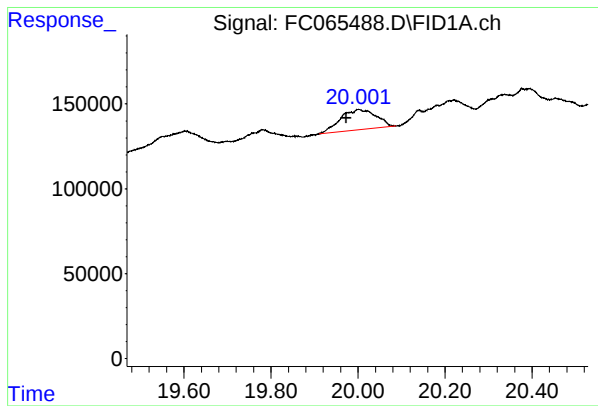

#20 n-Hexatriacontane (C36)

R.T.: 20.001 min
Delta R.T.: 0.028 min
Response: 676560
Conc: 4.41 ug/ml

Instrument :

FID_C

ClientSampleId :