

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121621AL\
 Data File : FC057518.D
 Signal(s) : FID1A.CH
 Acq On : 16 Dec 2021 8:46
 Operator : AJ\MA
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 16 11:38:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 20:43:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

17) T	n-Tricontane (C30)	16.976	57669	0.422 ug/ml
18) T	n-Dotriacontane (C32)	17.842	76990	0.574 ug/ml
19) T	n-Tetratriacontane (C34)	18.591	208269	1.597 ug/ml
20) T	n-Hexatriacontane (C36)	19.334	196669	1.656 ug/ml
21) T	n-Octatriacontane (C38)	20.058	138742	1.263 ug/ml
22) T	n-Tetracontane (C40)	21.028	173067	1.733 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121621AL\
Data File : FC057518.D
Signal(s) : FID1A.CH
Acq On : 16 Dec 2021 8:46
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 11:38:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 20:43:13 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

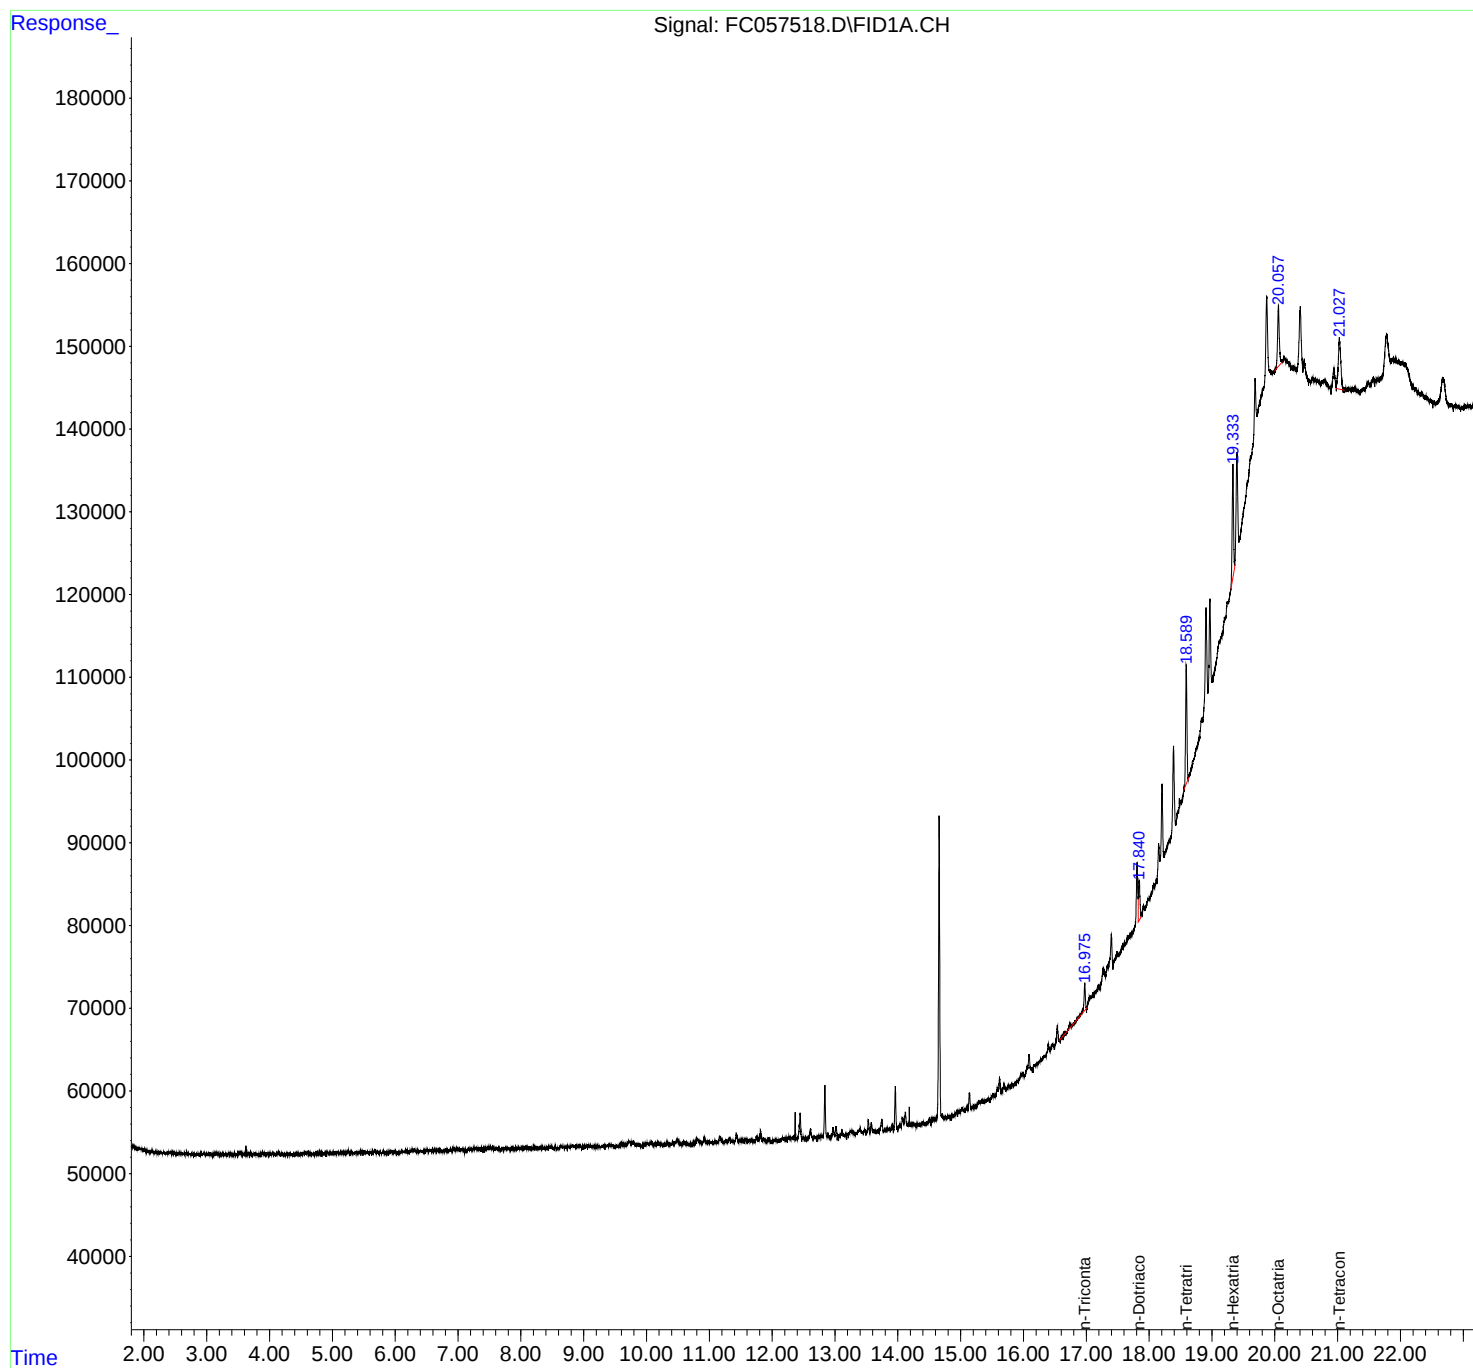


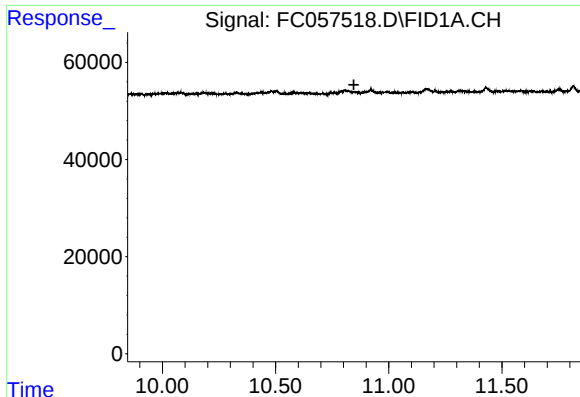

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 10.846 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

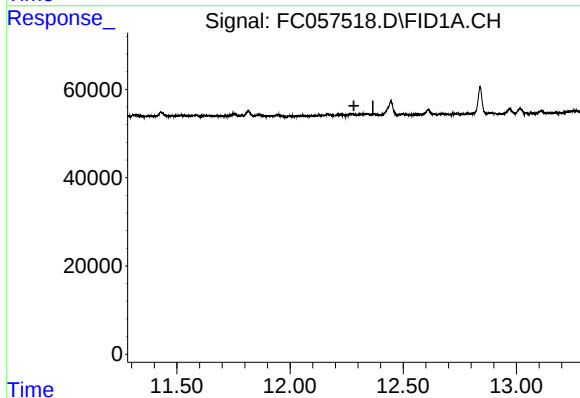


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 12.282 min
Response: 0
Conc: N.D.

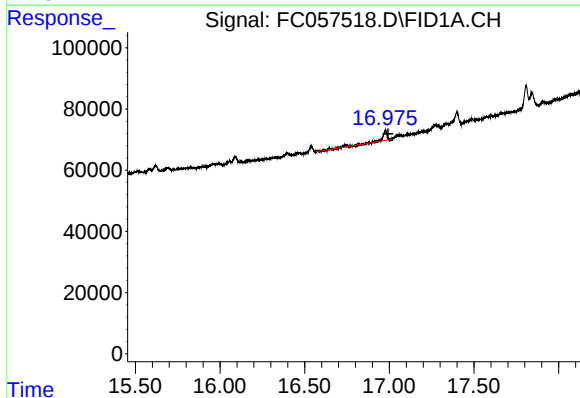


#17 n-Tricontane (C30)

R.T.: 16.976 min
Delta R.T.: -0.017 min
Response: 57669
Conc: 0.42 ug/ml

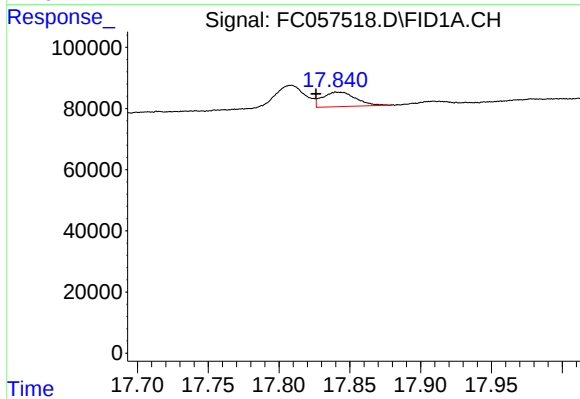

#18 n-Dotriacontane (C32)


R.T.: 17.842 min
Delta R.T.: 0.016 min
Response: 76990
Conc: 0.57 ug/ml

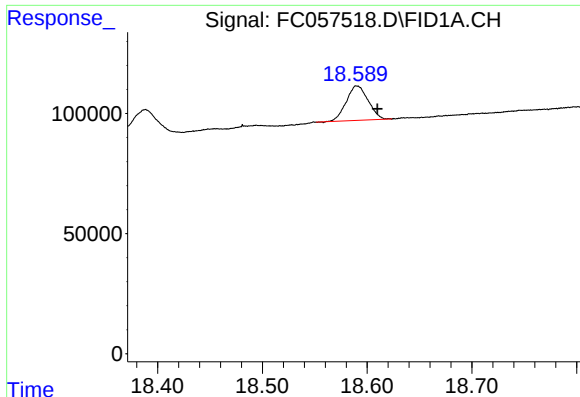

#19 n-Tetratriacontane (C34)


R.T.: 18.591 min
Delta R.T.: -0.019 min
Response: 208269
Conc: 1.60 ug/ml

Instrument :
FID_C
ClientSampleId :

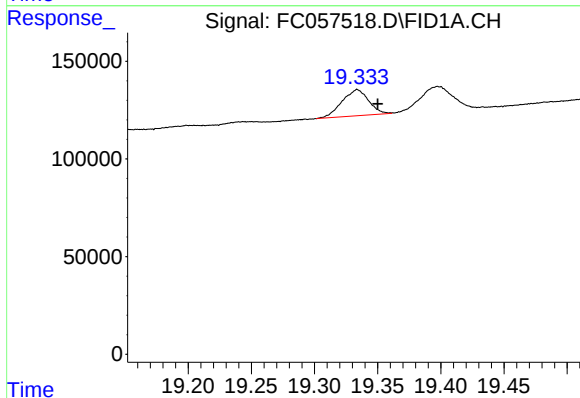


#20 n-Hexatriacontane (C36)

R.T.: 19.334 min
Delta R.T.: -0.016 min
Response: 196669
Conc: 1.66 ug/ml

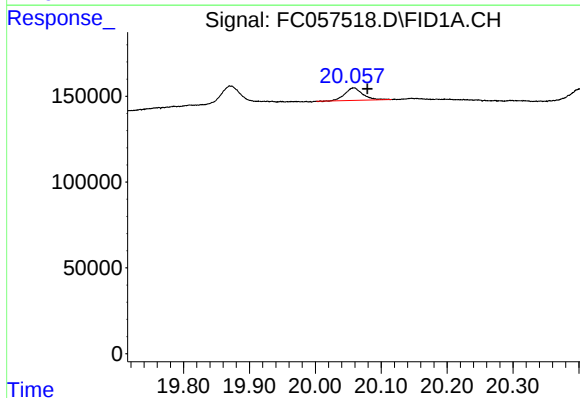

#21 n-Octatriacontane (C38)

R.T.: 20.058 min
Delta R.T.: -0.021 min
Response: 138742
Conc: 1.26 ug/ml

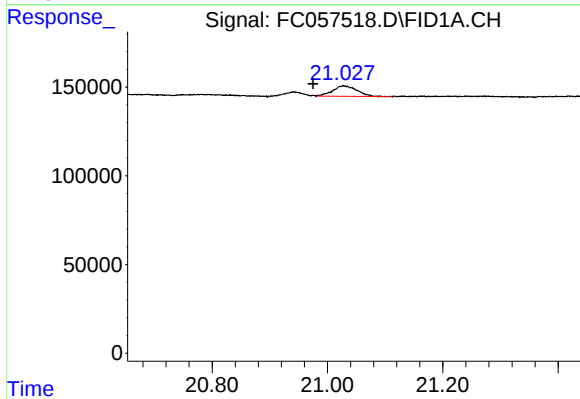

#22 n-Tetracontane (C40)

R.T.: 21.028 min
Delta R.T.: 0.053 min
Response: 173067
Conc: 1.73 ug/ml