

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121621AL\
 Data File : FC057560.D
 Signal(s) : FID1A.CH
 Acq On : 17 Dec 2021 8:29
 Operator : AJ\MA
 Sample : M5106-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 VAULT-WASTE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/17/2021
 Supervised By :Ankita Jodhani 12/17/2021

Integration File: sample.E
 Quant Time: Dec 17 09:24:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 121421.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 14 20:43:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.824	5652143	40.617 ug/mlm
Spiked Amount 50.000		Recovery =	81.23%
12) S 1-chlorooctadecane (S...	12.261	4600100	41.540 ug/mlm
Spiked Amount 50.000		Recovery =	83.08%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC121621AL\
Data File : FC057560.D
Signal(s) : FID1A.CH
Acq On : 17 Dec 2021 8:29
Operator : AJ\MA
Sample : M5106-01
Misc :
ALS Vial : 38 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
VAULT-WASTE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/17/2021
Supervised By :Ankita Jodhani 12/17/2021

Integration File: sample.E
Quant Time: Dec 17 09:24:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 121421.M
Quant Title : GC Extractables
QLast Update : Tue Dec 14 20:43:13 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

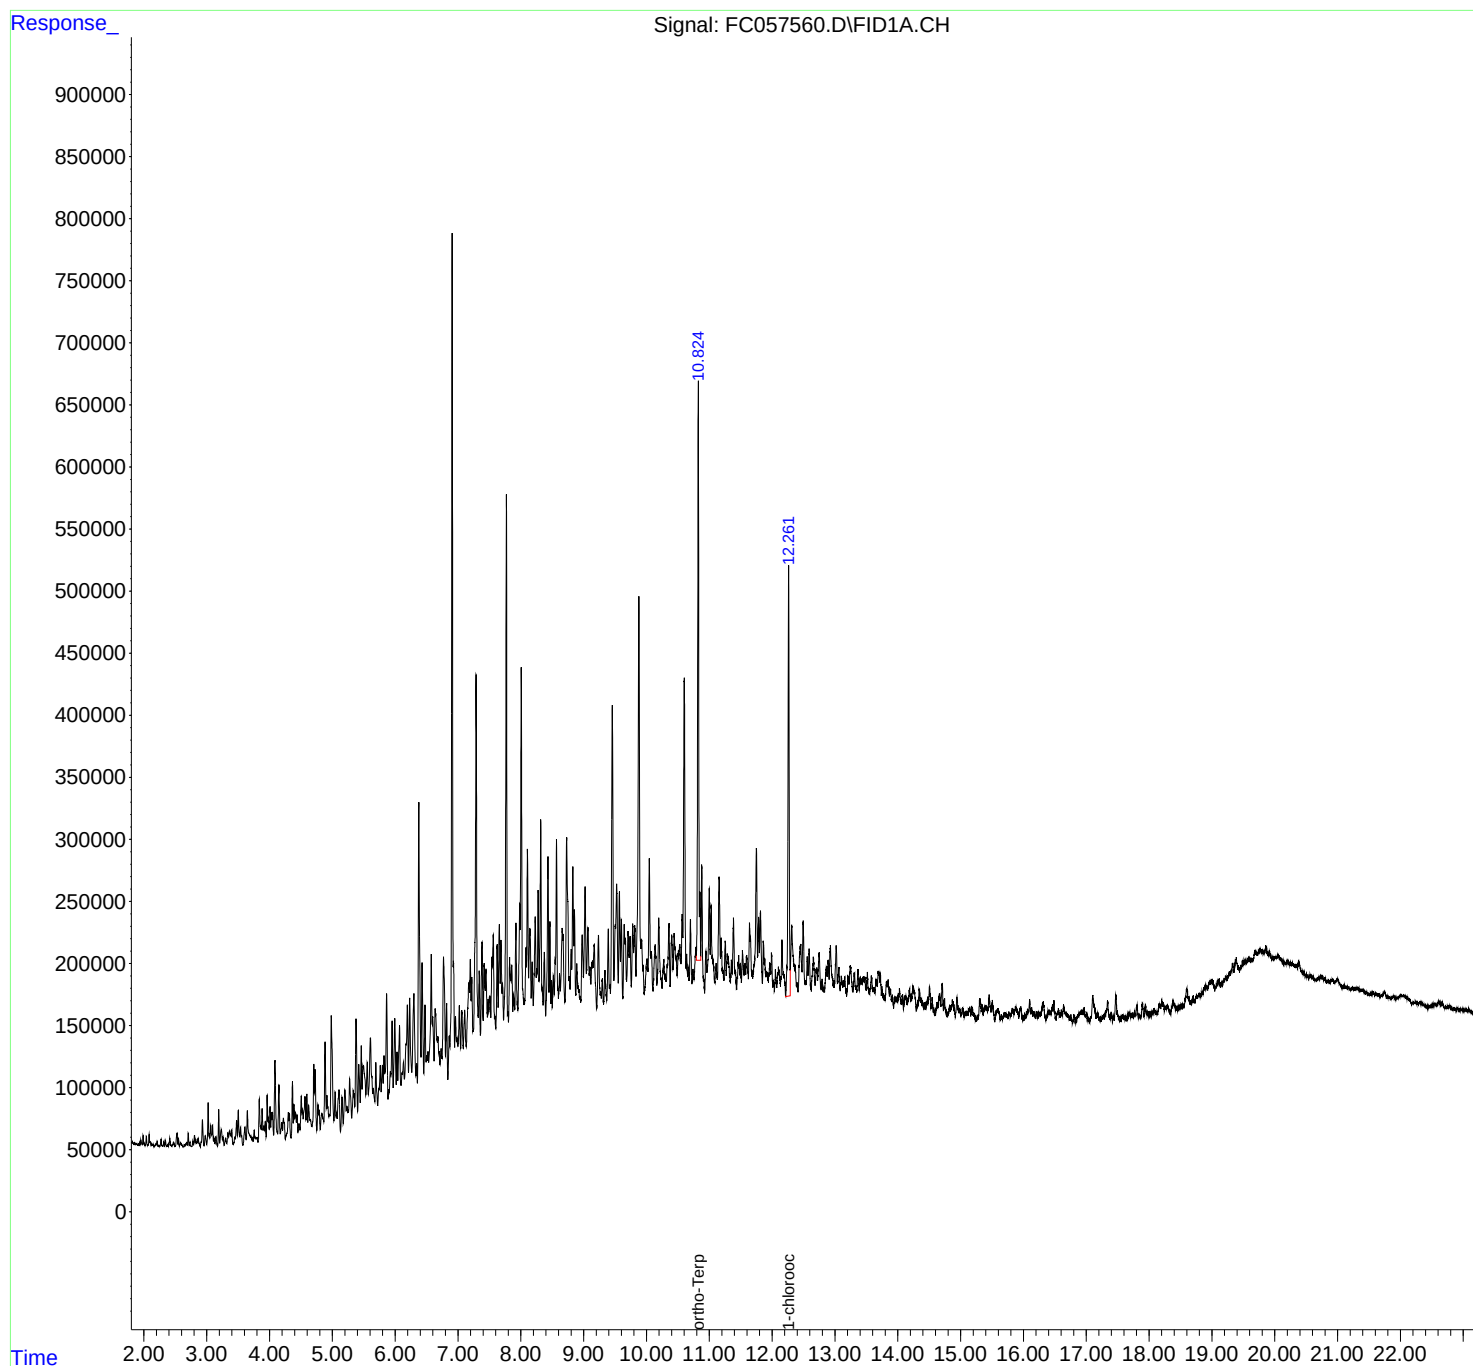

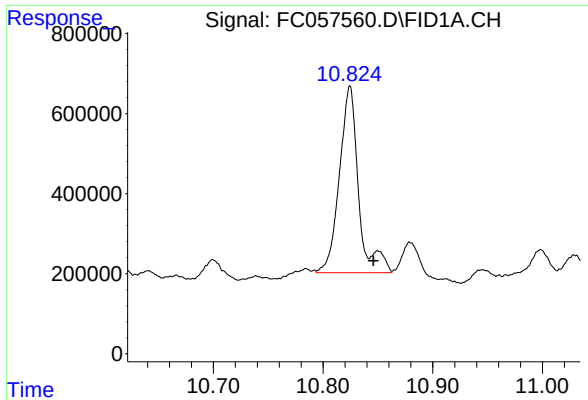


#9 ortho-Terphenyl (SURR)

R.T.: 10.824 min
Delta R.T.: -0.022 min
Response: 5652143
Conc: 40.62 ug/ml

Instrument :
FID_C
ClientSampleId :
VAULT-WASTE

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/17/2021
Supervised By :Ankita Jodhani 12/17/2021

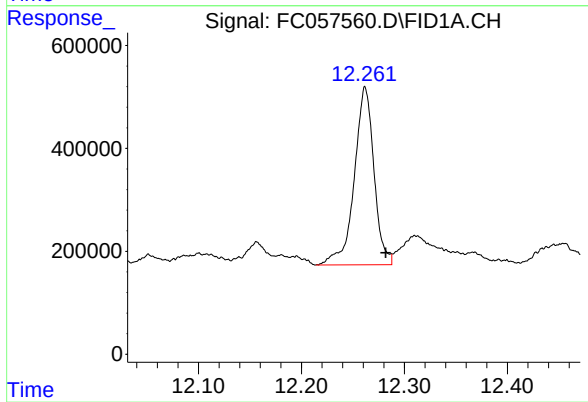

#12 1-chlorooctadecane (SURR)

R.T.: 12.261 min
Delta R.T.: -0.021 min
Response: 4600100
Conc: 41.54 ug/ml m