

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC122118AL\
 Data File : FC038380.D
 Signal(s) : FID1A.CH
 Acq On : 22 Dec 2018 8:26
 Operator : AJ\SJ
 Sample : J6505-13
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 23 21:54:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 121018.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 15 05:55:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.717	2008102	19.917 ug/ml
Spiked Amount 50.000		Recovery =	39.83%
Target Compounds			
14) T n-Tetracosane (C24)	14.569	27023	0.235 ug/ml
15) T n-Hexacosane (C26)	15.585	44859	0.399 ug/ml
16) T n-Octacosane (C28)	16.530	89109	0.793 ug/ml
17) T n-Tricontane (C30)	17.413	85036	0.775 ug/ml
18) T n-Dotriacontane (C32)	18.243	101845	0.994 ug/ml
19) T n-Tetratriacontane (C34)	19.025	46471	0.527 ug/ml
20) T n-Hexatriacontane (C36)	19.769	102504	1.308 ug/ml
21) T n-Octatriacontane (C38)	20.459	239901	3.100 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC122118AL\
Data File : FC038380.D
Signal(s) : FID1A.CH
Acq On : 22 Dec 2018 8:26
Operator : AJ\SJ
Sample : J6505-13
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 23 21:54:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 121018.M
Quant Title : GC Extractables
QLast Update : Sat Dec 15 05:55:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

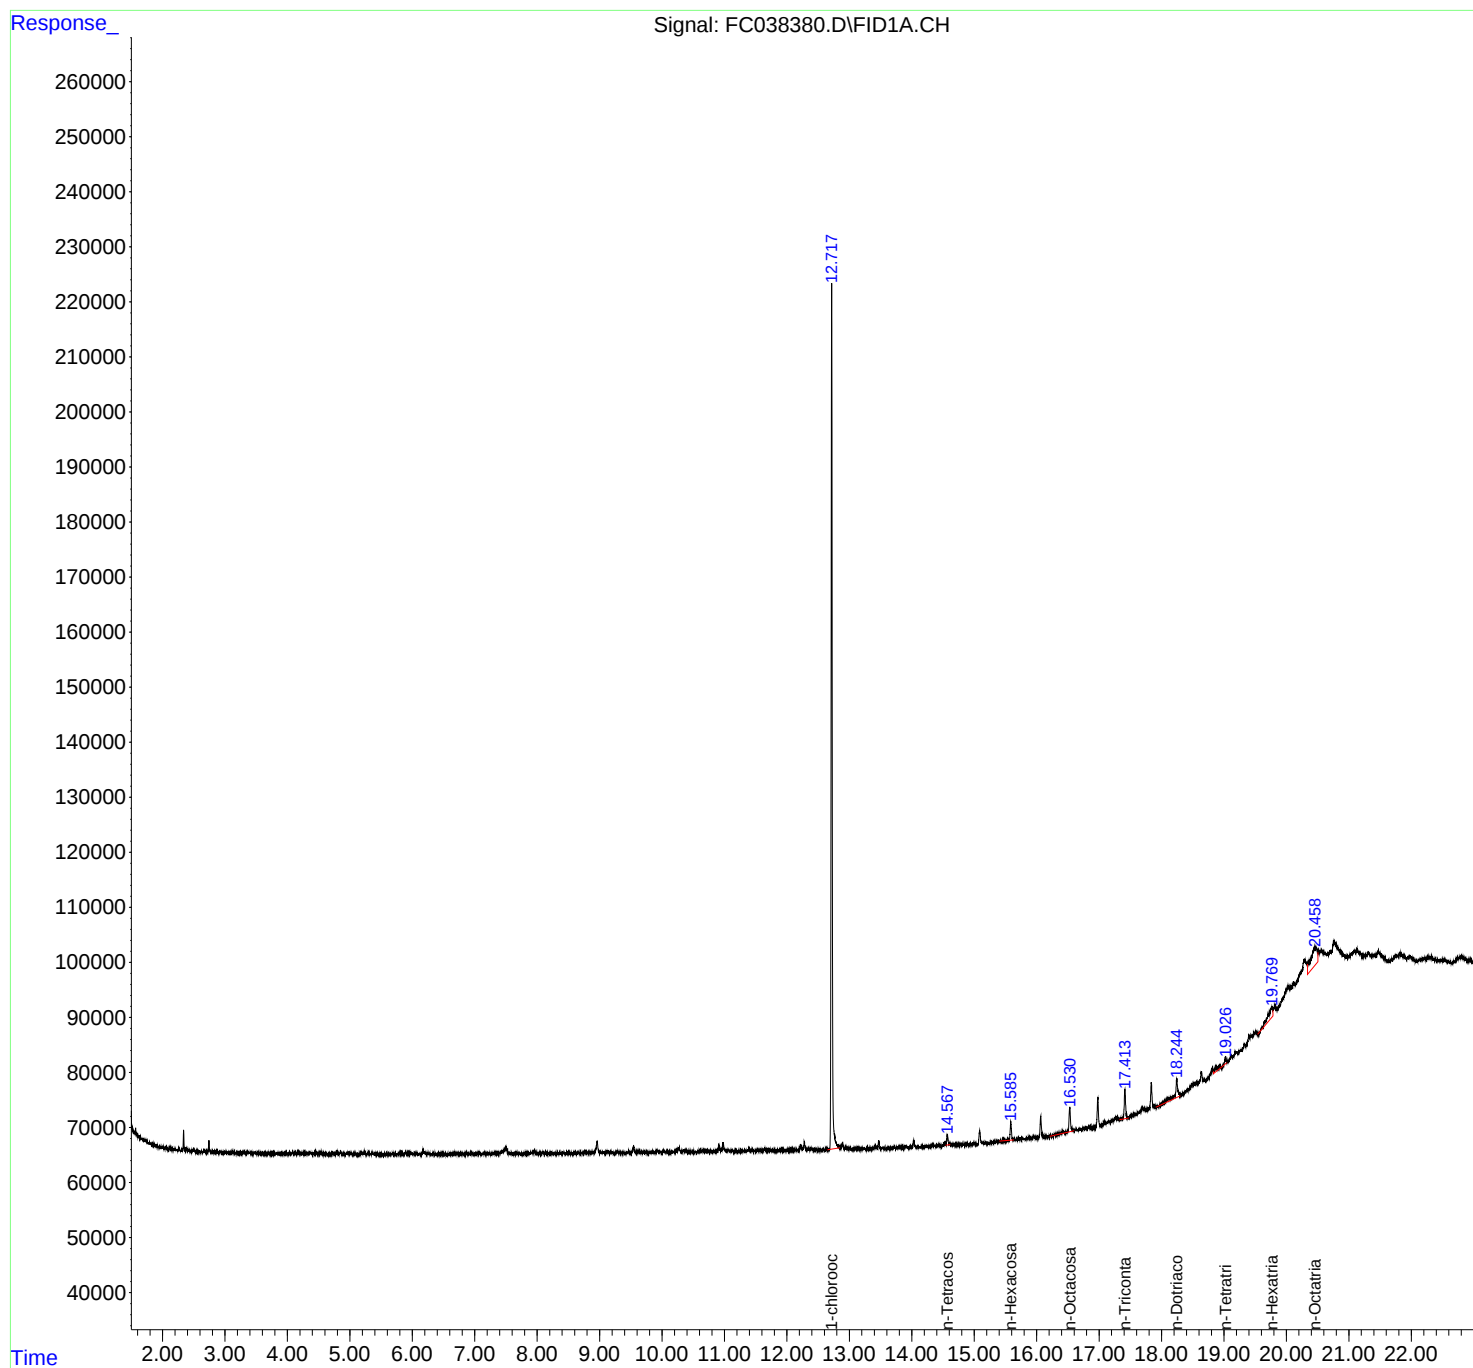


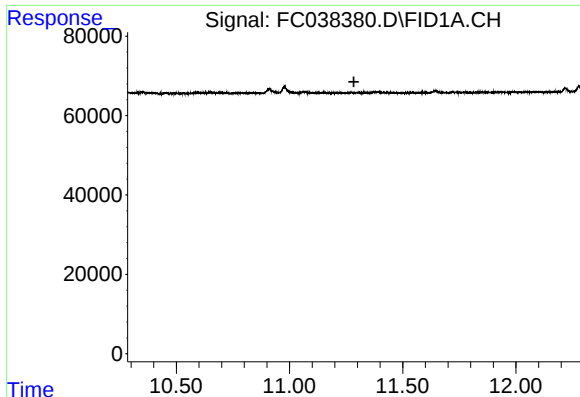

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.284 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

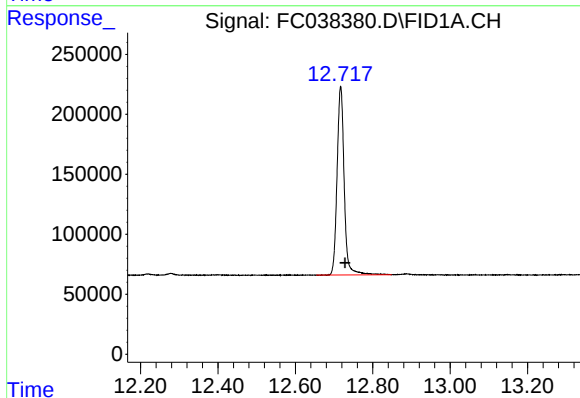


#12 1-chlorooctadecane (SURR)

R.T.: 12.717 min
Delta R.T.: -0.011 min
Response: 2008102
Conc: 19.92 ug/ml

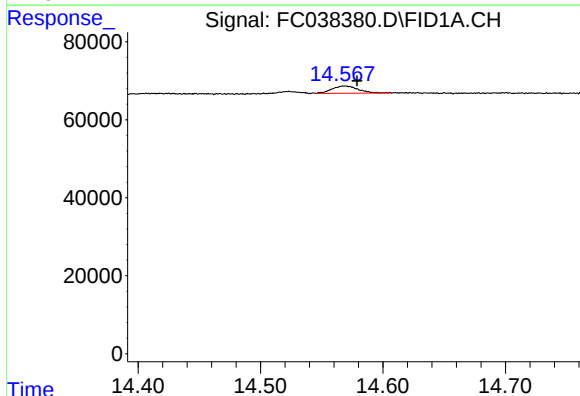


#14 n-Tetracosane (C24)

R.T.: 14.569 min
Delta R.T.: -0.010 min
Response: 27023
Conc: 0.24 ug/ml

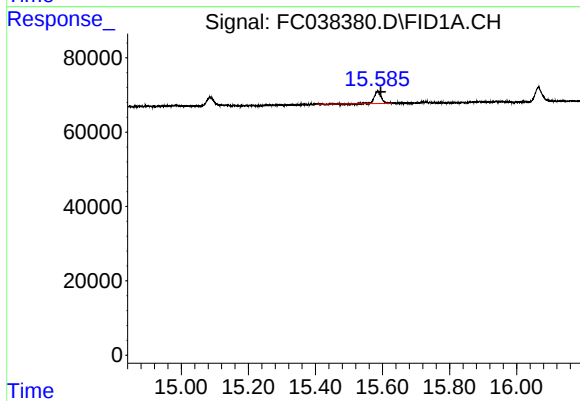

#15 n-Hexacosane (C26)


R.T.: 15.585 min
Delta R.T.: -0.009 min
Response: 44859
Conc: 0.40 ug/ml

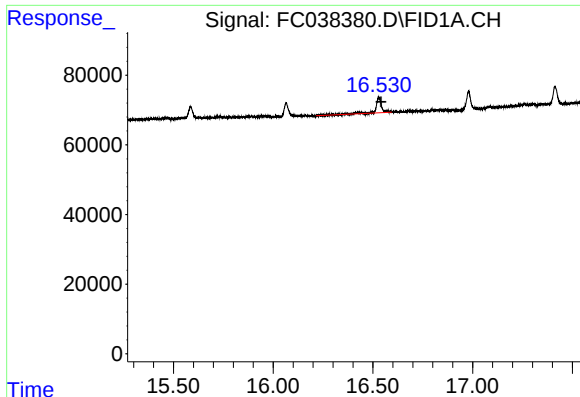

#16 n-Octacosane (C28)


R.T.: 16.530 min
Delta R.T.: -0.010 min
Response: 89109
Conc: 0.79 ug/ml

Instrument :
FID_C
ClientSampleId :

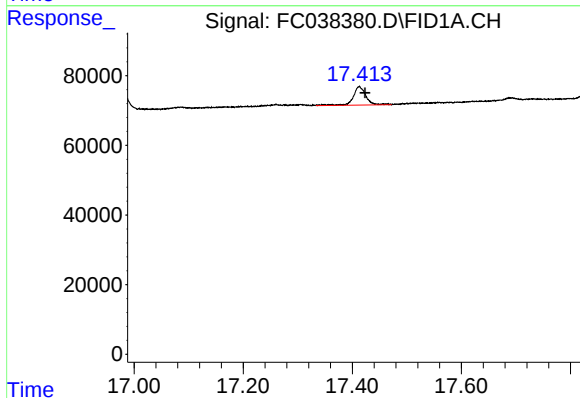


#17 n-Tricontane (C30)

R.T.: 17.413 min
Delta R.T.: -0.010 min
Response: 85036
Conc: 0.77 ug/ml

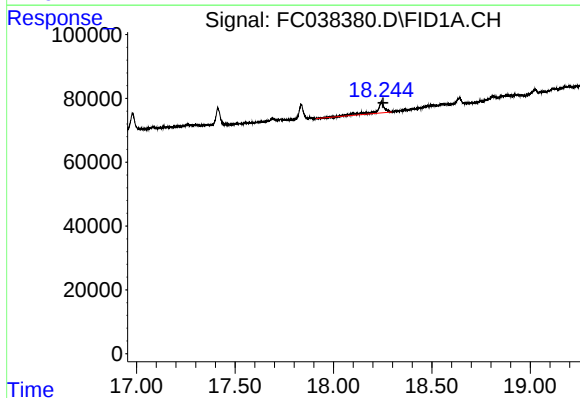


#18 n-Dotriacontane (C32)

R.T.: 18.243 min
Delta R.T.: -0.009 min
Response: 101845
Conc: 0.99 ug/ml

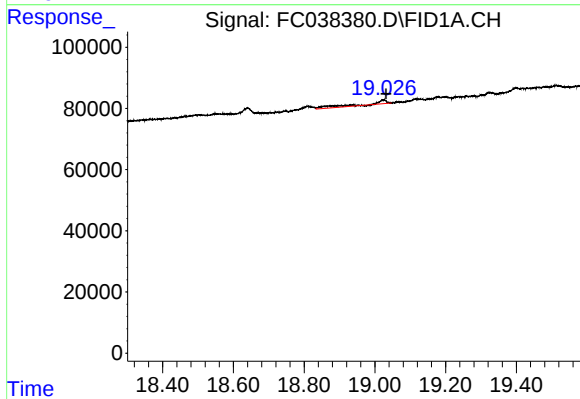

#19 n-Tetratriacontane (C34)


R.T.: 19.025 min
Delta R.T.: -0.007 min
Response: 46471
Conc: 0.53 ug/ml

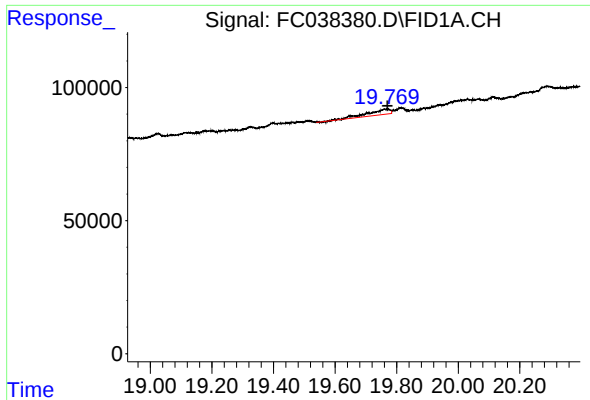

#20 n-Hexatriacontane (C36)

R.T.: 19.769 min
Delta R.T.: -0.001 min
Response: 102504
Conc: 1.31 ug/ml

Instrument :
FID_C
ClientSampleId :

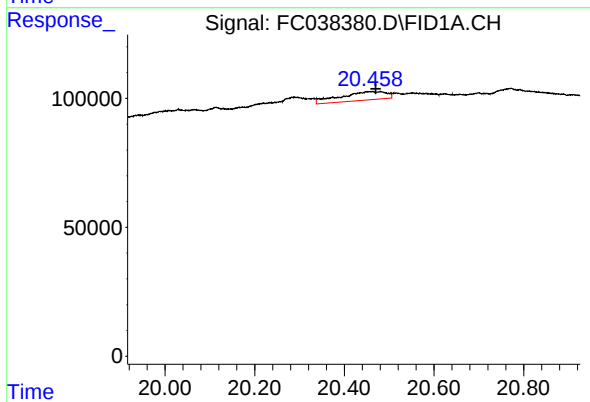

#21 n-Octatriacontane (C38)

R.T.: 20.459 min
Delta R.T.: -0.010 min
Response: 239901
Conc: 3.10 ug/ml