

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC122618AL\
 Data File : FC038390.D
 Signal(s) : FID1A.CH
 Acq On : 26 Dec 2018 8:51
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 26 15:09:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 121018.M
 Quant Title : GC Extractables
 QLast Update : Sat Dec 15 05:55:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
17) T n-Tricontane (C30)	17.404	24102	0.220 ug/ml
18) T n-Dotriacontane (C32)	18.261	78255	0.764 ug/ml
19) T n-Tetratriacontane (C34)	19.043	274878	3.119 ug/ml
20) T n-Hexatriacontane (C36)	19.741	168622	2.152 ug/ml
21) T n-Octatriacontane (C38)	20.485	290776	3.758 ug/ml
22) T n-Tetracontane (C40)	21.294	76016	0.870 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC122618AL\
Data File : FC038390.D
Signal(s) : FID1A.CH
Acq On : 26 Dec 2018 8:51
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 26 15:09:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 121018.M
Quant Title : GC Extractables
QLast Update : Sat Dec 15 05:55:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

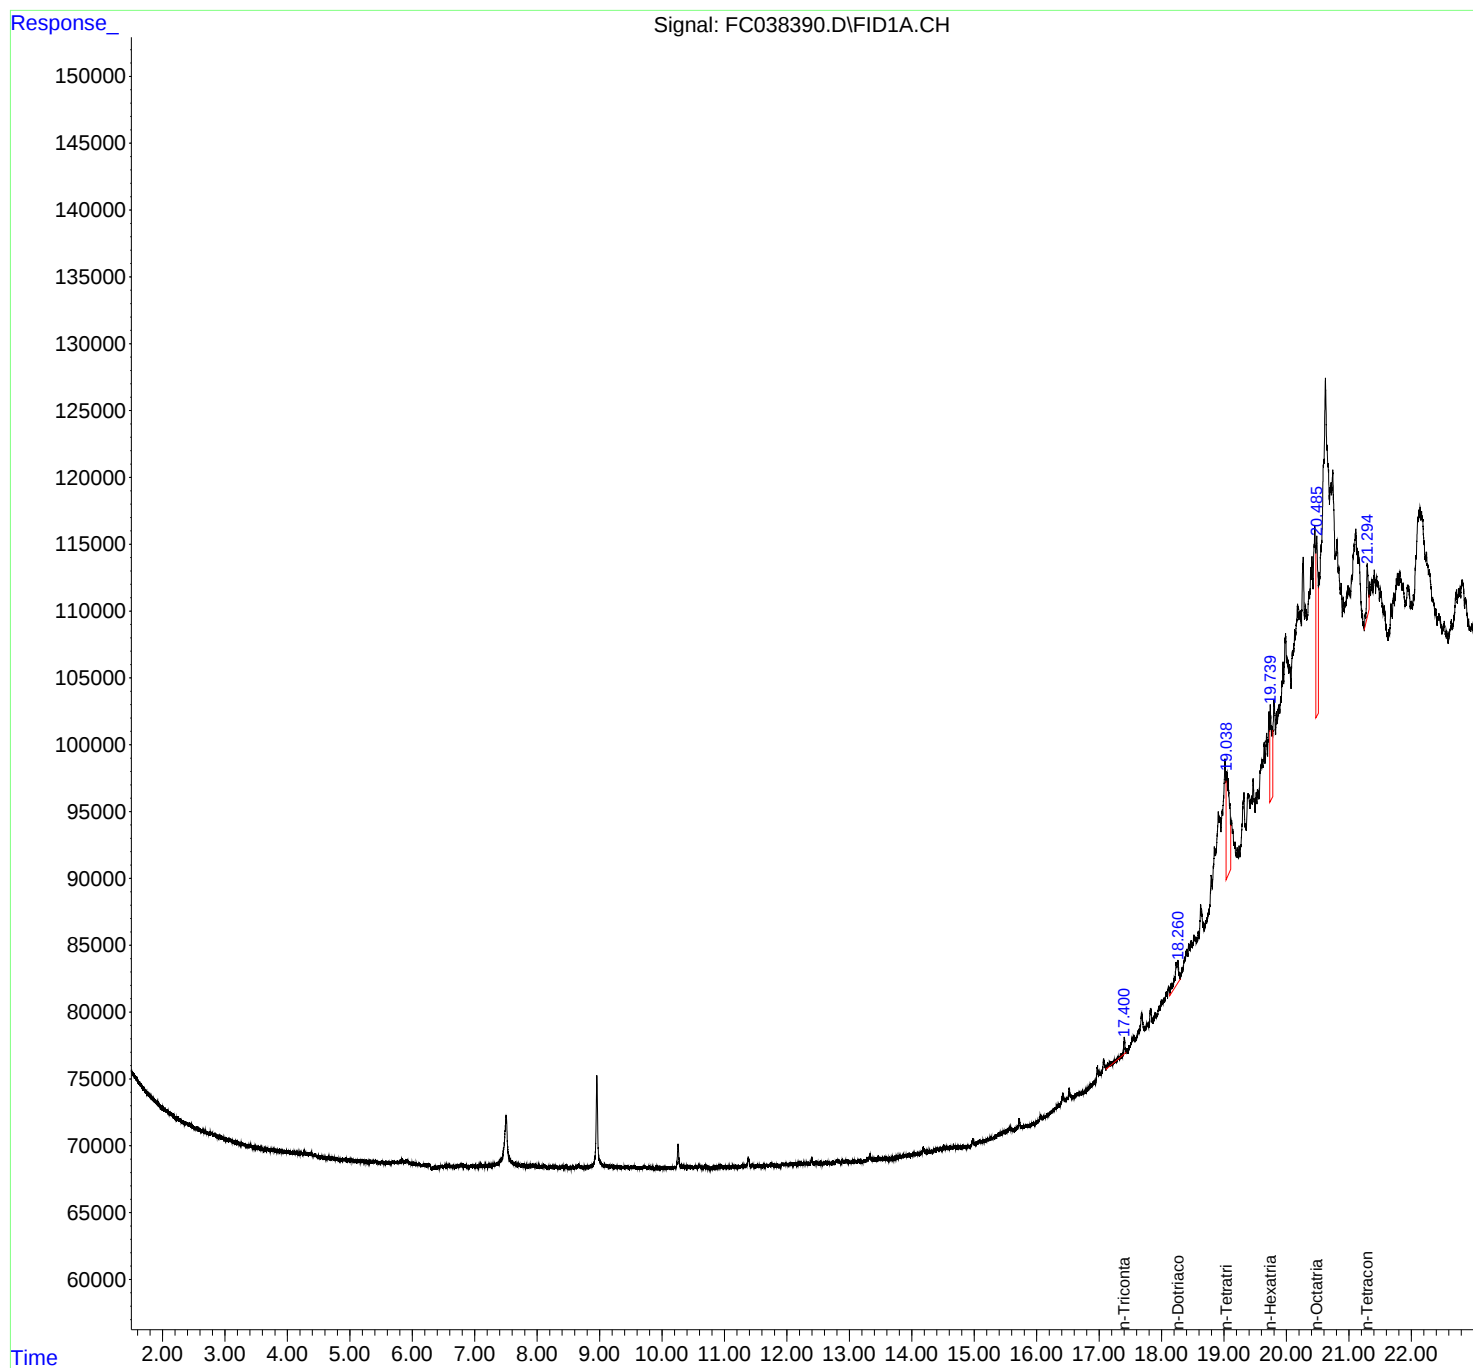


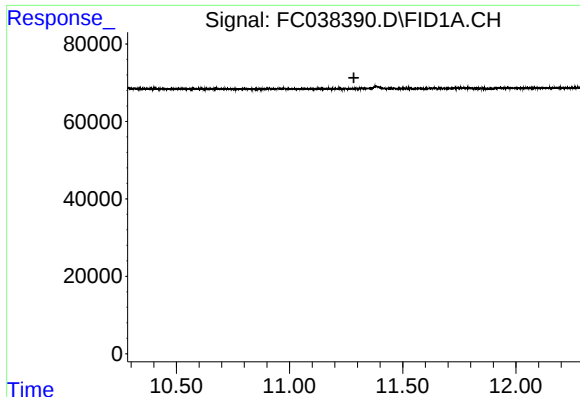

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T. : 11.284 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

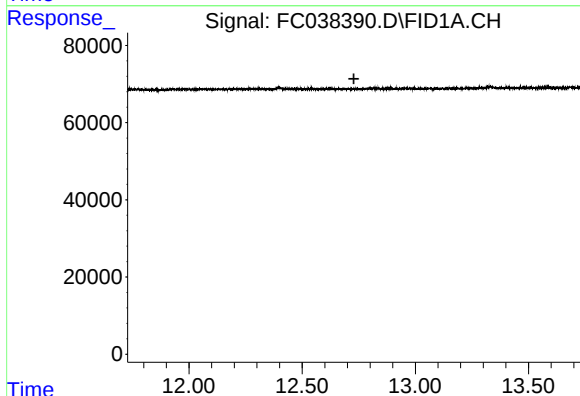


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T. : 12.728 min
Response: 0
Conc: N.D.

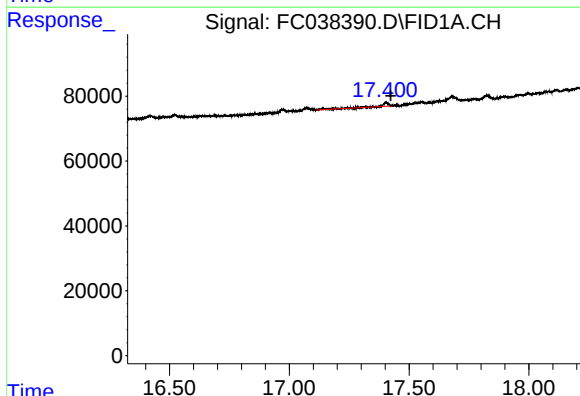


#17 n-Tricontane (C30)

R.T.: 17.404 min
Delta R.T.: -0.019 min
Response: 24102
Conc: 0.22 ug/ml

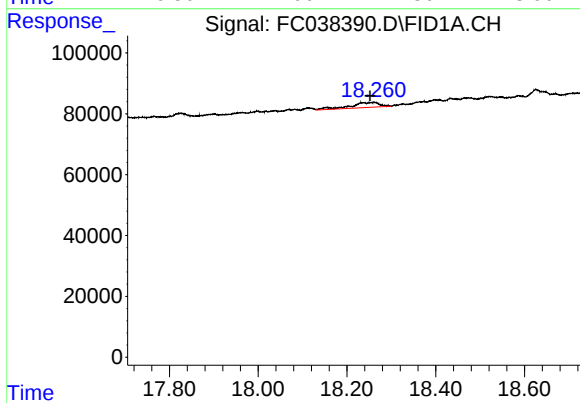

#18 n-Dotriacontane (C32)


R.T.: 18.261 min
Delta R.T.: 0.009 min
Response: 78255
Conc: 0.76 ug/ml

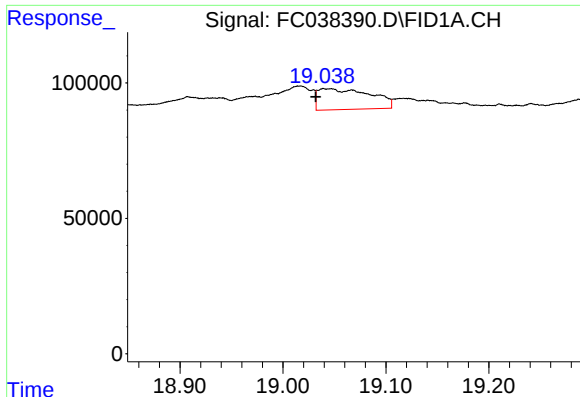

#19 n-Tetratriacontane (C34)


R.T.: 19.043 min
Delta R.T.: 0.011 min
Response: 274878
Conc: 3.12 ug/ml

Instrument :
FID_C
ClientSampleId :

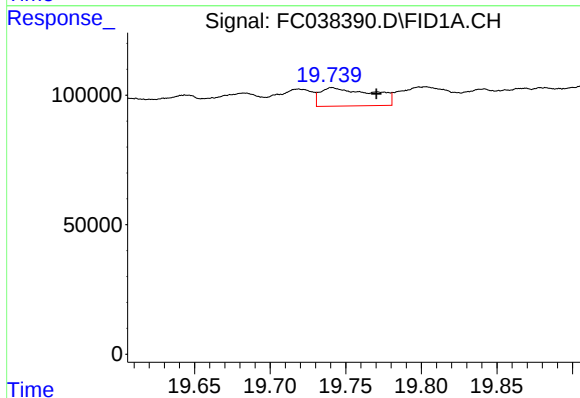


#20 n-Hexatriacontane (C36)

R.T.: 19.741 min
Delta R.T.: -0.029 min
Response: 168622
Conc: 2.15 ug/ml

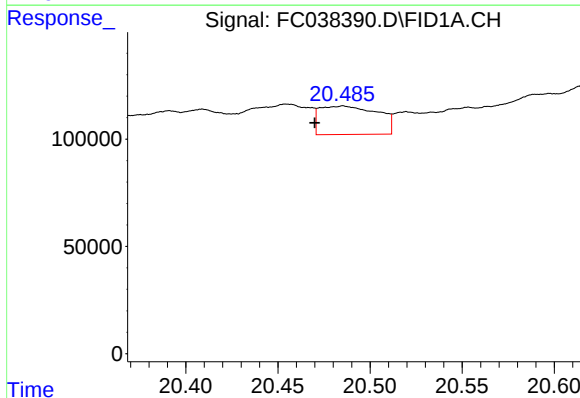

#21 n-Octatriacontane (C38)

R.T.: 20.485 min
Delta R.T.: 0.015 min
Response: 290776
Conc: 3.76 ug/ml

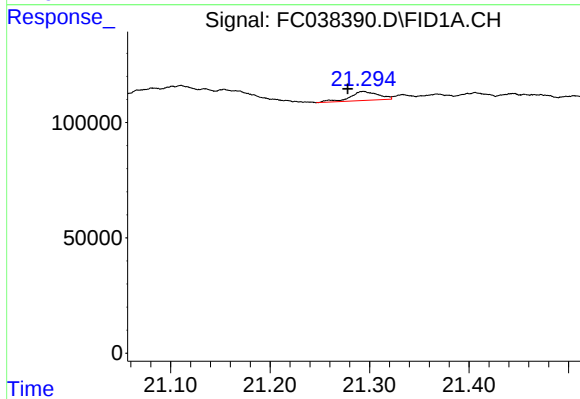

#22 n-Tetracontane (C40)

R.T.: 21.294 min
Delta R.T.: 0.016 min
Response: 76016
Conc: 0.87 ug/ml