

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC122822AL\
Data File : FC062488.D
Signal(s) : FID1A.ch
Acq On : 28 Dec 2022 09:36
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 28 18:04:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 120722.M
Quant Title : GC Extractables
QLast Update : Thu Dec 08 01:05:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.569	86865	0.782 ug/ml
20) T	n-Hexatriacontane (C36)	20.070	65130	0.642 ug/ml
22) T	n-Tetracontane (C40)	21.771	120648	1.190 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC122822AL\
Data File : FC062488.D
Signal(s) : FID1A.ch
Acq On : 28 Dec 2022 09:36
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 28 18:04:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 120722.M
Quant Title : GC Extractables
QLast Update : Thu Dec 08 01:05:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

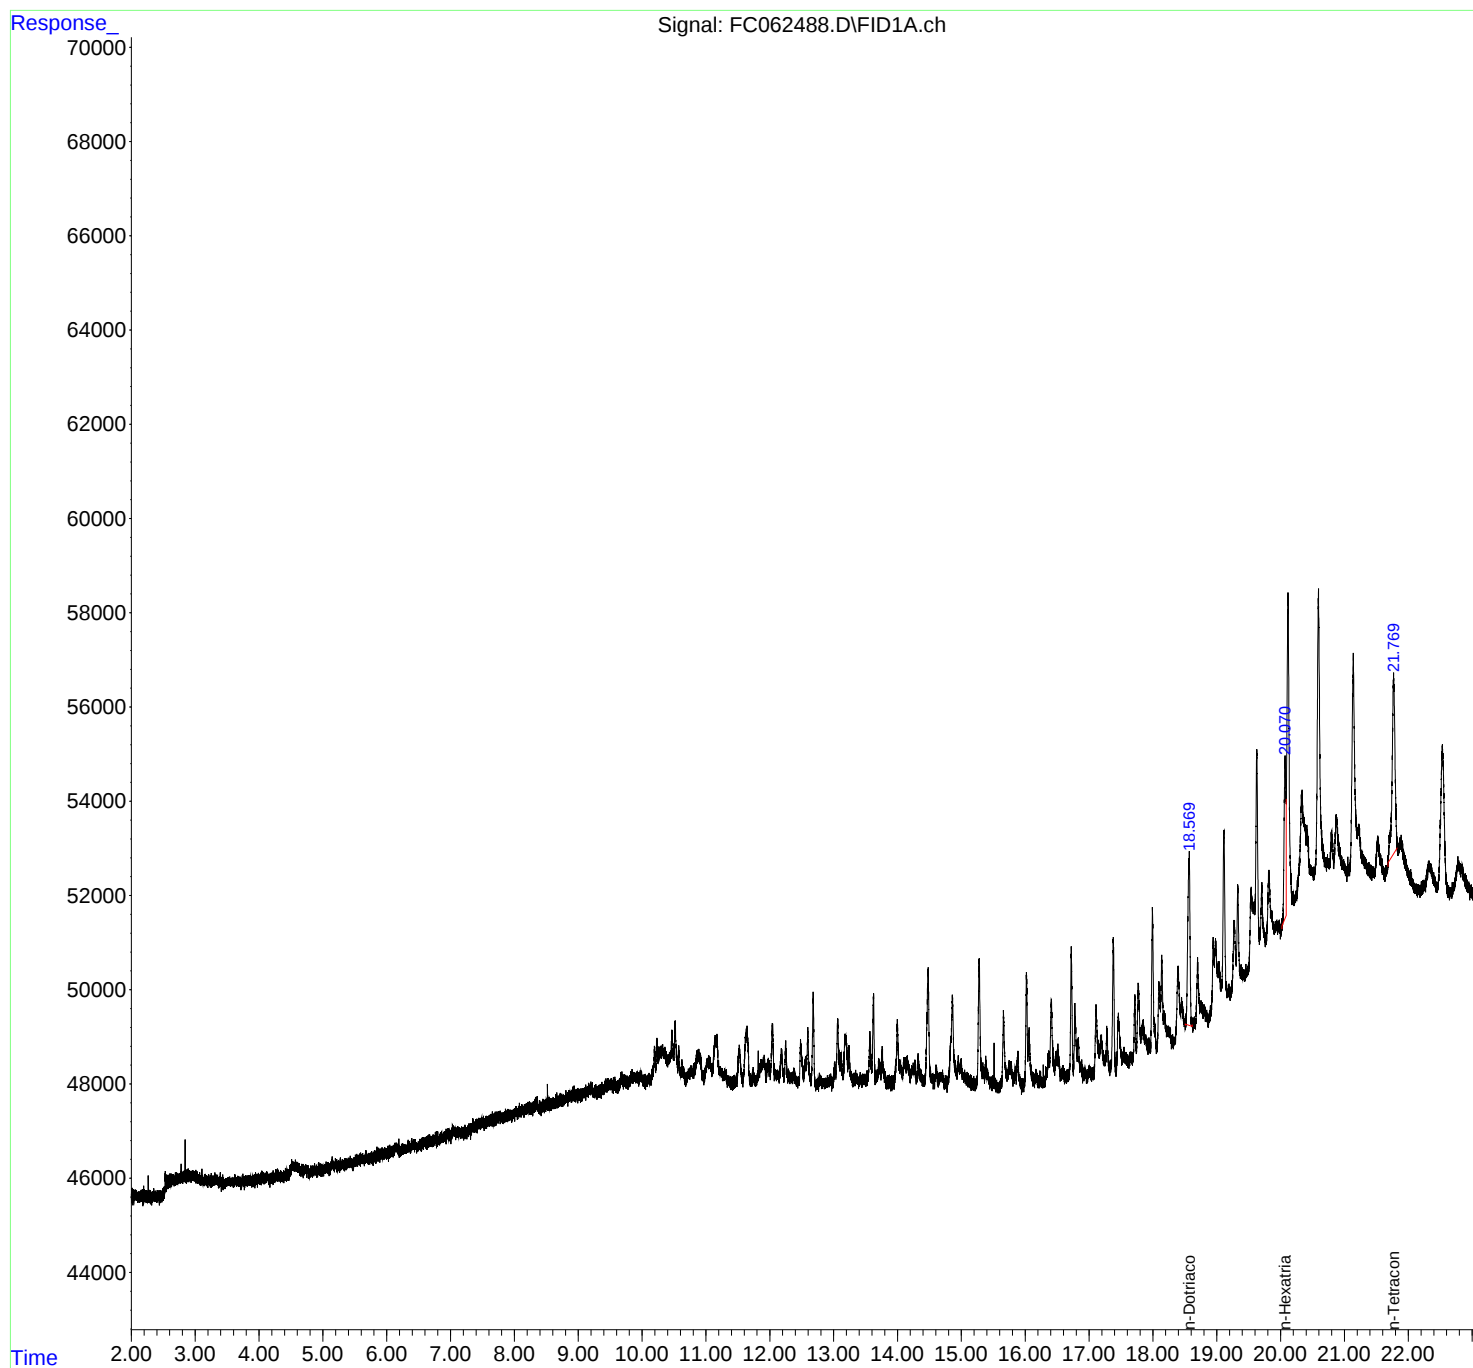


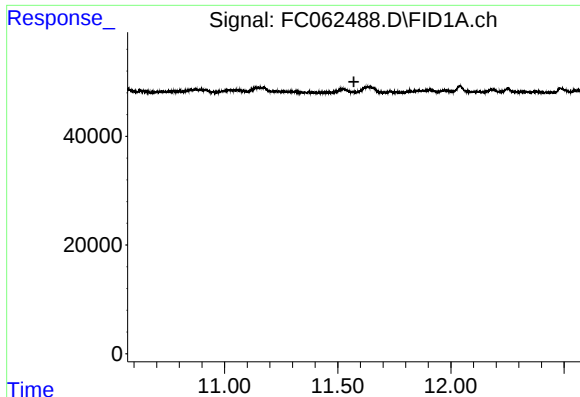

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.571 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

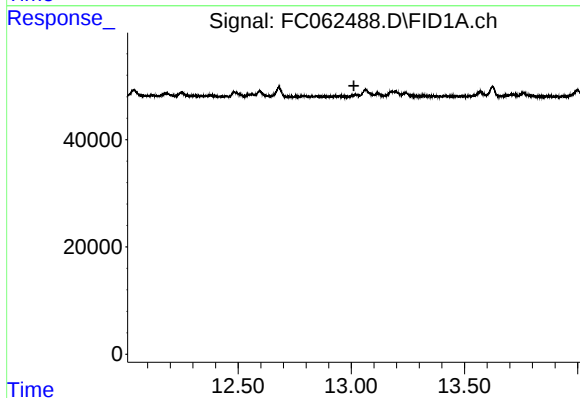


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.011 min
Response: 0
Conc: N.D.

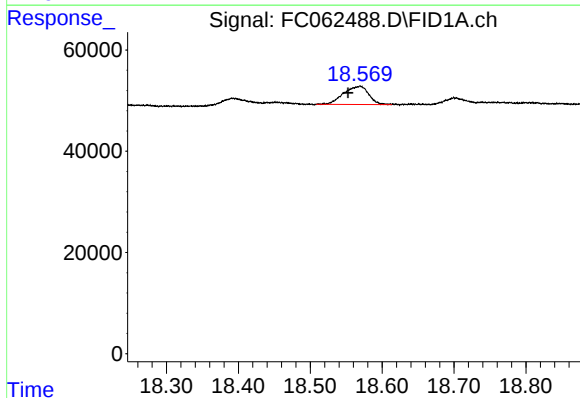


#18 n-Dotriacontane (C32)

R.T.: 18.569 min
Delta R.T.: 0.017 min
Response: 86865
Conc: 0.78 ug/ml

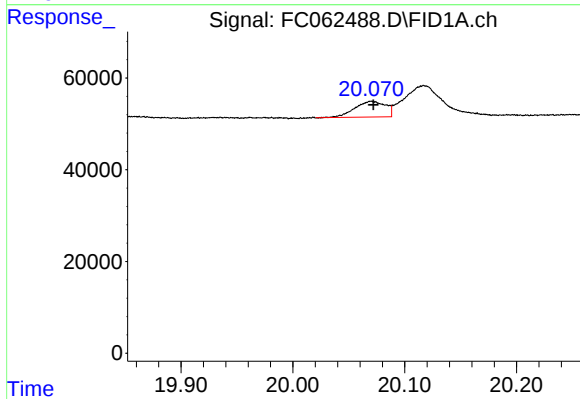

#20 n-Hexatriacontane (C36)

R.T.: 20.070 min
Delta R.T.: -0.002 min
Response: 65130
Conc: 0.64 ug/ml

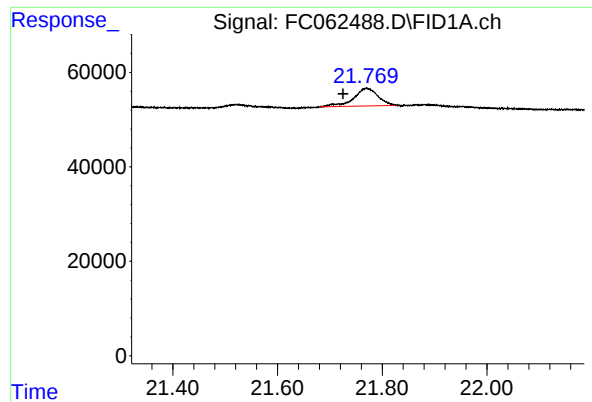

#22 n-Tetracontane (C40)

R.T.: 21.771 min
Delta R.T.: 0.045 min
Response: 120648
Conc: 1.19 ug/ml

Instrument :
FID_C
ClientSampleId :