

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC122922AL\
 Data File : FC062514.D
 Signal(s) : FID1A.ch
 Acq On : 29 Dec 2022 17:27
 Operator : YP/AJ
 Sample : N6231-01D
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 30 06:00:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 120722.M
 Quant Title : GC Extractables
 QLast Update : Thu Dec 08 01:05:24 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.569	3608705	25.582 ug/ml
Spiked Amount 50.000		Recovery =	51.16%
12) S 1-chlorooctadecane (S...	13.007	2761077	25.905 ug/ml
Spiked Amount 50.000		Recovery =	51.81%
Target Compounds			
17) T n-Tricontane (C30)	17.713	52669	0.471 ug/ml
18) T n-Dotriacontane (C32)	18.543	78920	0.710 ug/ml
19) T n-Tetratriacontane (C34)	19.327	47998	0.444 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC122922AL\
Data File : FC062514.D
Signal(s) : FID1A.ch
Acq On : 29 Dec 2022 17:27
Operator : YP/AJ
Sample : N6231-01D
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 30 06:00:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 120722.M
Quant Title : GC Extractables
QLast Update : Thu Dec 08 01:05:24 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

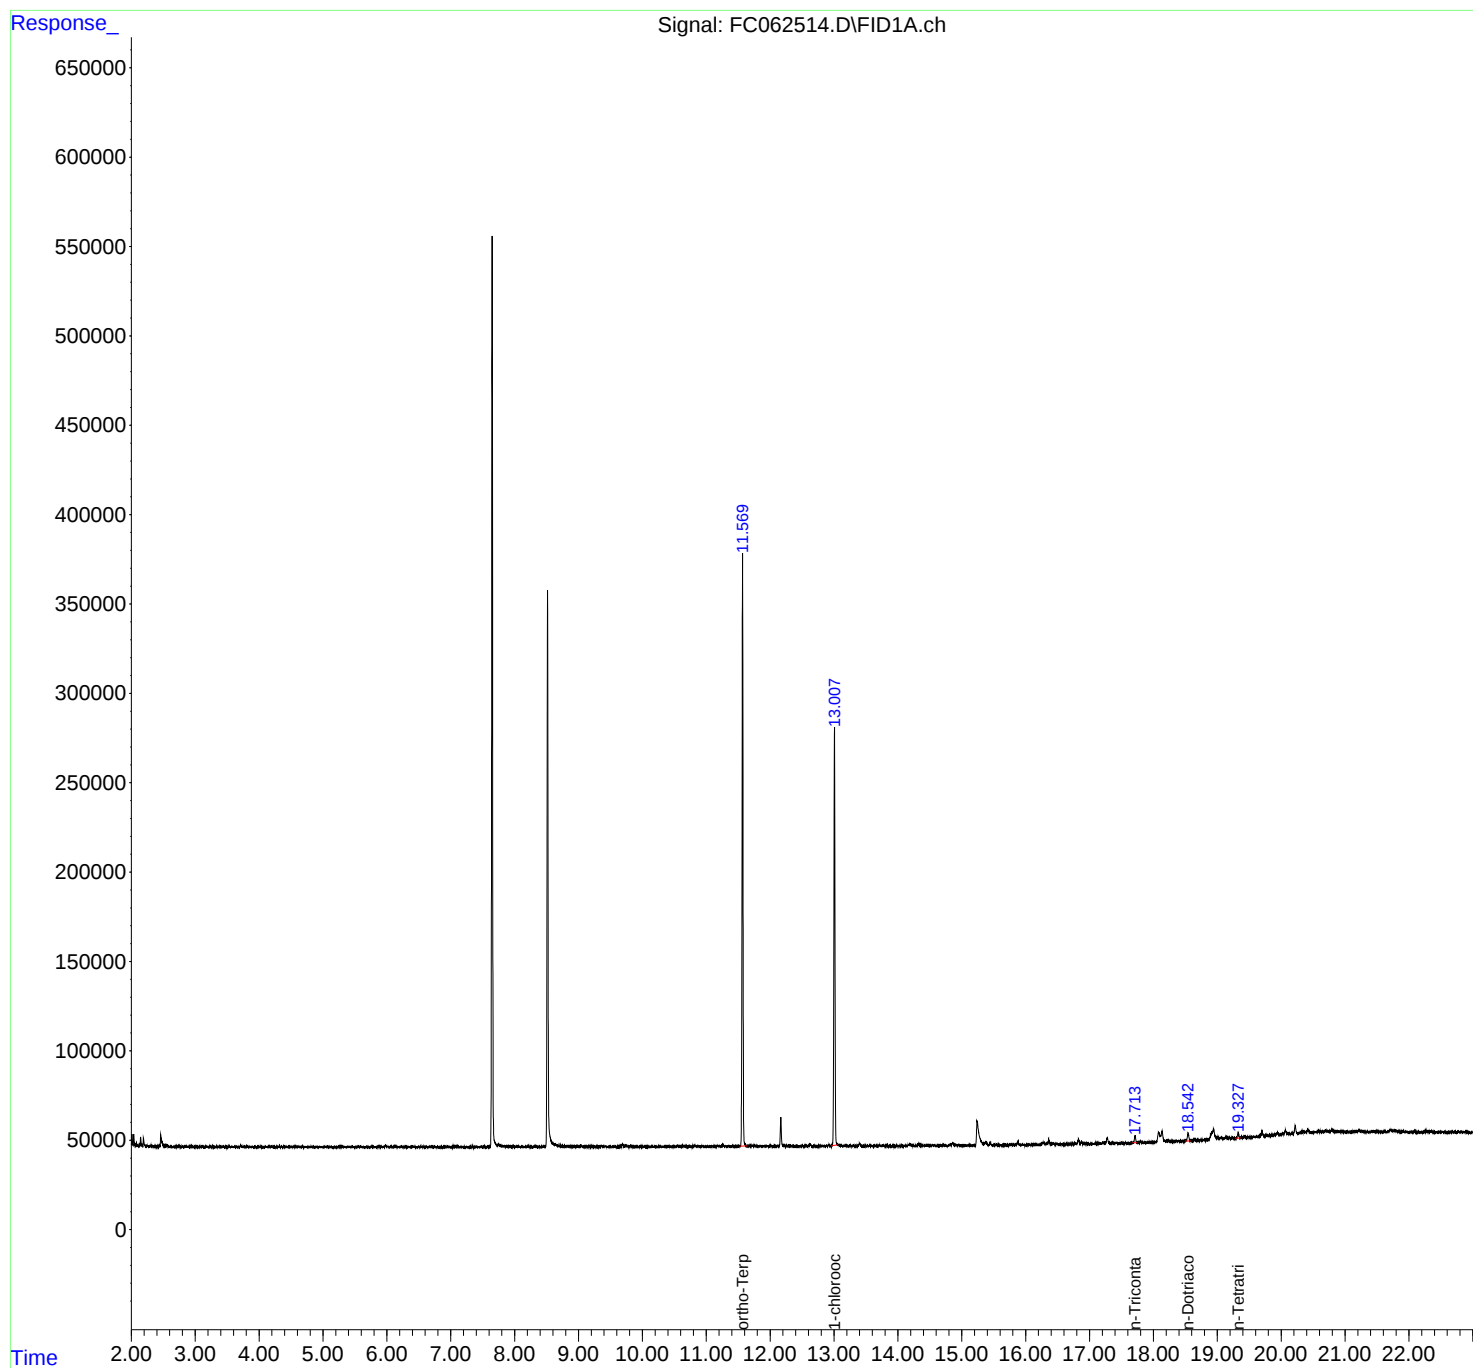


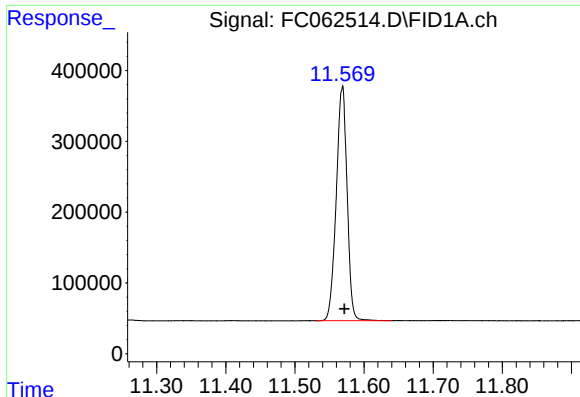

#9 ortho-Terphenyl (SURR)


R.T.: 11.569 min
Delta R.T.: -0.003 min
Response: 3608705
Conc: 25.58 ug/ml

Instrument :
FID_C
ClientSampleId :

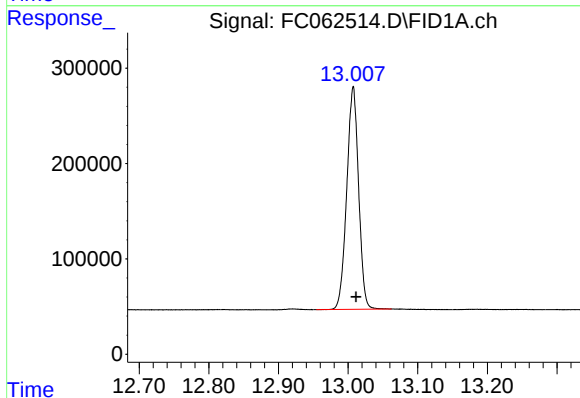


#12 1-chlorooctadecane (SURR)

R.T.: 13.007 min
Delta R.T.: -0.004 min
Response: 2761077
Conc: 25.91 ug/ml

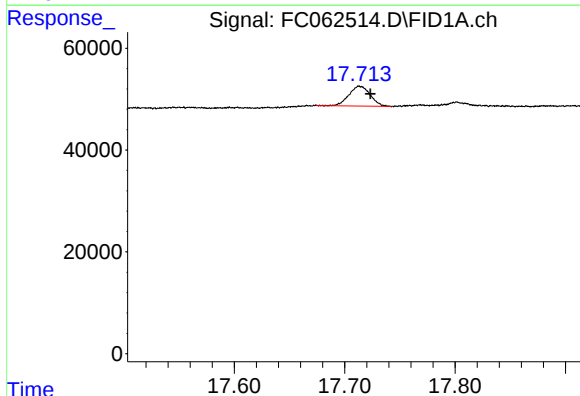


#17 n-Tricontane (C30)

R.T.: 17.713 min
Delta R.T.: -0.010 min
Response: 52669
Conc: 0.47 ug/ml

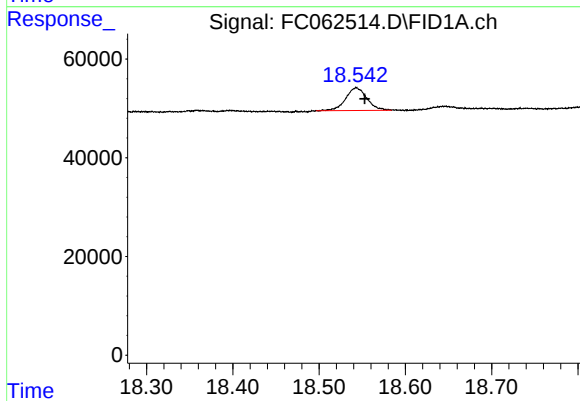

#18 n-Dotriacontane (C32)

R.T.: 18.543 min
Delta R.T.: -0.010 min
Response: 78920
Conc: 0.71 ug/ml

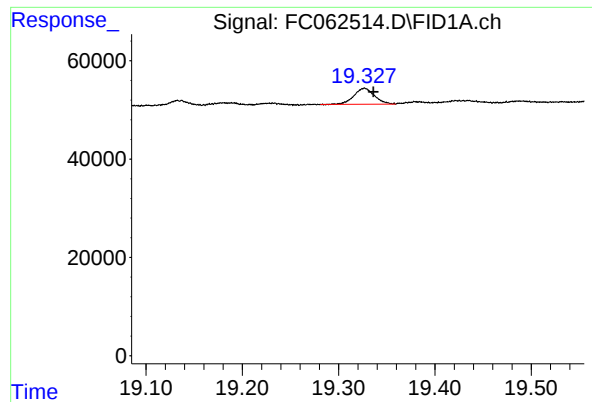

#19 n-Tetratriacontane (C34)

R.T.: 19.327 min
Delta R.T.: -0.009 min
Response: 47998
Conc: 0.44 ug/ml

Instrument :

FID_C

ClientSampleId :