

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD010322AL\
 Data File : FD040382.D
 Signal(s) : FID2B.CH
 Acq On : 04 Jan 2022 8:28
 Operator : AJ\MA
 Sample : M5340-01DL 5X
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :
 BAYSHORE-FILL DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/04/2022
 Supervised By :Ankita Jodhani 01/04/2022

Integration File: autoint1.e
 Quant Time: Jan 04 09:02:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 122821.M
 Quant Title : GC Extractables
 QLast Update : Wed Dec 29 02:26:30 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.672	1076215	6.908 ug/mlm
Spiked Amount 50.000		Recovery =	13.82%
12) S 1-chlorooctadecane (S...	12.107	875293	7.258 ug/mlm
Spiked Amount 50.000		Recovery =	14.52%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD010322AL\
Data File : FD040382.D
Signal(s) : FID2B.CH
Acq On : 04 Jan 2022 8:28
Operator : AJ\MA
Sample : M5340-01DL 5X
Misc :
ALS Vial : 76 Sample Multiplier: 1


Instrument :
FID_D
ClientSampleId :
BAYSHORE-FILL DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/04/2022
Supervised By :Ankita Jodhani 01/04/2022

Integration File: autoint1.e
Quant Time: Jan 04 09:02:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 122821.M
Quant Title : GC Extractables
QLast Update : Wed Dec 29 02:26:30 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

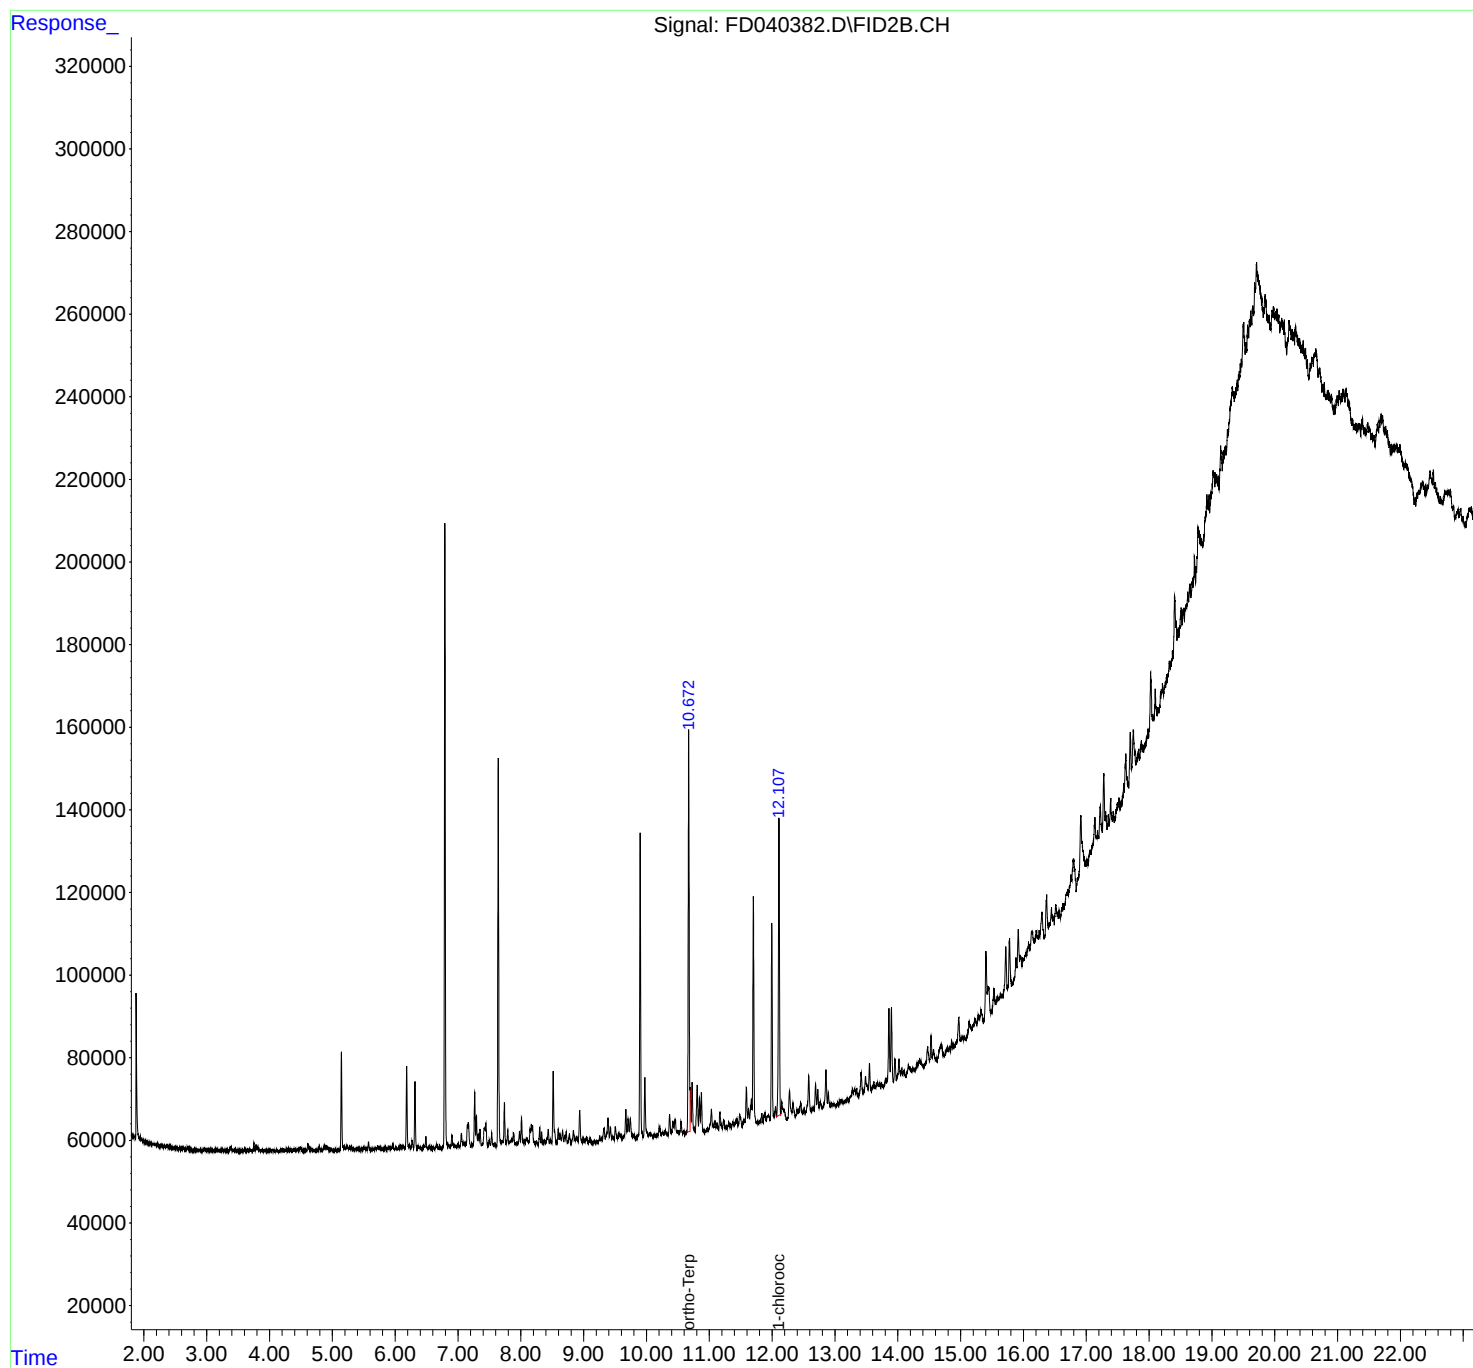

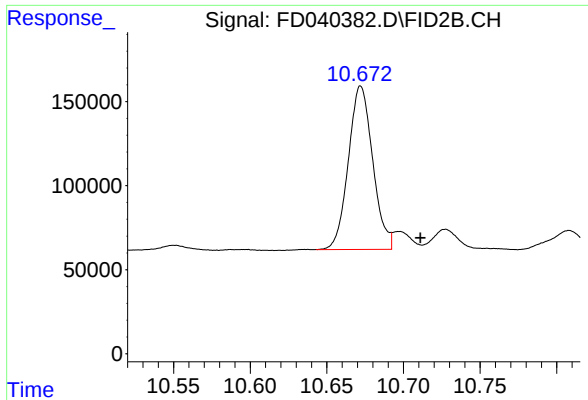


#9 ortho-Terphenyl (SURR)

R.T.: 10.672 min
Delta R.T.: -0.039 min
Response: 1076215
Conc: 6.91 ug/ml

Instrument :
FID_D
ClientSampleId :
BAYSHORE-FILL DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/04/2022
Supervised By :Ankita Jodhani 01/04/2022

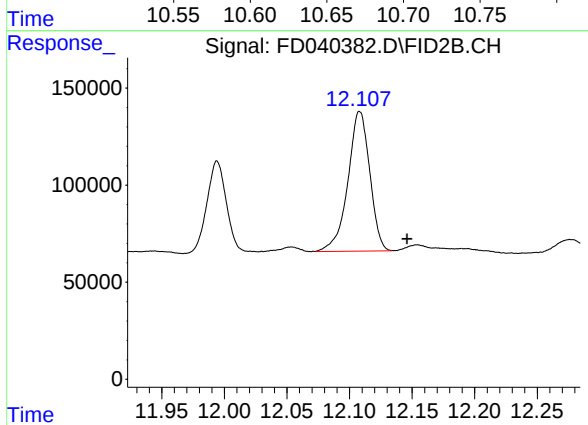

#12 1-chlorooctadecane (SURR)

R.T.: 12.107 min
Delta R.T.: -0.039 min
Response: 875293
Conc: 7.26 ug/ml m