

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD010422AL\
 Data File : FD040422.D
 Signal(s) : FID2B.CH
 Acq On : 05 Jan 2022 12:20
 Operator : AJ\MA
 Sample : N1004-01D
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :
 RO-R2-IEC

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/05/2022
 Supervised By :Ankita Jodhani 01/05/2022

Integration File: autoint1.e
 Quant Time: Jan 05 12:45:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 010422.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 07:08:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.635	8259308	53.566 ug/mlm
Spiked Amount	50.000	Recovery	= 107.13%
12) S 1-chlorooctadecane (S...	12.071	6343297	53.891 ug/mlm
Spiked Amount	50.000	Recovery	= 107.78%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD010422AL\
Data File : FD040422.D
Signal(s) : FID2B.CH
Acq On : 05 Jan 2022 12:20
Operator : AJ\MA
Sample : N1004-01D
Misc :
ALS Vial : 71 Sample Multiplier: 1


Instrument :
FID_D
ClientSampleId :
RO-R2-IEC


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/05/2022
Supervised By :Ankita Jodhani 01/05/2022

Integration File: autoint1.e
Quant Time: Jan 05 12:45:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 010422.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 07:08:39 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

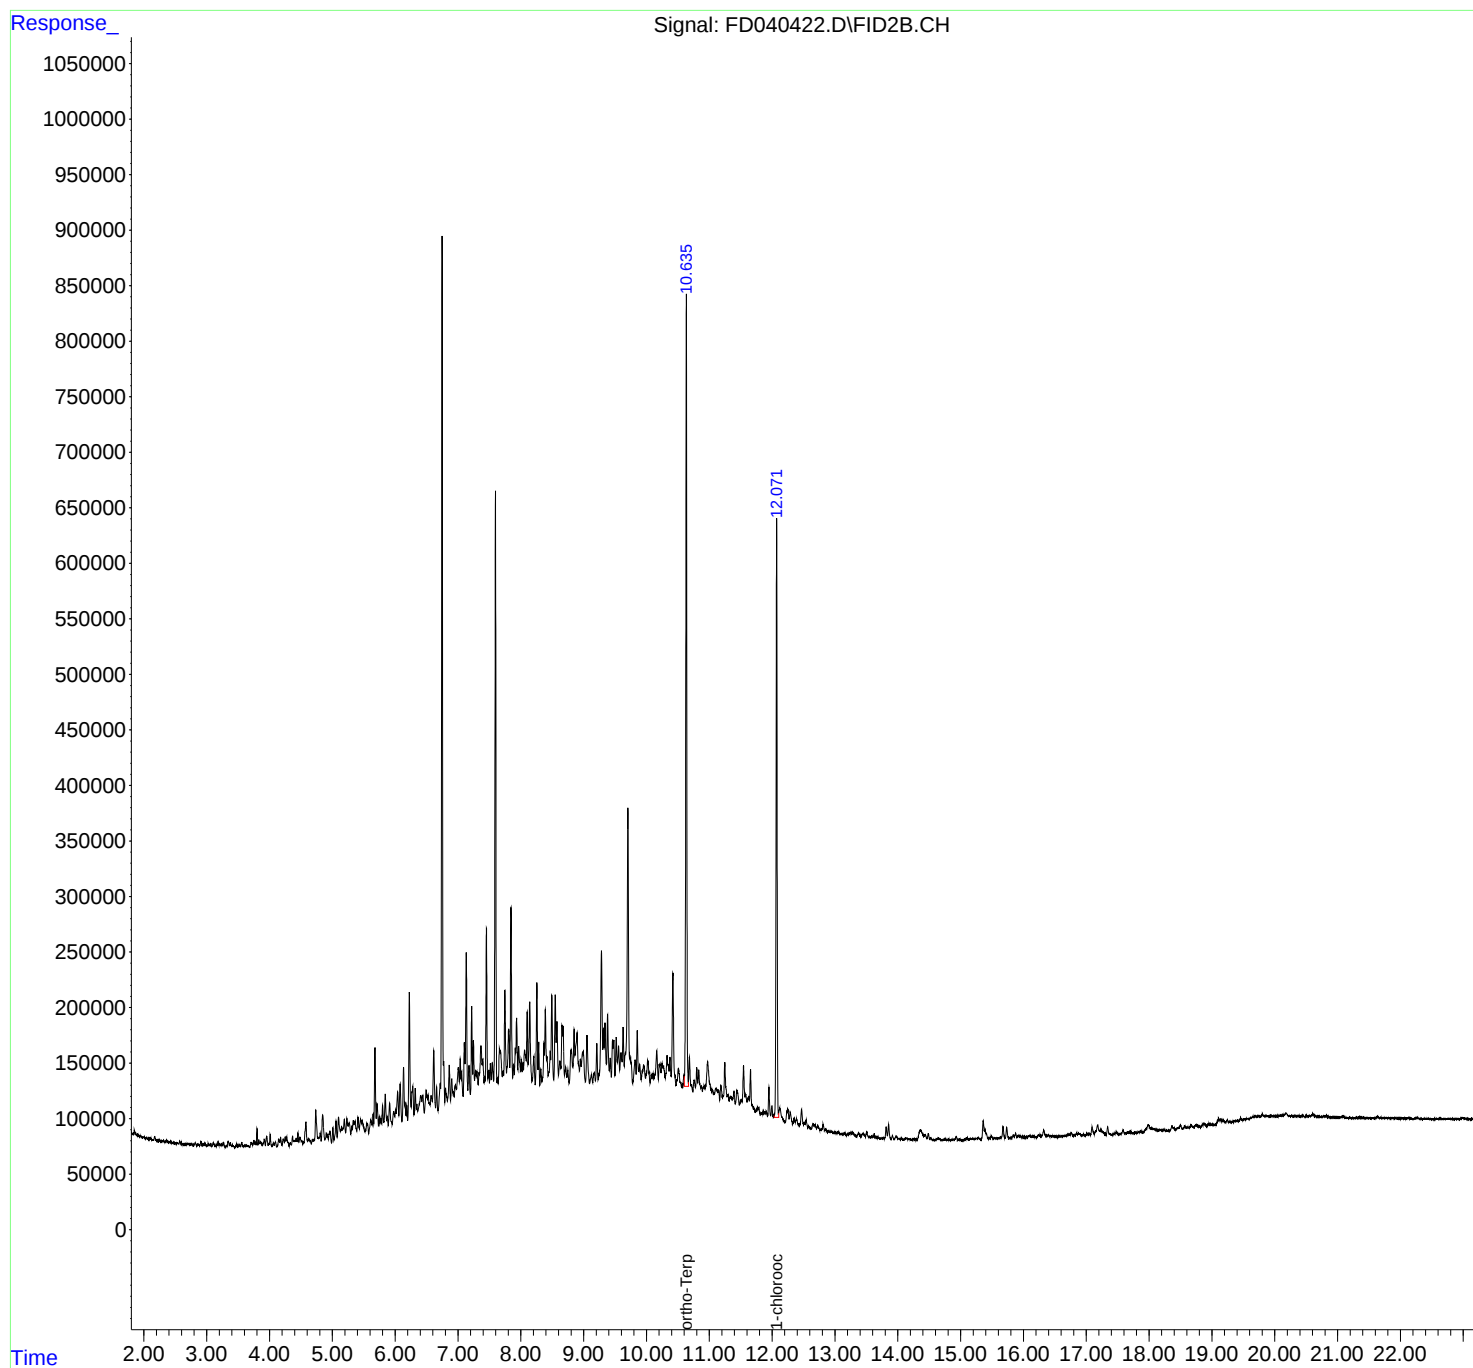

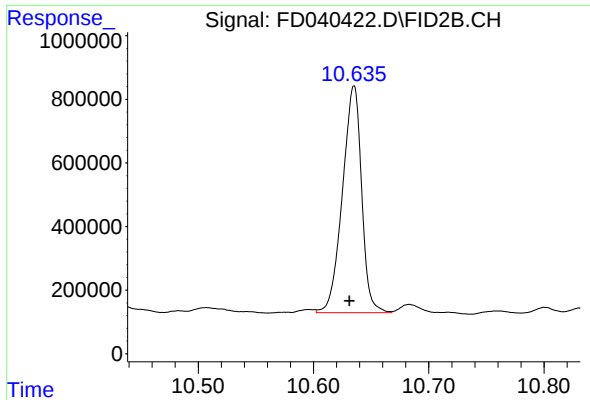


#9 ortho-Terphenyl (SURR)

R.T.: 10.635 min
Delta R.T.: 0.004 min
Response: 8259308
Conc: 53.57 ug/ml

Instrument :
FID_D
ClientSampleId :
RO-R2-IEC

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/05/2022
Supervised By :Ankita Jodhani 01/05/2022

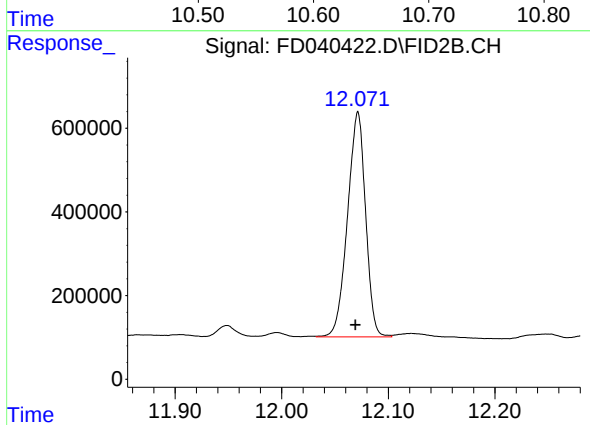

#12 1-chlorooctadecane (SURR)

R.T.: 12.071 min
Delta R.T.: 0.002 min
Response: 6343297
Conc: 53.89 ug/ml m