

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD010622AL\
 Data File : FD040464.D
 Signal(s) : FID2B.CH
 Acq On : 06 Jan 2022 13:05
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 07 00:43:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 010422.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 05 07:08:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

13) T	n-Docosane (C22)	12.772	53260	0.386 ug/ml
14) T	n-Tetracosane (C24)	13.913	46624	0.333 ug/ml
15) T	n-Hexacosane (C26)	14.928	52097	0.378 ug/ml
16) T	n-Octacosane (C28)	15.872	63783	0.470 ug/ml
17) T	n-Tricontane (C30)	16.755	85912	0.659 ug/ml
18) T	n-Dotriacontane (C32)	17.584	73077	0.611 ug/ml
19) T	n-Tetratriacontane (C34)	18.361	46646	0.443 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD010622AL\
Data File : FD040464.D
Signal(s) : FID2B.CH
Acq On : 06 Jan 2022 13:05
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 07 00:43:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 010422.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 07:08:39 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

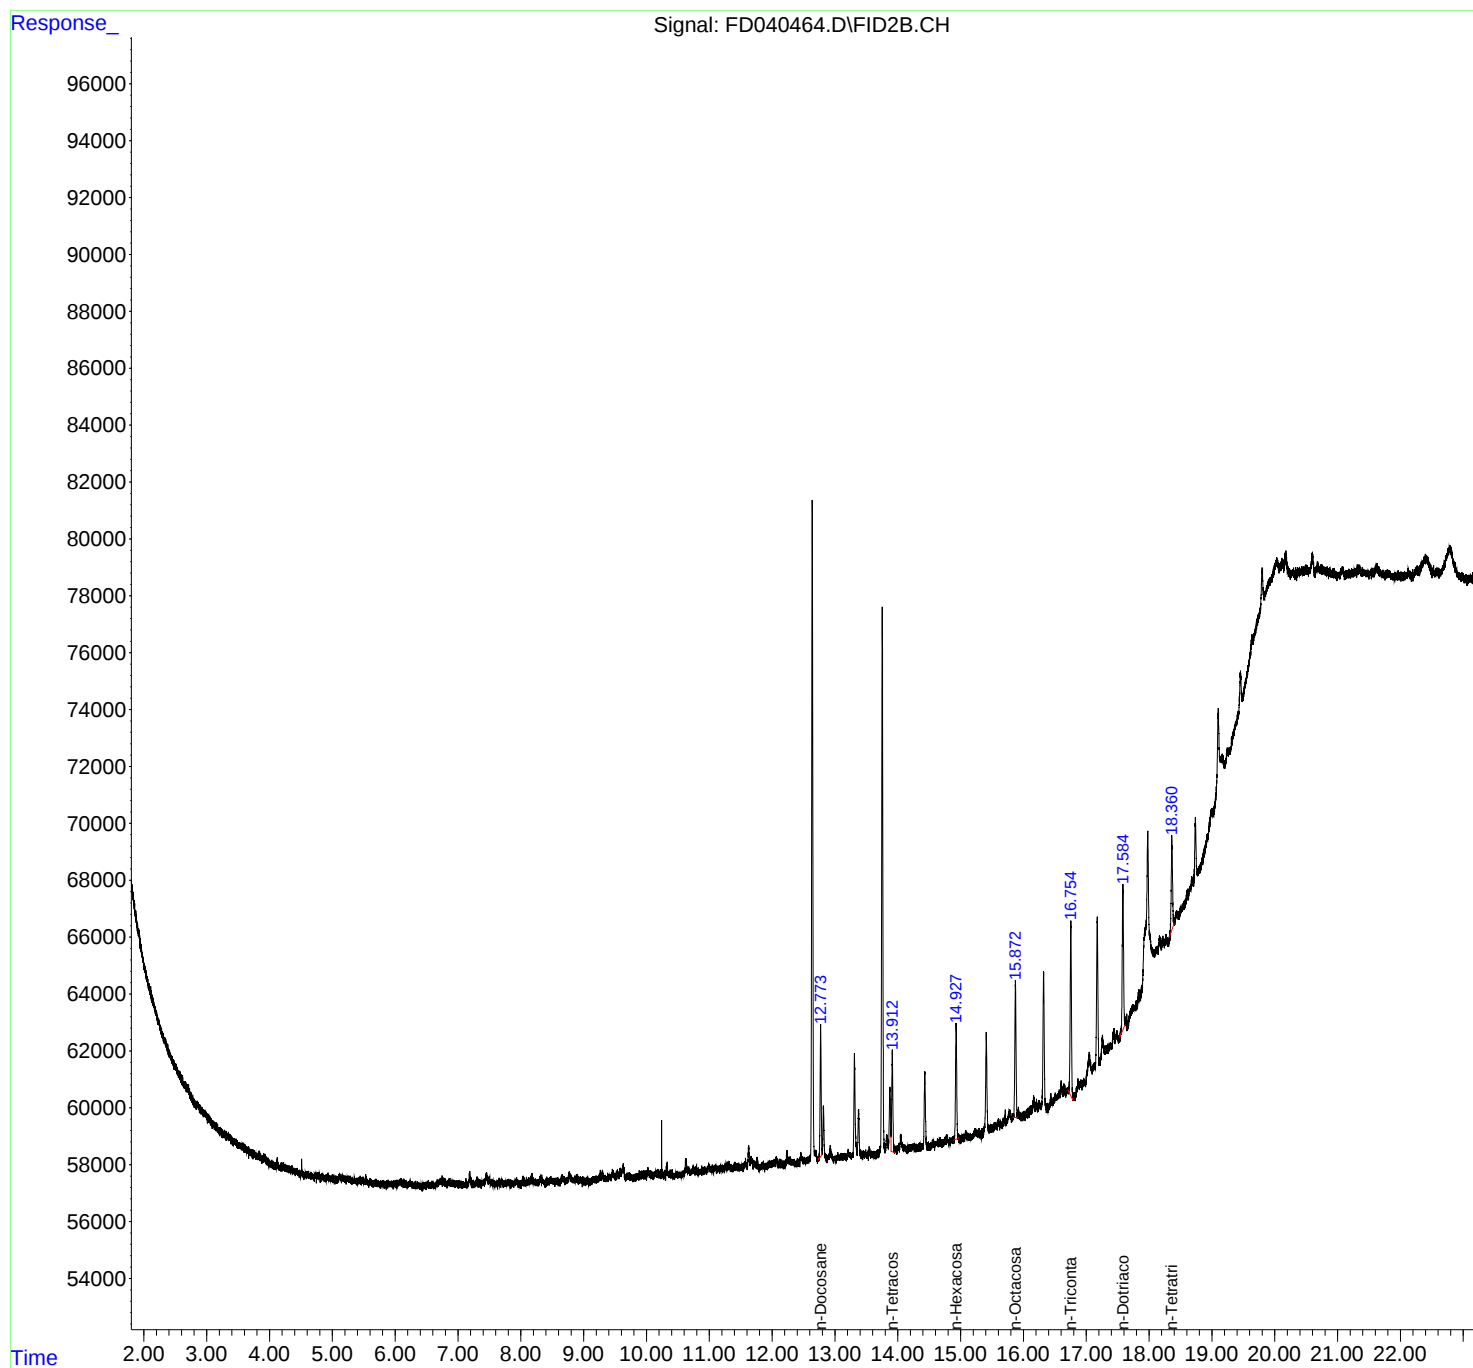


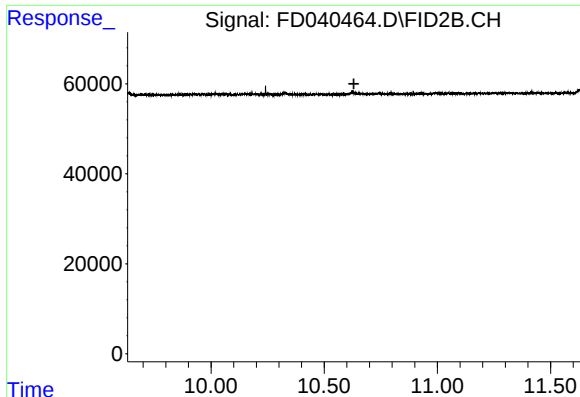

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.631 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

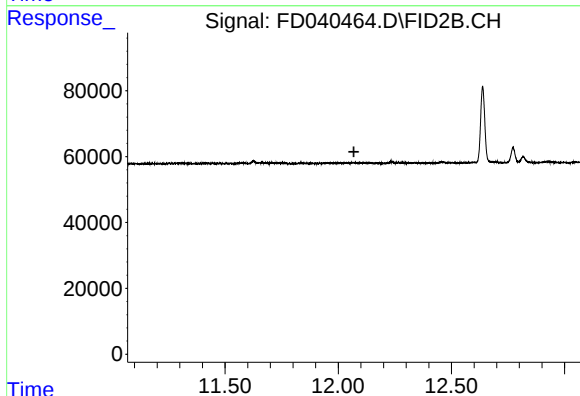


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.069 min
Response: 0
Conc: N.D.

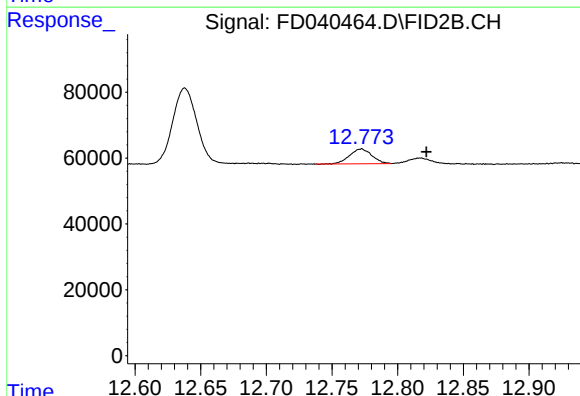


#13 n-Docosane (C22)

R.T.: 12.772 min
Delta R.T.: -0.050 min
Response: 53260
Conc: 0.39 ug/ml

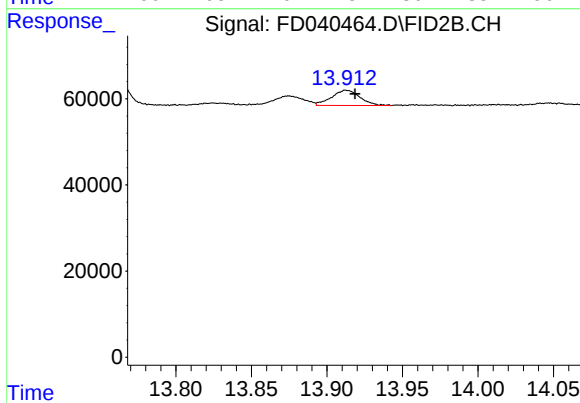

#14 n-Tetracosane (C24)


R.T.: 13.913 min
Delta R.T.: -0.006 min
Response: 46624
Conc: 0.33 ug/ml

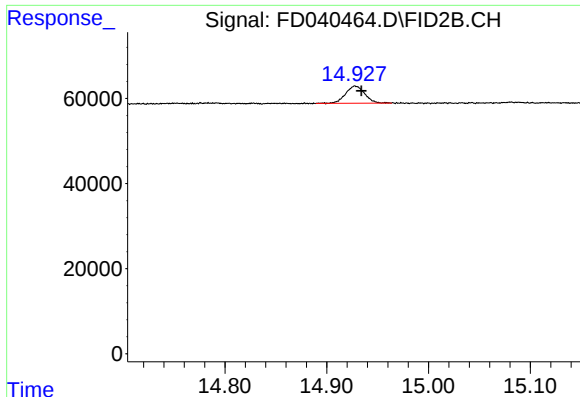

#15 n-Hexacosane (C26)


R.T.: 14.928 min
Delta R.T.: -0.006 min
Response: 52097
Conc: 0.38 ug/ml

Instrument :
FID_D
ClientSampleId :

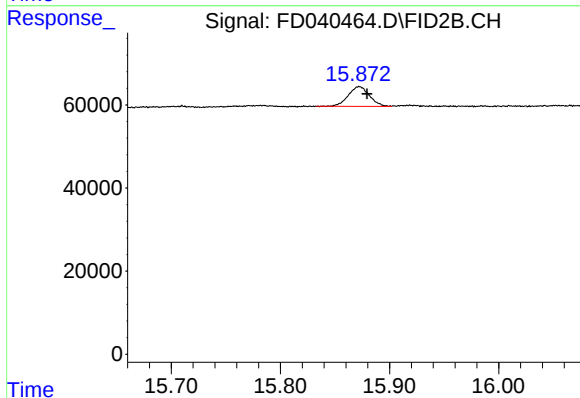


#16 n-Octacosane (C28)

R.T.: 15.872 min
Delta R.T.: -0.007 min
Response: 63783
Conc: 0.47 ug/ml

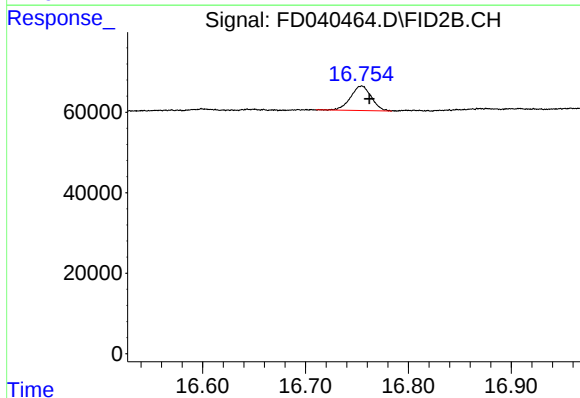


#17 n-Tricontane (C30)

R.T.: 16.755 min
Delta R.T.: -0.008 min
Response: 85912
Conc: 0.66 ug/ml

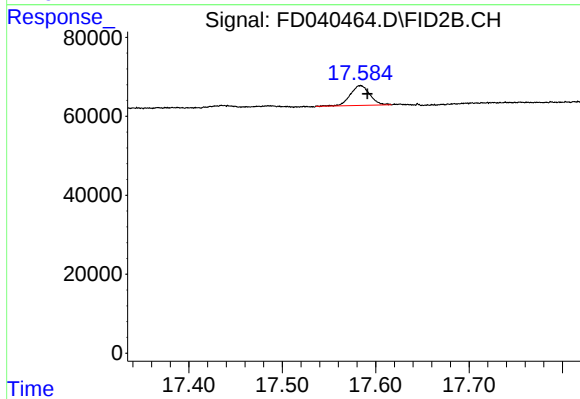

#18 n-Dotriacontane (C32)

R.T.: 17.584 min
Delta R.T.: -0.007 min
Response: 73077
Conc: 0.61 ug/ml

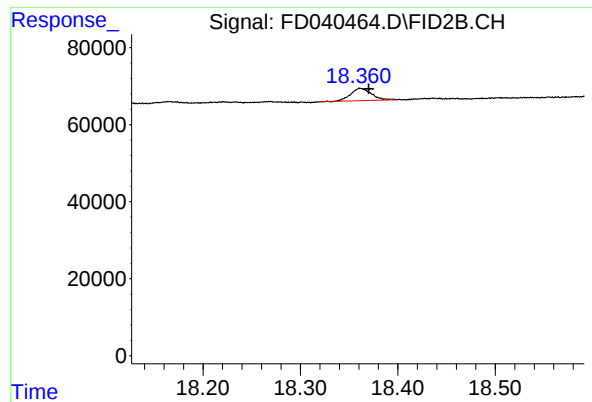

#19 n-Tetratriacontane (C34)

R.T.: 18.361 min
Delta R.T.: -0.009 min
Response: 46646
Conc: 0.44 ug/ml

Instrument :

FID_D

ClientSampleId :