

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD010622AL\
Data File : FD040471.D
Signal(s) : FID2B.CH
Acq On : 06 Jan 2022 17:36
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 07 00:46:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 010422.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 07:08:39 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

13) T	n-Docosane (C22)	12.768f	58568	0.425 ug/ml
14) T	n-Tetracosane (C24)	13.909	50541	0.361 ug/ml
15) T	n-Hexacosane (C26)	14.925	58191	0.422 ug/ml
16) T	n-Octacosane (C28)	15.869	69112	0.509 ug/ml
17) T	n-Tricontane (C30)	16.752	89139	0.684 ug/ml
18) T	n-Dotriacontane (C32)	17.580	74233	0.621 ug/ml
19) T	n-Tetratriacontane (C34)	18.360	47166	0.448 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD010622AL\
Data File : FD040471.D
Signal(s) : FID2B.CH
Acq On : 06 Jan 2022 17:36
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 07 00:46:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 010422.M
Quant Title : GC Extractables
QLast Update : Wed Jan 05 07:08:39 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

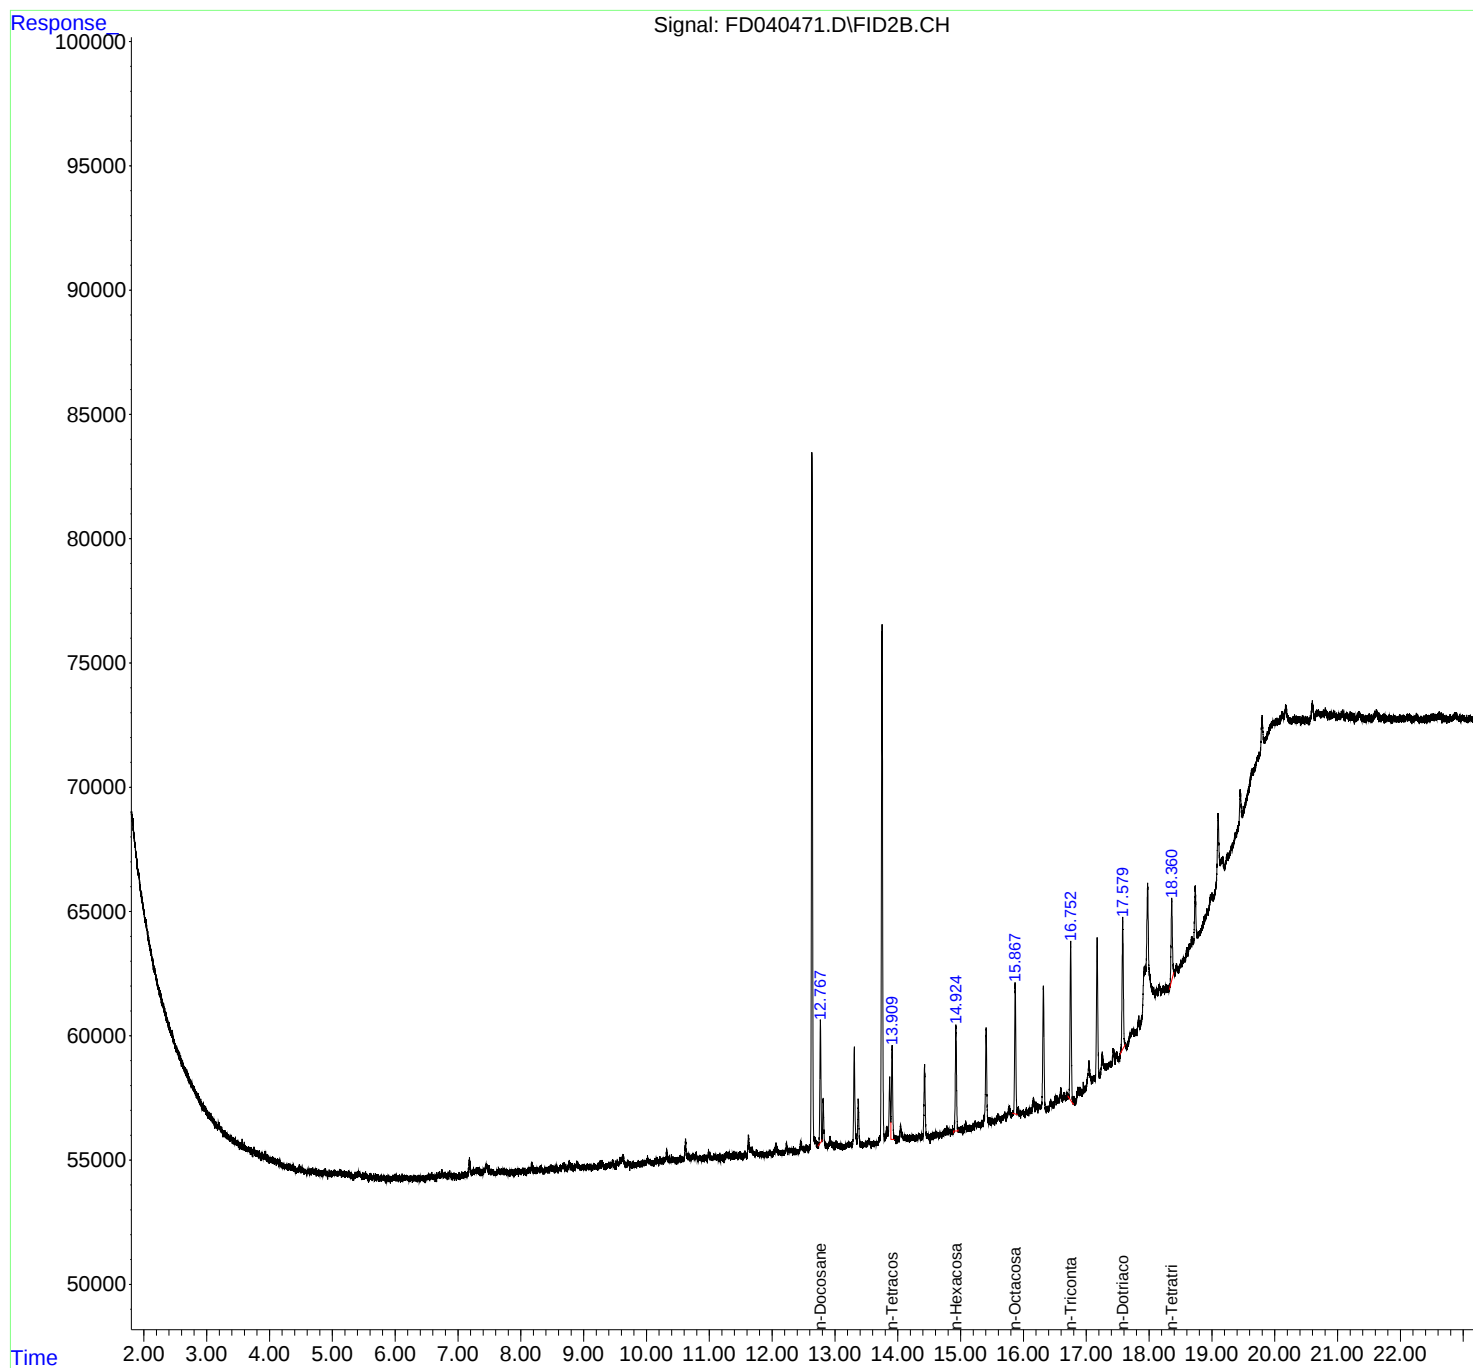


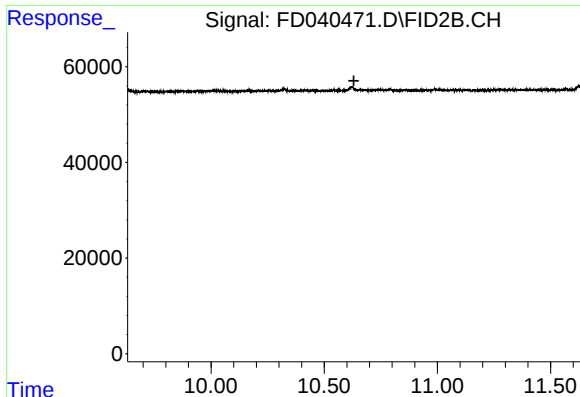

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.631 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

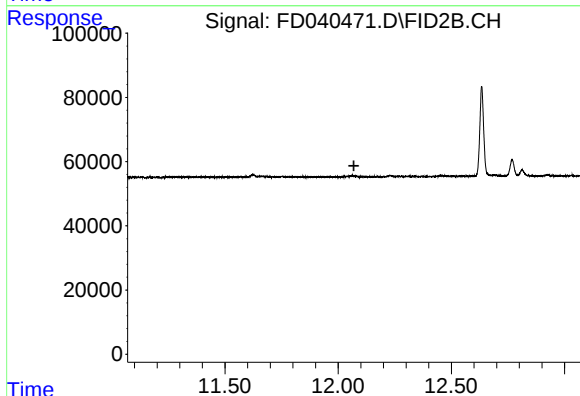


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.069 min
Response: 0
Conc: N.D.

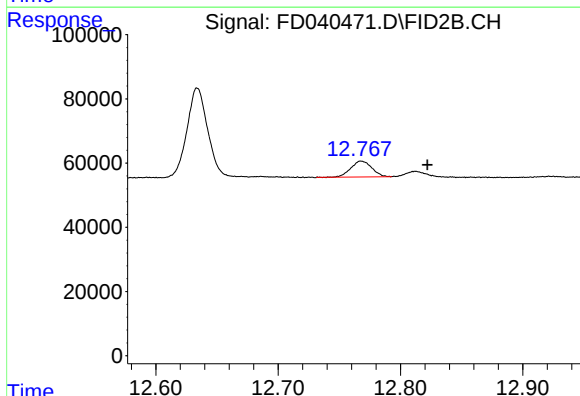


#13 n-Docosane (C22)

R.T.: 12.768 min
Delta R.T.: -0.054 min
Response: 58568
Conc: 0.42 ug/ml

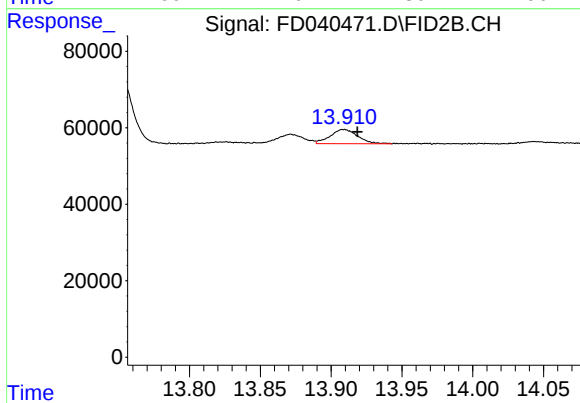

#14 n-Tetracosane (C24)


R.T.: 13.909 min
Delta R.T.: -0.010 min
Response: 50541
Conc: 0.36 ug/ml

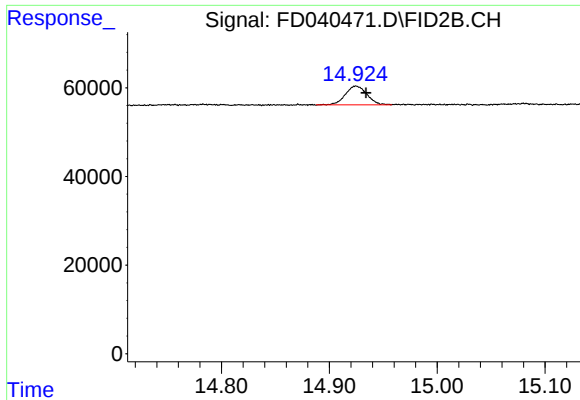

#15 n-Hexacosane (C26)


R.T.: 14.925 min
Delta R.T.: -0.009 min
Response: 58191
Conc: 0.42 ug/ml

Instrument :
FID_D
ClientSampleId :

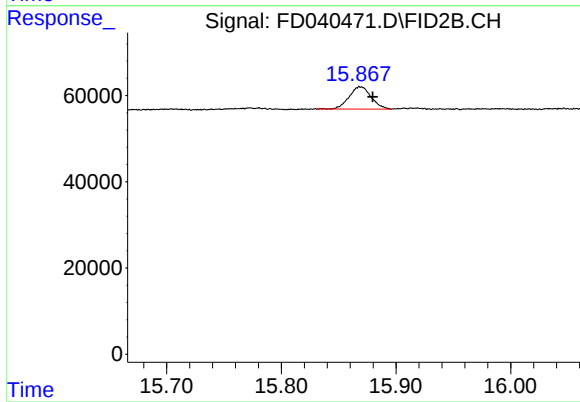


#16 n-Octacosane (C28)

R.T.: 15.869 min
Delta R.T.: -0.011 min
Response: 69112
Conc: 0.51 ug/ml

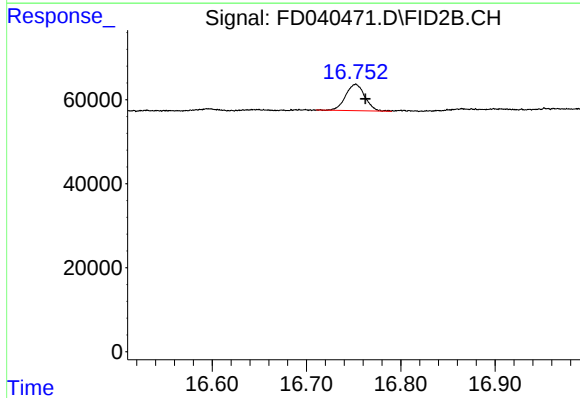


#17 n-Tricontane (C30)

R.T.: 16.752 min
Delta R.T.: -0.010 min
Response: 89139
Conc: 0.68 ug/ml

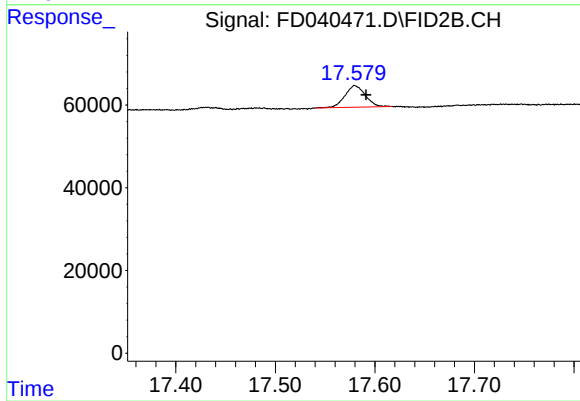

#18 n-Dotriacontane (C32)

R.T.: 17.580 min
Delta R.T.: -0.011 min
Response: 74233
Conc: 0.62 ug/ml

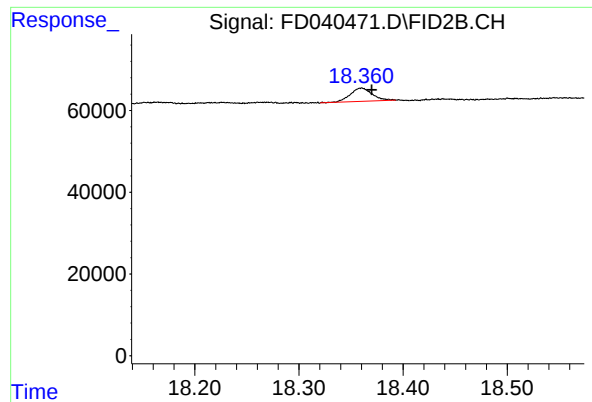

#19 n-Tetratriacontane (C34)

R.T.: 18.360 min
Delta R.T.: -0.010 min
Response: 47166
Conc: 0.45 ug/ml

Instrument :

FID_D

ClientSampleId :