

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD010820AL\
 Data File : FD031979.D
 Signal(s) : FID2B.CH
 Acq On : 09 Jan 2020 00:31
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 09 02:54:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 010620.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 07 01:05:13 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
16) T	n-Octacosane (C28)	16.766	21796 0.171 ug/ml
17) T	n-Tricontane (C30)	17.650	32240 0.263 ug/ml
18) T	n-Dotriacontane (C32)	18.480	24426 0.233 ug/ml
19) T	n-Tetratriacontane (C34)	19.254	29157 0.330 ug/ml
20) T	n-Hexatriacontane (C36)	20.031	34033 0.432 ug/ml
21) T	n-Octatriacontane (C38)	20.703	20941 0.284 ug/ml
22) T	n-Tetracontane (C40)	21.610	66230 0.875 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD010820AL\
Data File : FD031979.D
Signal(s) : FID2B.CH
Acq On : 09 Jan 2020 00:31
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 09 02:54:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 010620.M
Quant Title : GC Extractables
QLast Update : Tue Jan 07 01:05:13 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

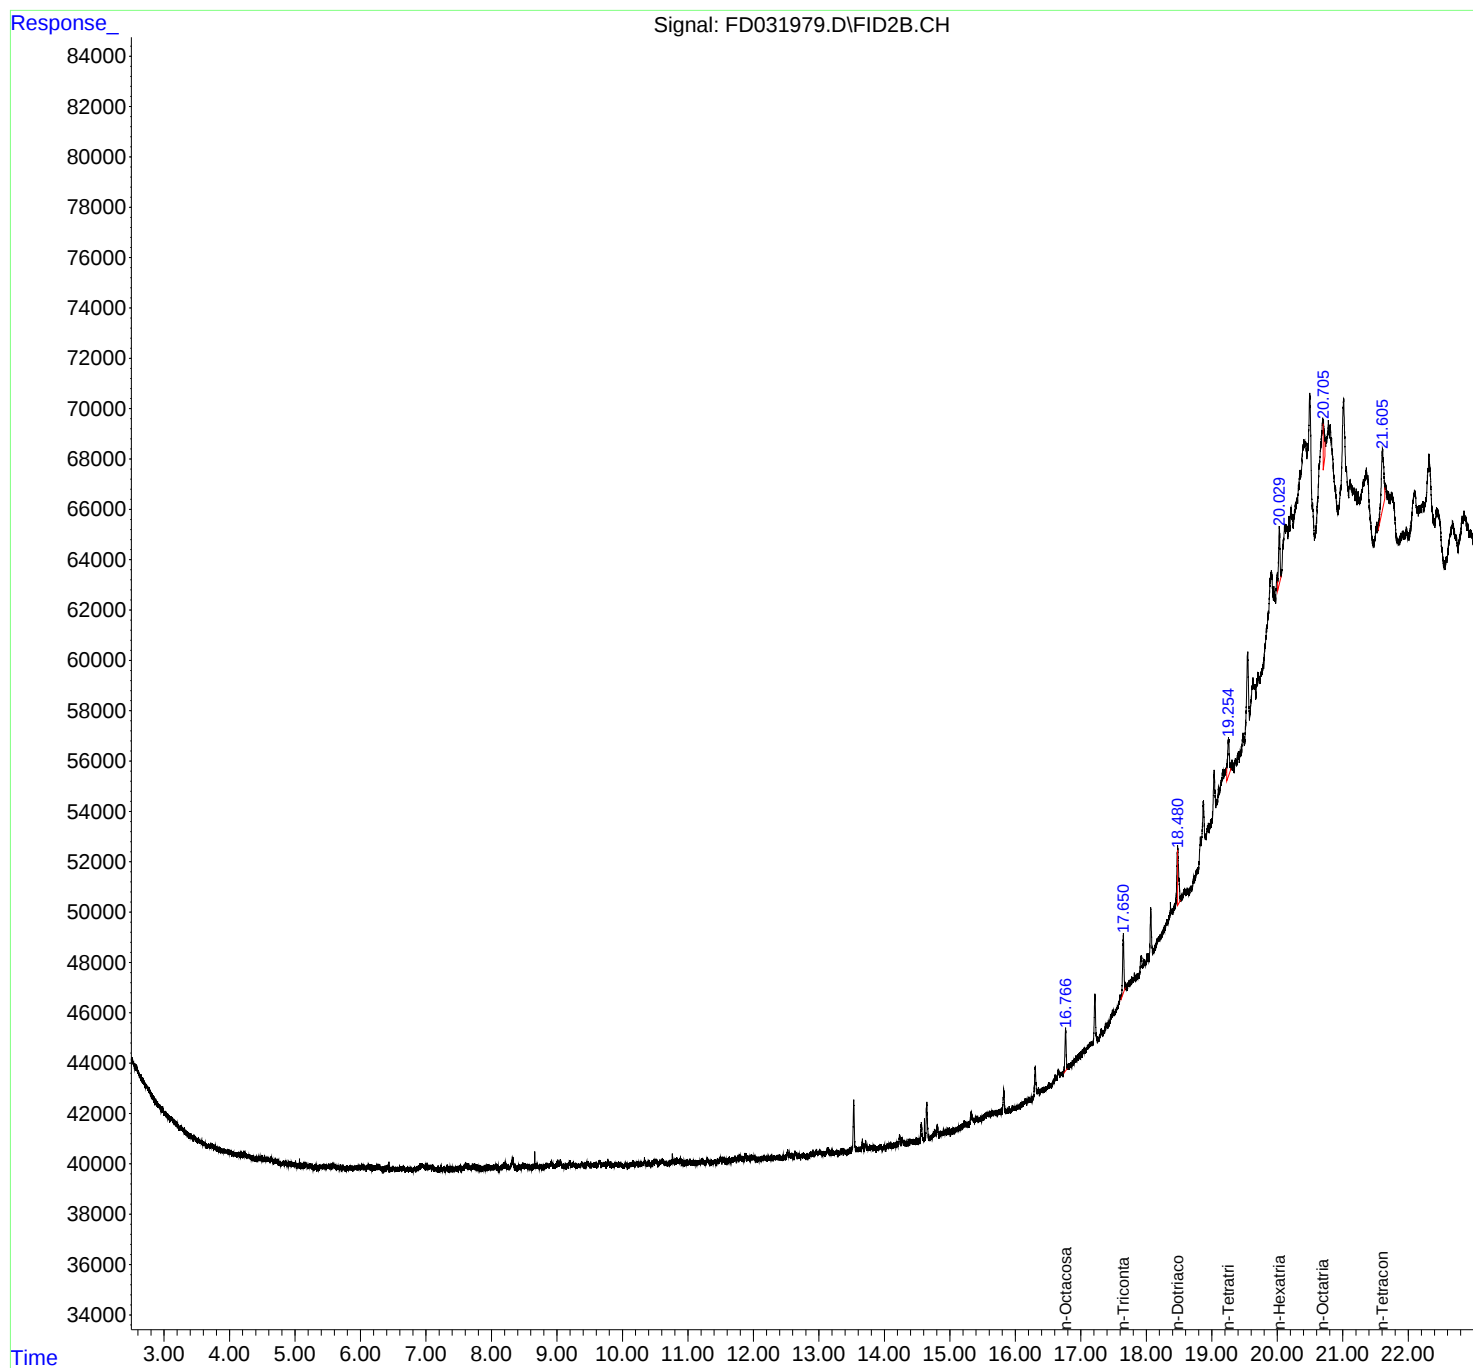

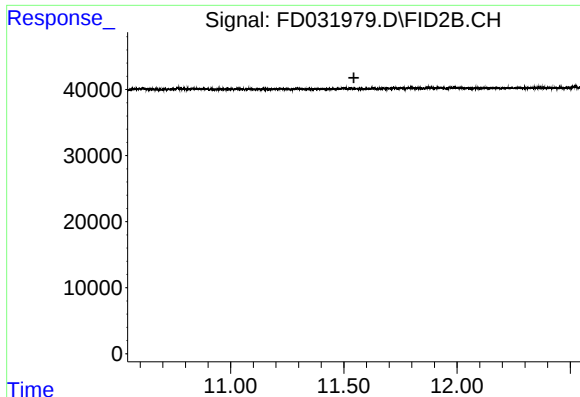


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.544 min
Response: 0
Conc: N.D.

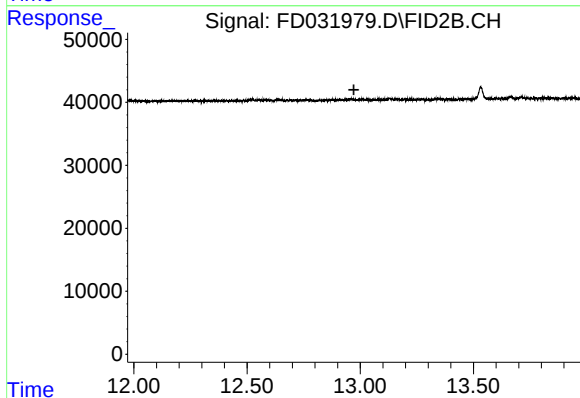


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 12.972 min
Response: 0
Conc: N.D.

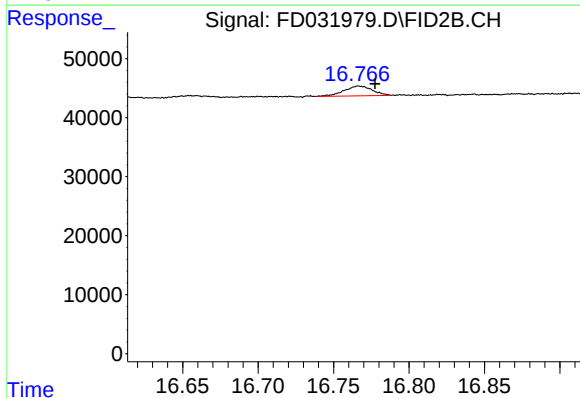


#16 n-Octacosane (C28)

R.T.: 16.766 min
Delta R.T.: -0.011 min
Response: 21796
Conc: 0.17 ug/ml

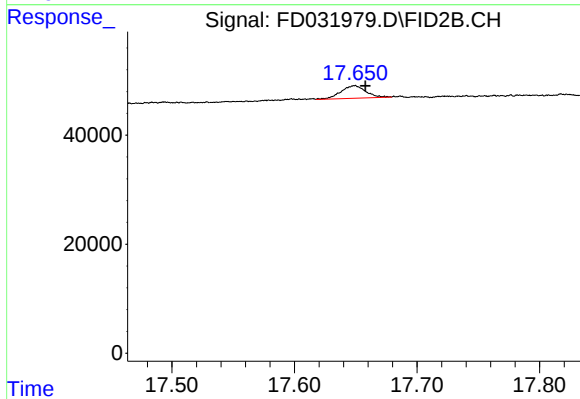


#17 n-Tricontane (C30)

R.T.: 17.650 min
Delta R.T.: -0.008 min
Response: 32240
Conc: 0.26 ug/ml

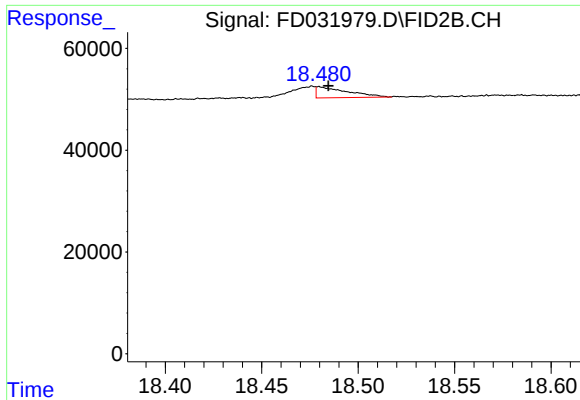


#18 n-Dotriacontane (C32)

R.T.: 18.480 min
Delta R.T.: -0.005 min
Response: 24426
Conc: 0.23 ug/ml

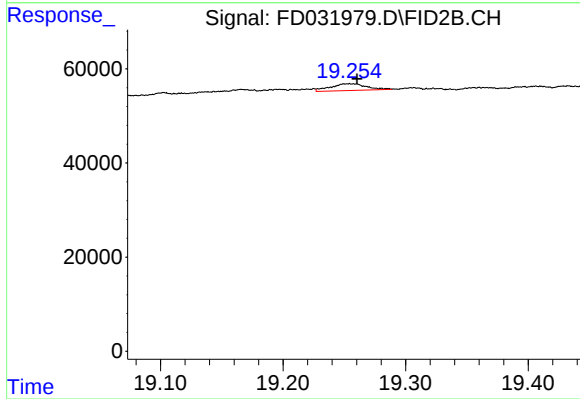


#19 n-Tetratriacontane (C34)

R.T.: 19.254 min
Delta R.T.: -0.006 min
Response: 29157
Conc: 0.33 ug/ml

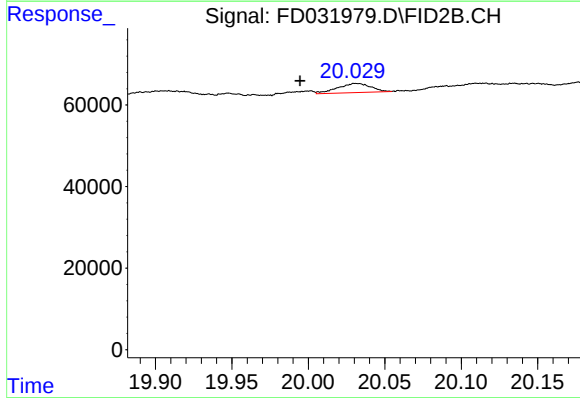


#20 n-Hexatriacontane (C36)

R.T.: 20.031 min
Delta R.T.: 0.036 min
Response: 34033
Conc: 0.43 ug/ml

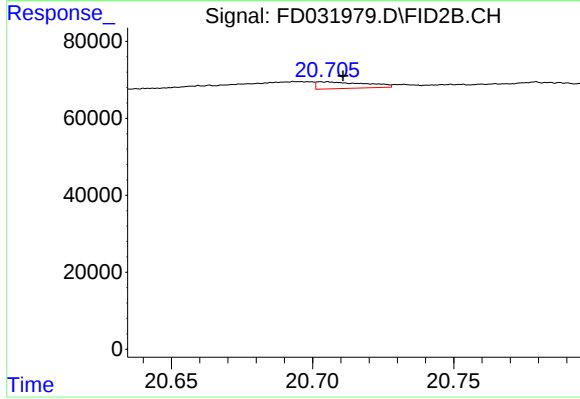

#21 n-Octatriacontane (C38)

R.T.: 20.703 min
Delta R.T.: -0.008 min
Response: 20941
Conc: 0.28 ug/ml

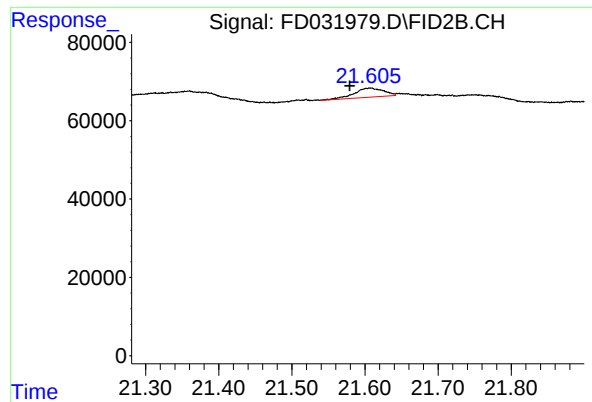

#22 n-Tetracontane (C40)

R.T.: 21.610 min
Delta R.T.: 0.030 min
Response: 66230
Conc: 0.88 ug/ml