

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD012425AR\
Data File : FD048943.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2025 07:37
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 25 03:39:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 012425.M
Quant Title : GC Extractables
QLast Update : Sat Jan 25 03:38:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

18) T	Benzo[a]pyrene (C31.34)	16.398	73869	0.531 ug/ml
19) T	Indeno[1,2,3-cd]pyren...	17.668f	80208	0.769 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD012425AR\
Data File : FD048943.D
Signal(s) : FID2B.ch
Acq On : 24 Jan 2025 07:37
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 25 03:39:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 012425.M
Quant Title : GC Extractables
QLast Update : Sat Jan 25 03:38:15 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

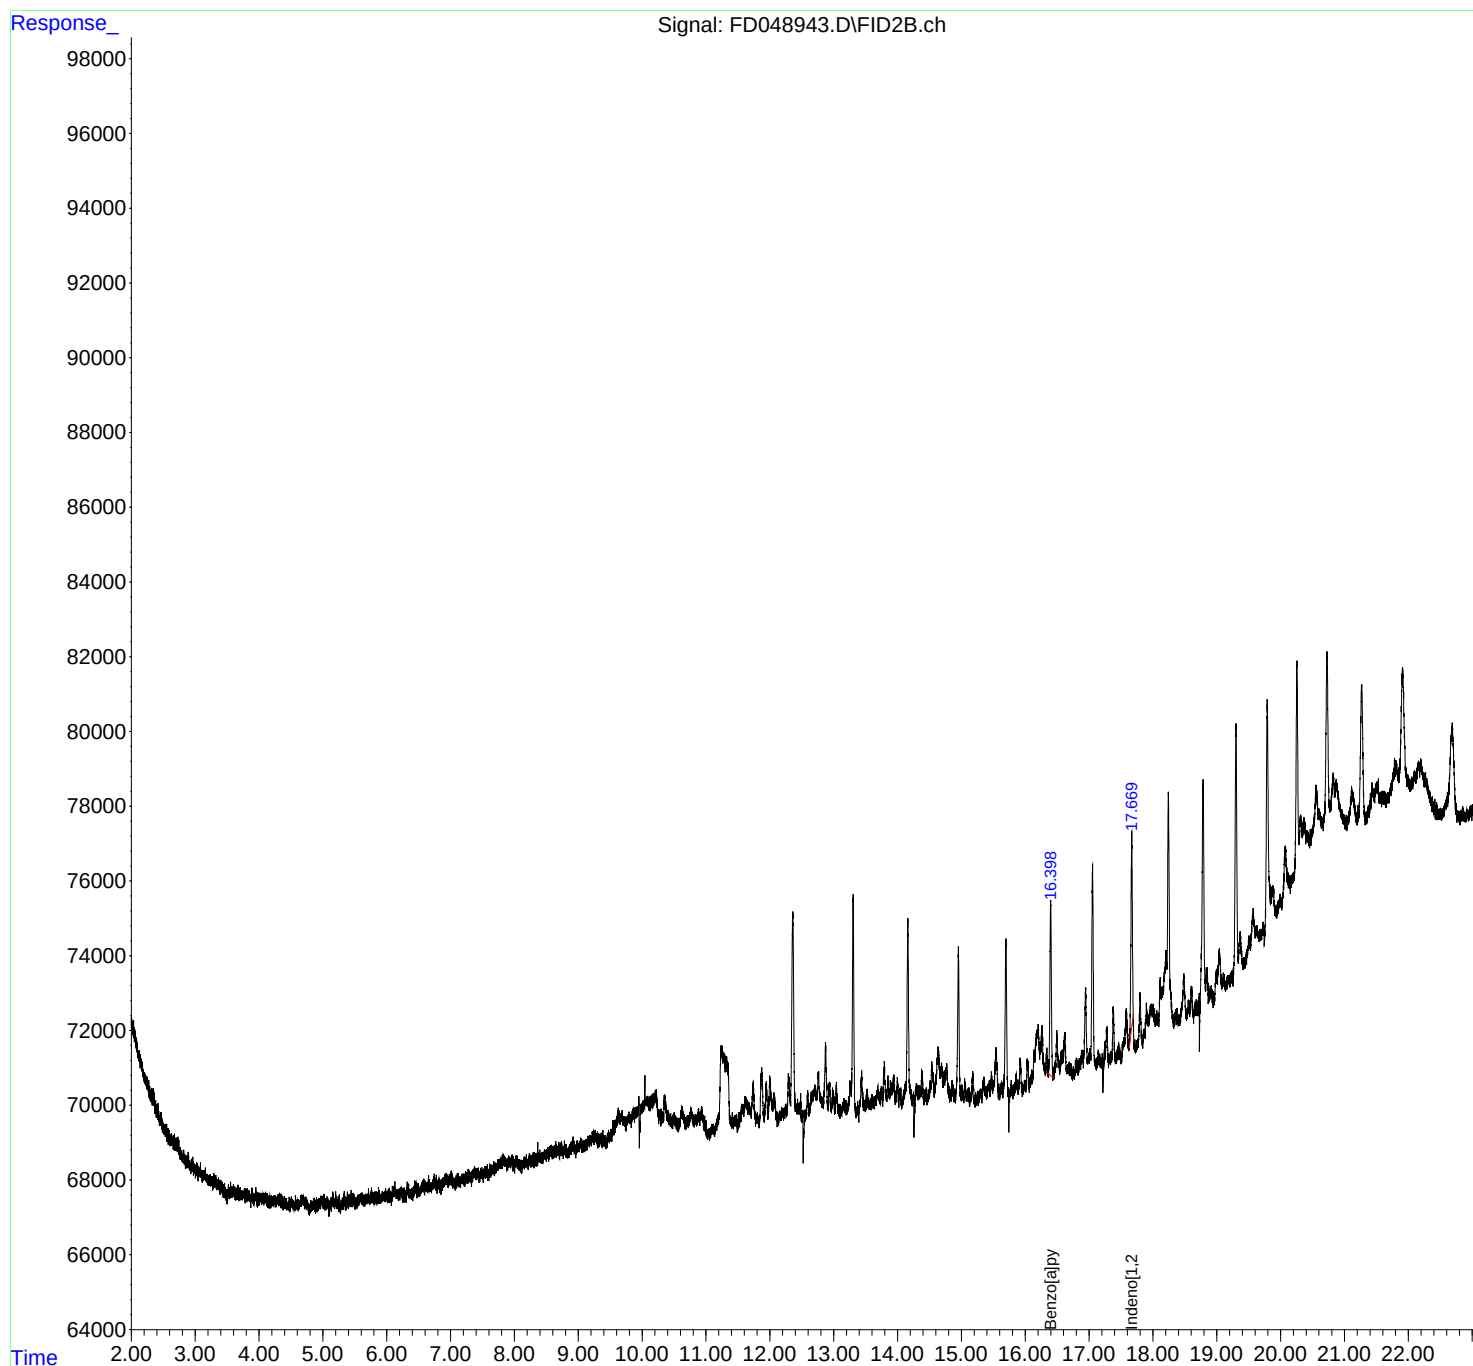


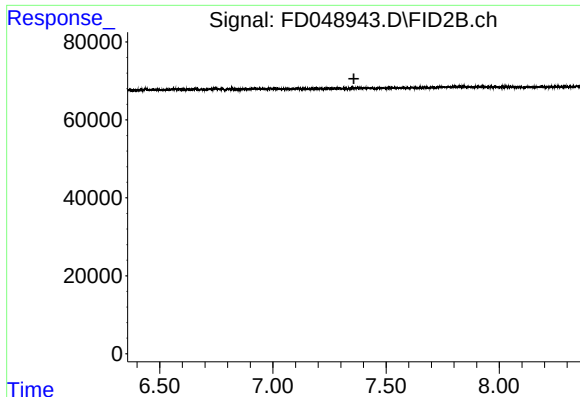

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T. : 7.358 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

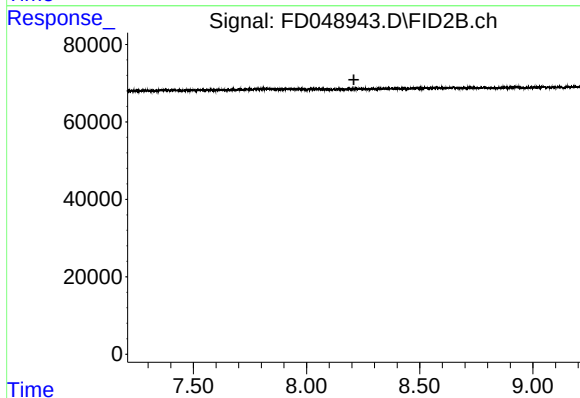


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 8.209 min
Response: 0
Conc: N.D.

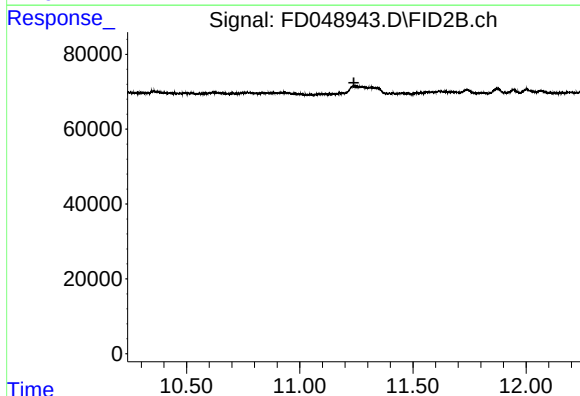


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.239 min
Response: 0
Conc: N.D.

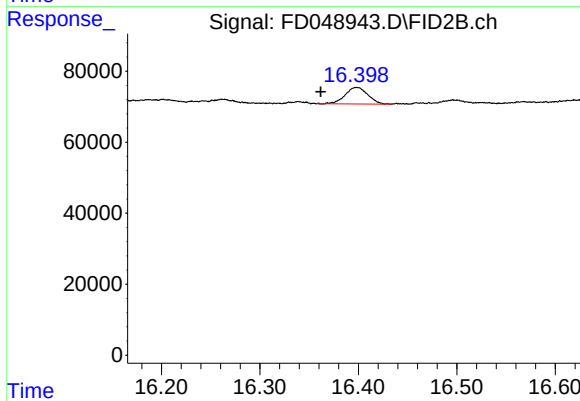

#18 Benzo[a]pyrene (C31.34)

R.T.: 16.398 min
Delta R.T.: 0.037 min
Response: 73869
Conc: 0.53 ug/ml

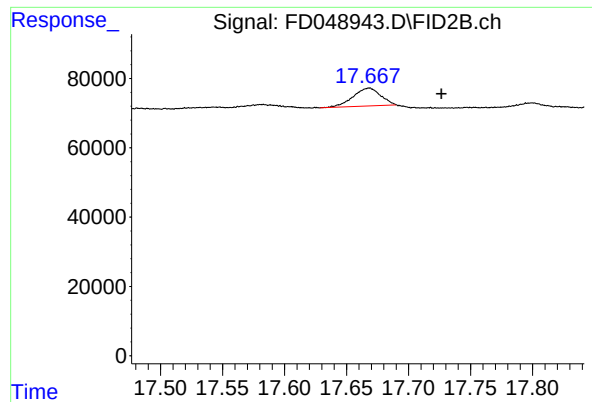

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 17.668 min
Delta R.T.: -0.059 min
Response: 80208
Conc: 0.77 ug/ml

Instrument :

FID_D

ClientSampleId :