

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD012723AR\
Data File : FD044907.D
Signal(s) : FID2B.ch
Acq On : 27 Jan 2023 10:30
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 28 00:49:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 012323.M
Quant Title : GC Extractables
QLast Update : Mon Jan 23 15:00:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) T Benzo[a]pyrene (C31.34)	16.595	68922	0.493 ug/ml
19) T Indeno[1,2,3-cd]pyren...	17.859f	67957	0.505 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD012723AR\
Data File : FD044907.D
Signal(s) : FID2B.ch
Acq On : 27 Jan 2023 10:30
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 28 00:49:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 012323.M
Quant Title : GC Extractables
QLast Update : Mon Jan 23 15:00:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

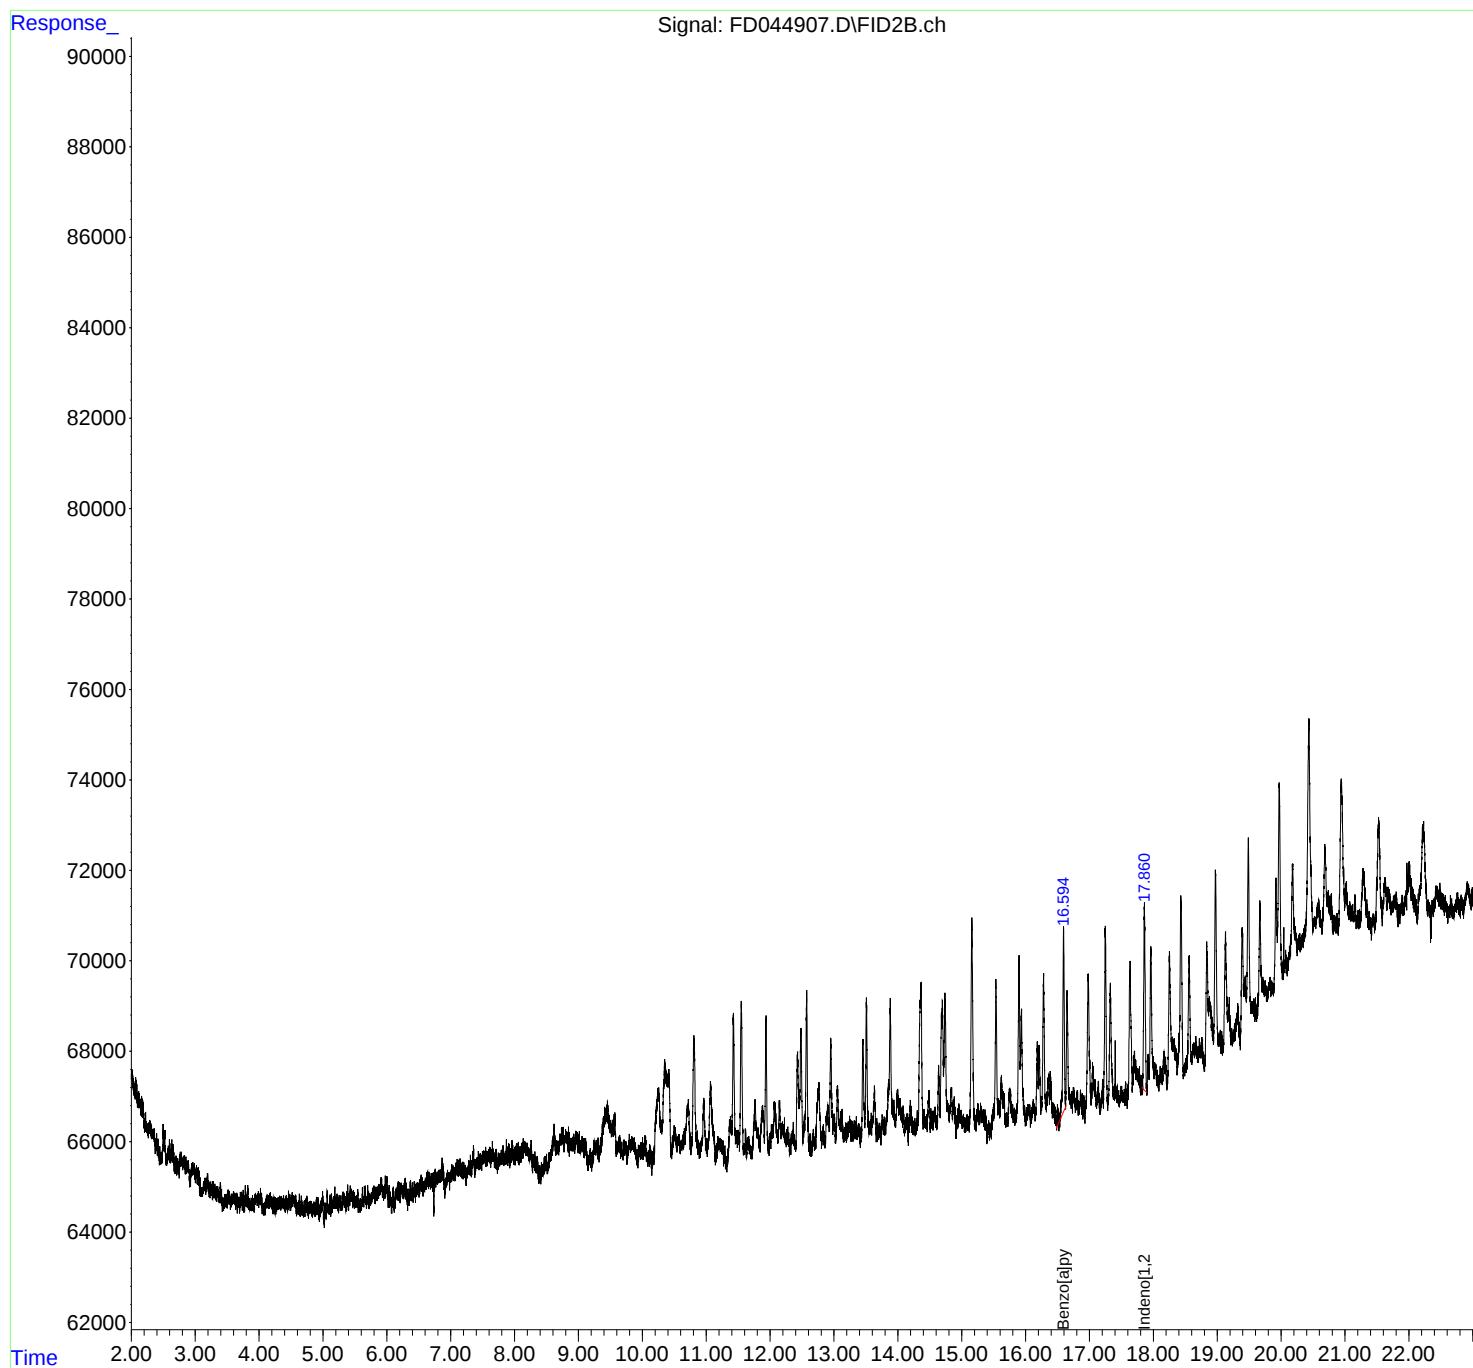


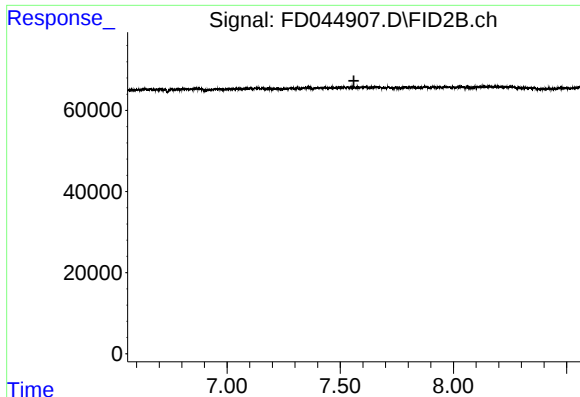

#4 2-Bromonaphthalene (SURR)


R.T.: 0.000 min
Exp R.T. : 7.560 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

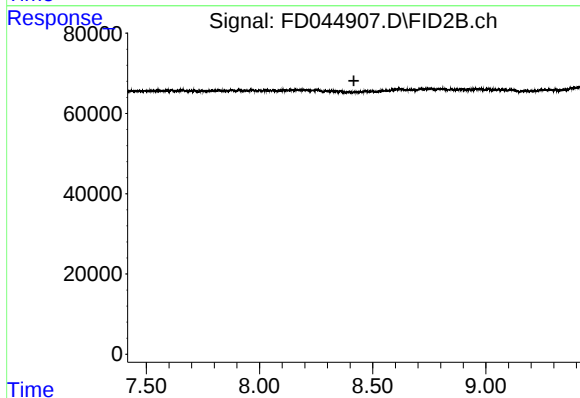


#6 2-Fluorobiphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 8.417 min
Response: 0
Conc: N.D.

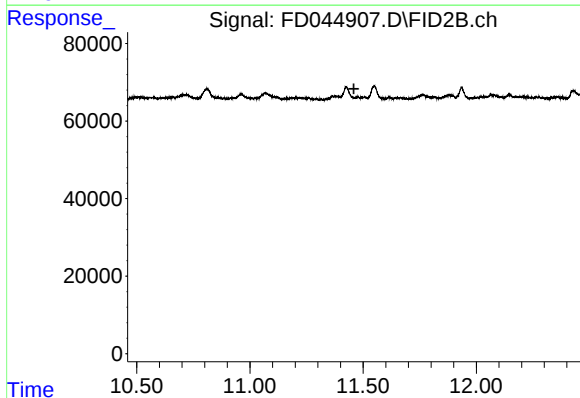


#11 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.459 min
Response: 0
Conc: N.D.

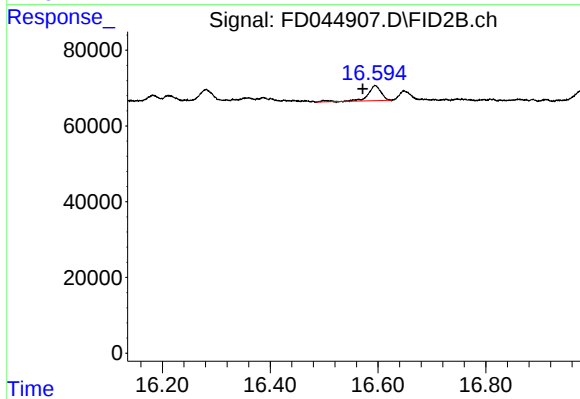

#18 Benzo[a]pyrene (C31.34)

R.T.: 16.595 min
Delta R.T.: 0.023 min
Response: 68922
Conc: 0.49 ug/ml

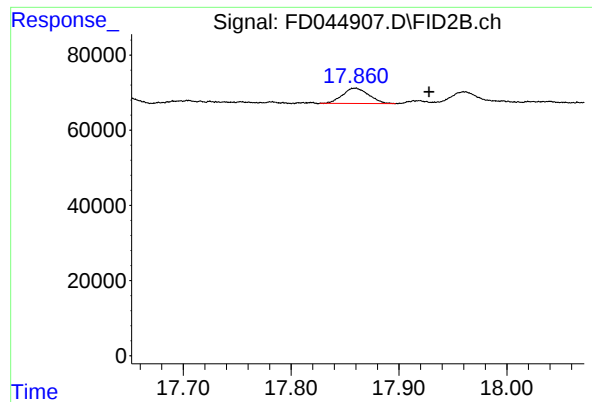

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 17.859 min
Delta R.T.: -0.069 min
Response: 67957
Conc: 0.50 ug/ml

Instrument :

FID_D

ClientSampleId :