

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD012925AL\
Data File : FD048995.D
Signal(s) : FID2B.ch
Acq On : 29 Jan 2025 13:36
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 30 05:01:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 012425.M
Quant Title : GC Extractables
QLast Update : Sat Jan 25 05:57:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.392	63583	0.370 ug/ml
18) T	n-Dotriacontane (C32)	18.220	73365	0.449 ug/ml
19) T	n-Tetratriacontane (C34)	19.006	54865	0.394 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD012925AL\
Data File : FD048995.D
Signal(s) : FID2B.ch
Acq On : 29 Jan 2025 13:36
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 30 05:01:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 012425.M
Quant Title : GC Extractables
QLast Update : Sat Jan 25 05:57:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

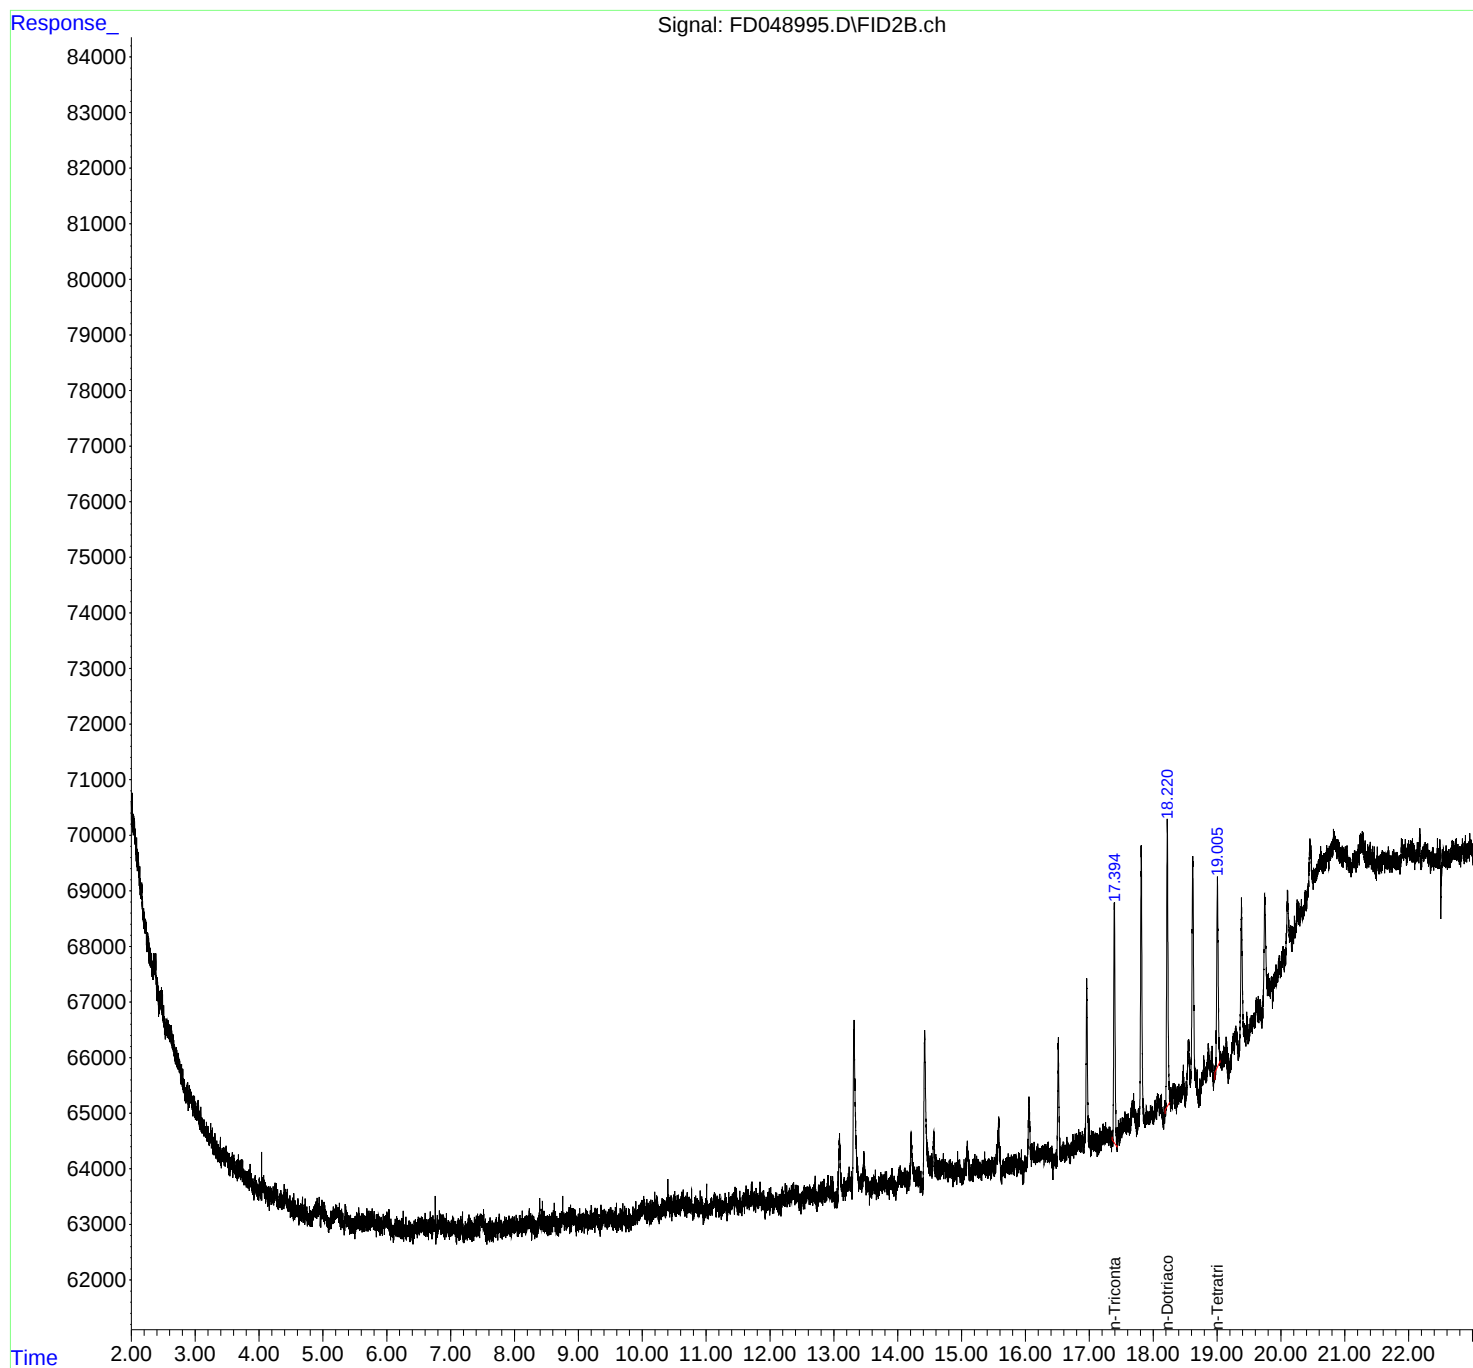


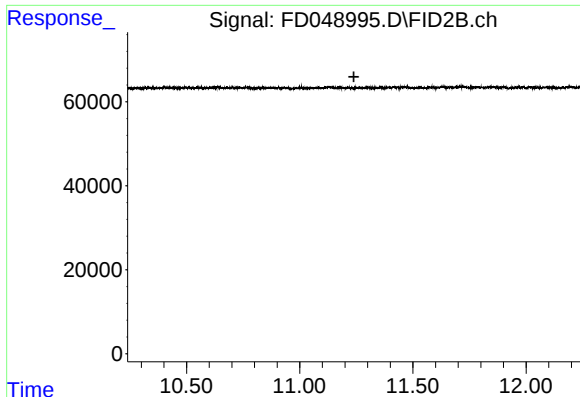

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.239 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

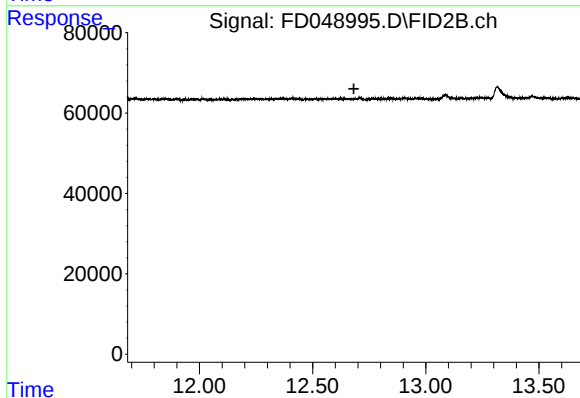


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.682 min
Response: 0
Conc: N.D.

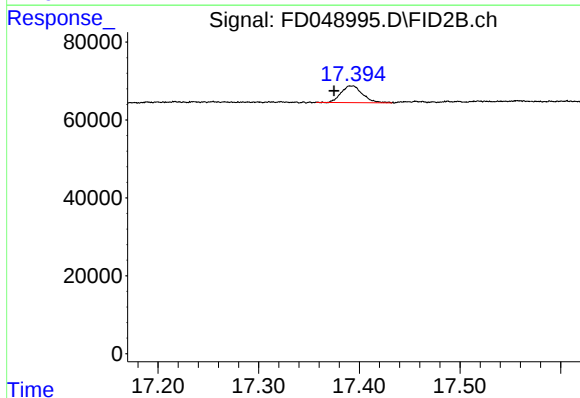


#17 n-Tricontane (C30)

R.T.: 17.392 min
Delta R.T.: 0.017 min
Response: 63583
Conc: 0.37 ug/ml

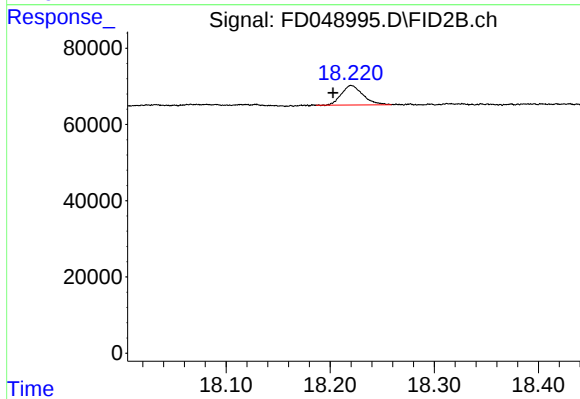

#18 n-Dotriacontane (C32)

R.T.: 18.220 min
Delta R.T.: 0.018 min
Response: 73365
Conc: 0.45 ug/ml

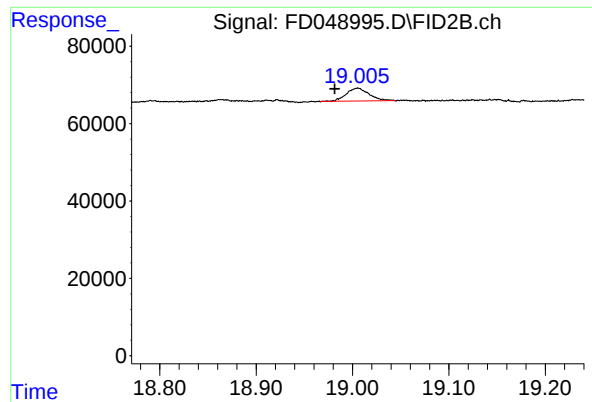

#19 n-Tetratriacontane (C34)

R.T.: 19.006 min
Delta R.T.: 0.024 min
Response: 54865
Conc: 0.39 ug/ml

Instrument :

FID_D

ClientSampleId :