

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD012925AL\
Data File : FD049003.D
Signal(s) : FID2B.ch
Acq On : 29 Jan 2025 19:05
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 30 05:04:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 012425.M
Quant Title : GC Extractables
QLast Update : Sat Jan 25 05:57:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.390	68594	0.400 ug/ml
18) T	n-Dotriacontane (C32)	18.219	82394	0.504 ug/ml
19) T	n-Tetratriacontane (C34)	19.002	57039	0.409 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD012925AL\
Data File : FD049003.D
Signal(s) : FID2B.ch
Acq On : 29 Jan 2025 19:05
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 30 05:04:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 012425.M
Quant Title : GC Extractables
QLast Update : Sat Jan 25 05:57:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

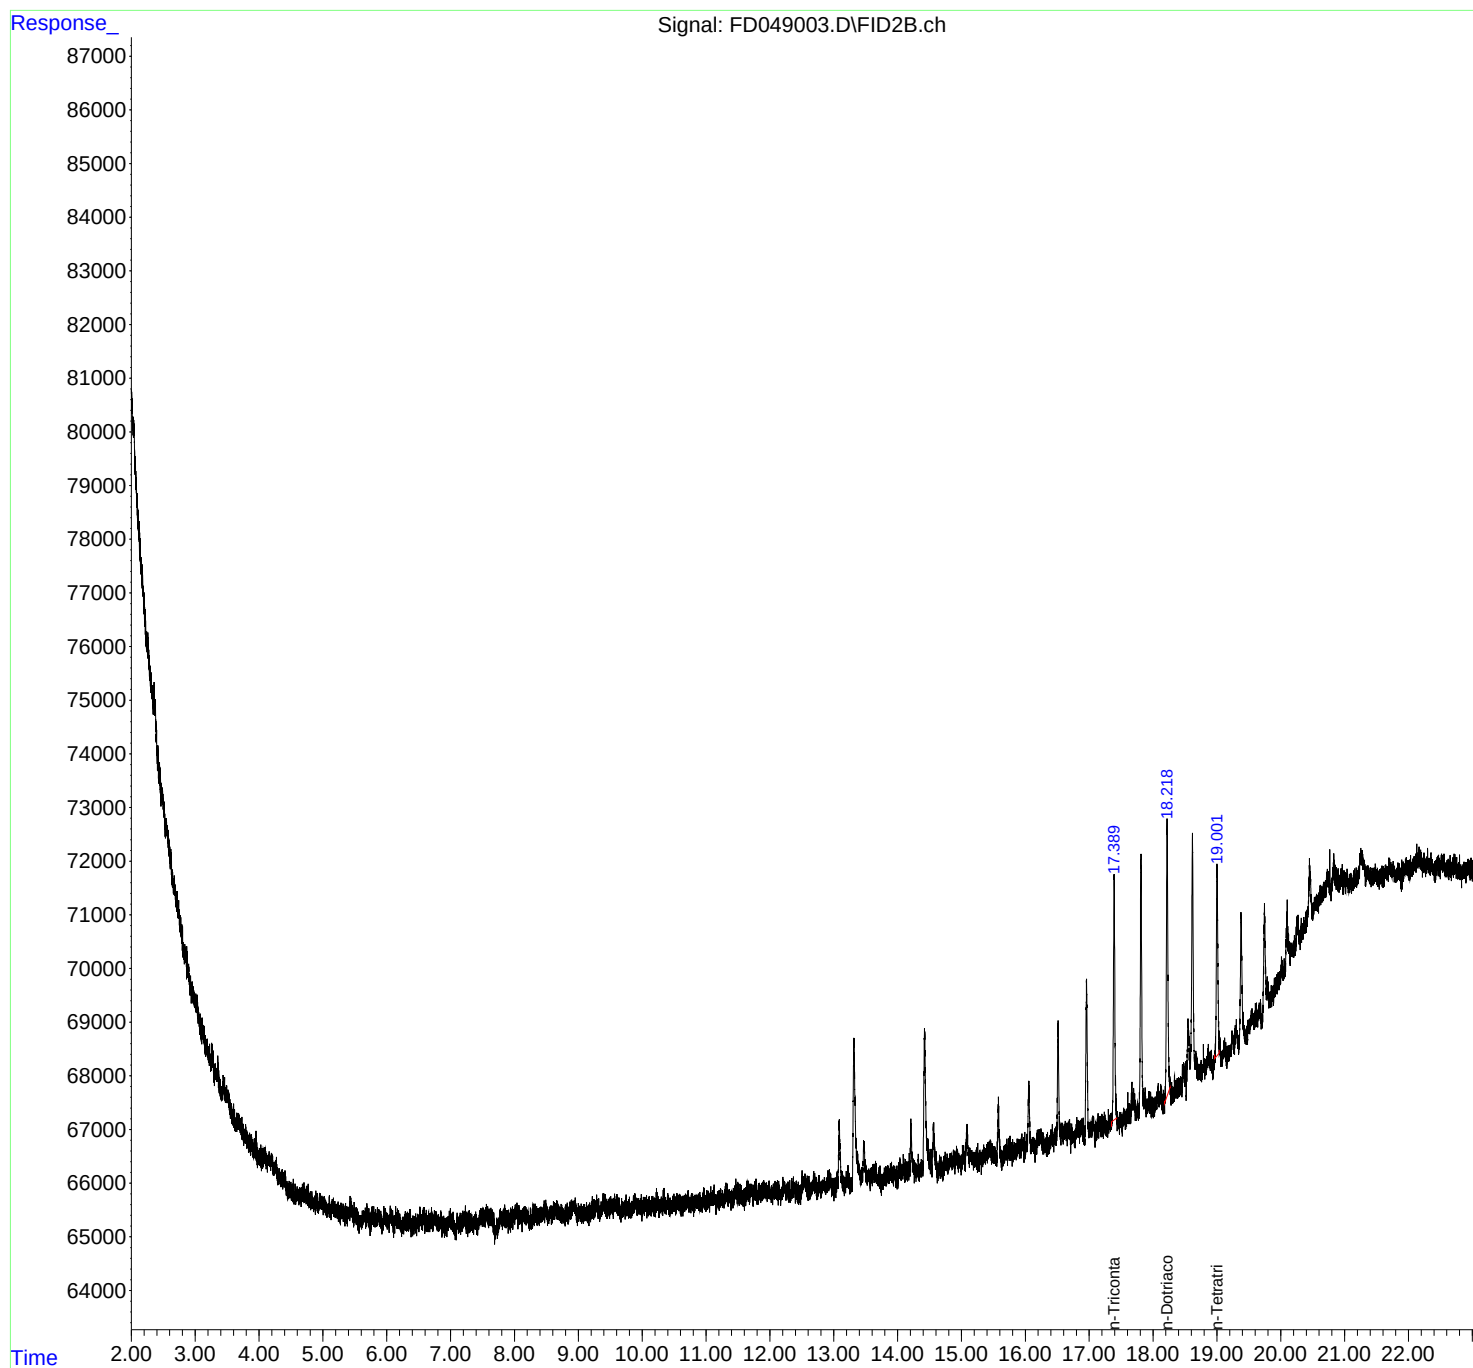


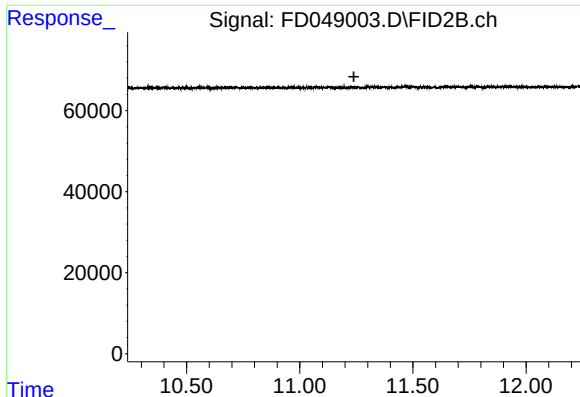

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.239 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

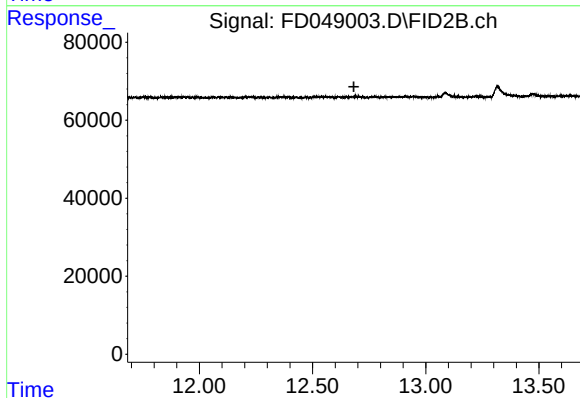


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.682 min
Response: 0
Conc: N.D.

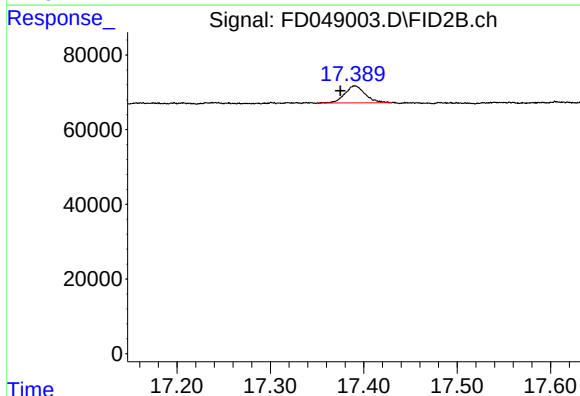


#17 n-Tricontane (C30)

R.T.: 17.390 min
Delta R.T.: 0.015 min
Response: 68594
Conc: 0.40 ug/ml

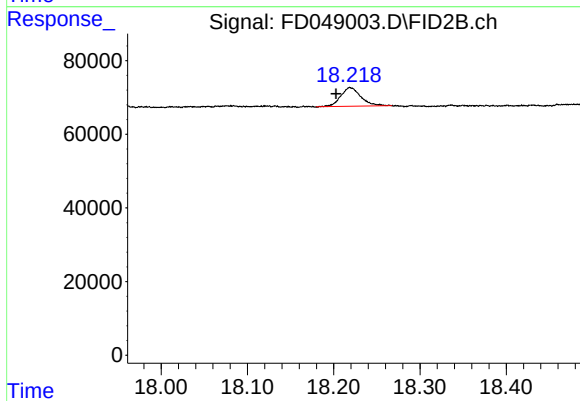

#18 n-Dotriacontane (C32)

R.T.: 18.219 min
Delta R.T.: 0.016 min
Response: 82394
Conc: 0.50 ug/ml

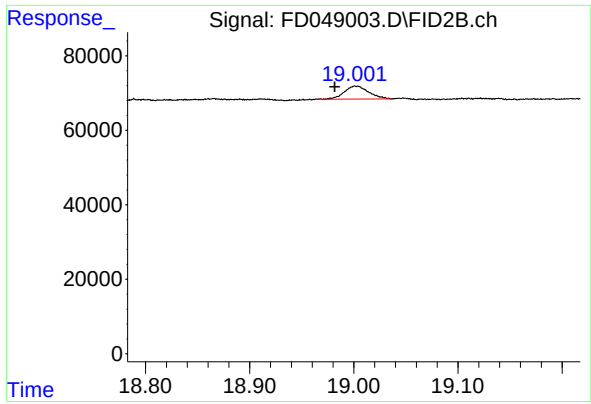

#19 n-Tetratriacontane (C34)

R.T.: 19.002 min
Delta R.T.: 0.020 min
Response: 57039
Conc: 0.41 ug/ml

Instrument :
FID_D
ClientSampleId :