

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_D\Data\FD013123AR\  
 Data File : FD044928.D  
 Signal(s) : FID2B.ch  
 Acq On : 31 Jan 2023 08:56  
 Operator : YP/AJ  
 Sample : MECL2  
 Misc :  
 ALS Vial : 51 Sample Multiplier: 1

Instrument :  
 FID\_D  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Jan 31 12:47:32 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aromatic EPH 012323.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Jan 23 15:00:18 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18µm

| Compound                       | R.T.   | Response   | Conc Units  |
|--------------------------------|--------|------------|-------------|
| -----                          |        |            |             |
| System Monitoring Compounds    |        |            |             |
| 11) S ortho-Terphenyl (SURR)   | 11.423 | 76898      | 0.414 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 0.83%       |
| Target Compounds               |        |            |             |
| 15) T Chrysene (C27.41)        | 14.736 | 56414      | 0.381 ug/ml |
| 18) T Benzo[a]pyrene (C31.34)  | 16.594 | 67717      | 0.485 ug/ml |
| 19) T Indeno[1,2,3-cd]pyren... | 17.958 | 68854      | 0.512 ug/ml |
| 20) T Dibenz[a,h]anthracene... | 17.958 | 68854      | 0.520 ug/ml |
| -----                          |        |            |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_D\Data\FD013123AR\  
Data File : FD044928.D  
Signal(s) : FID2B.ch  
Acq On : 31 Jan 2023 08:56  
Operator : YP/AJ  
Sample : MECL2  
Misc :  
ALS Vial : 51 Sample Multiplier: 1

Instrument :  
FID\_D  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jan 31 12:47:32 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aromatic EPH 012323.M  
Quant Title : GC Extractables  
QLast Update : Mon Jan 23 15:00:18 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18µm

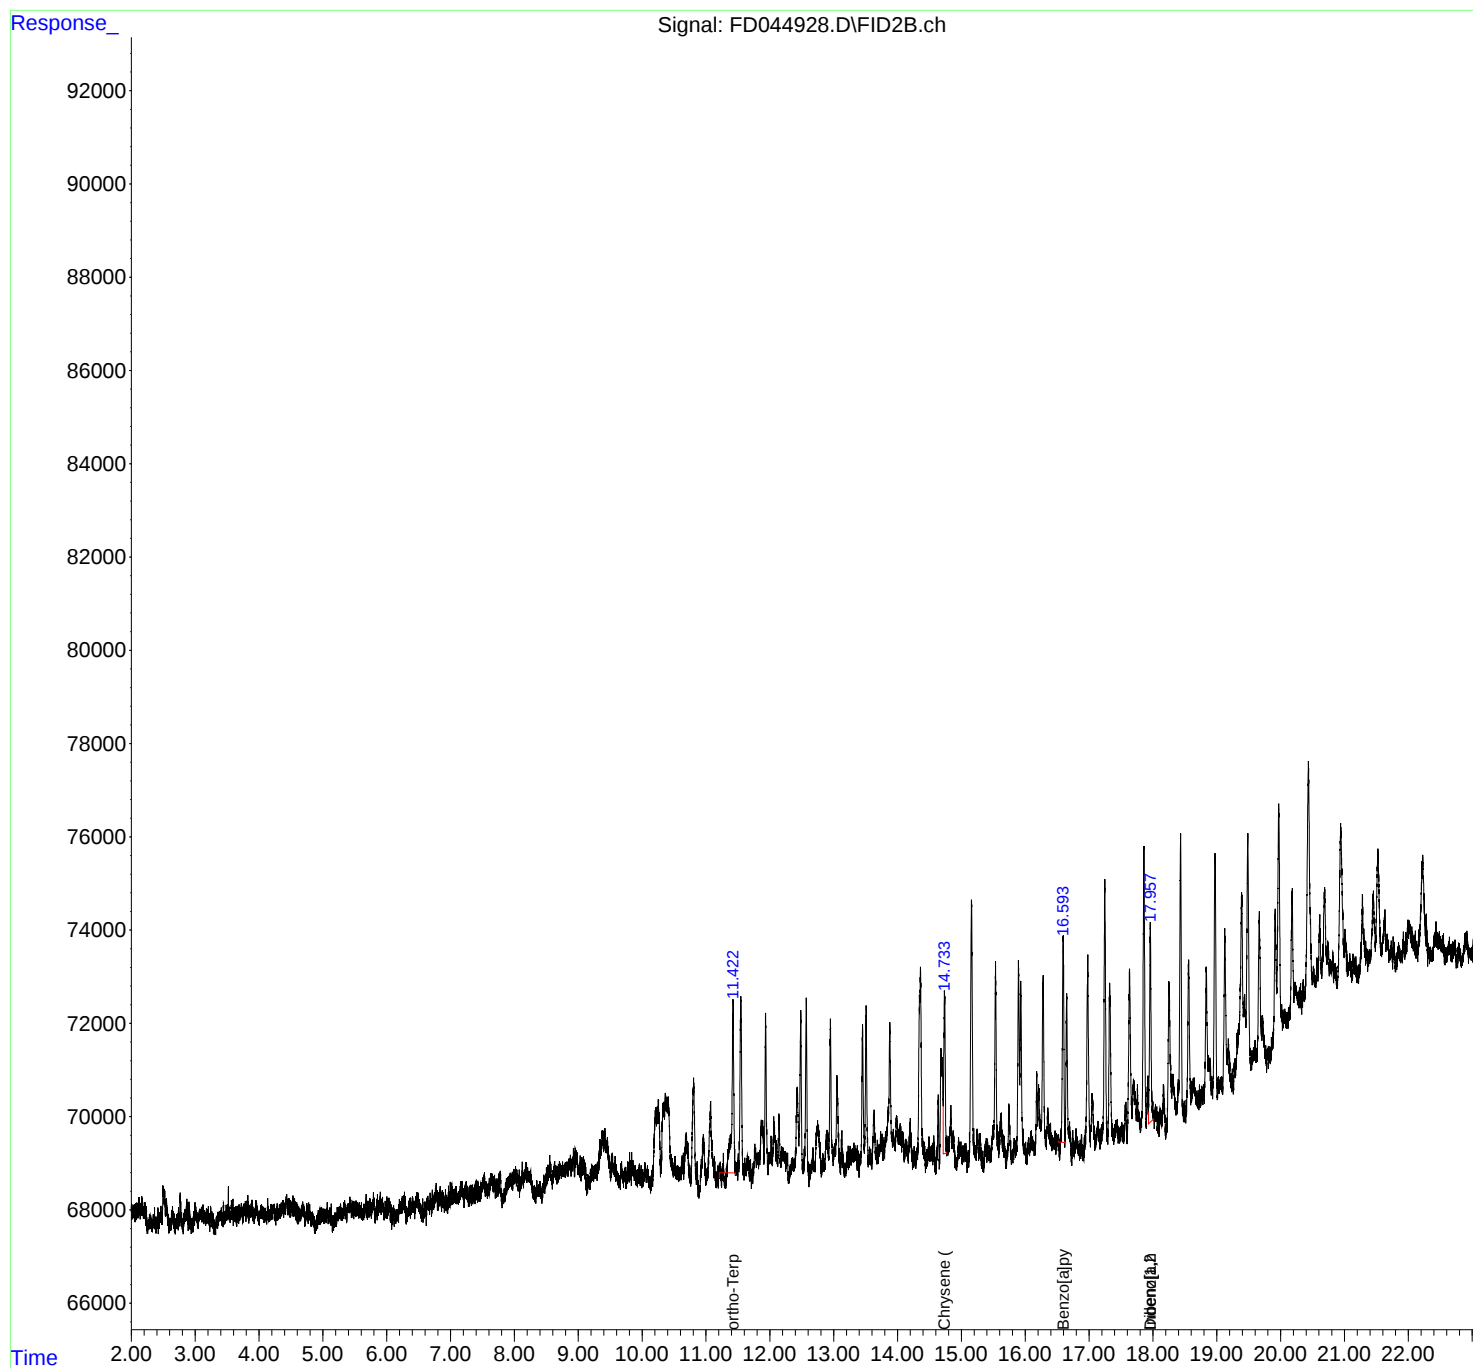


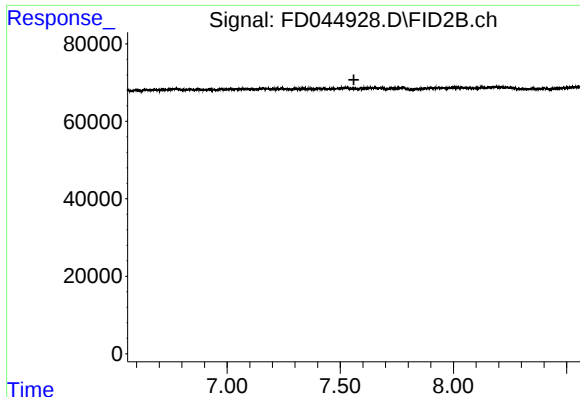

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min  
Exp R.T.: 7.560 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_D  
ClientSampleId :

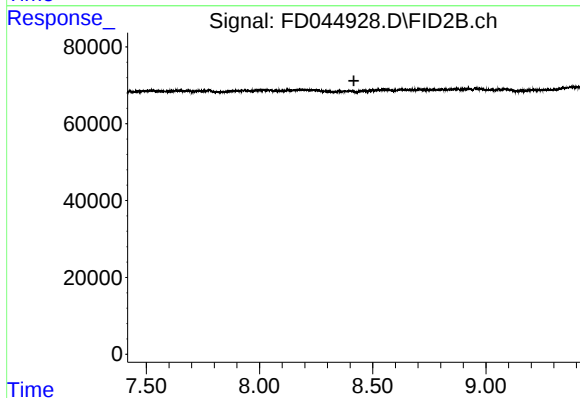


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min  
Exp R.T.: 8.417 min  
Response: 0  
Conc: N.D.

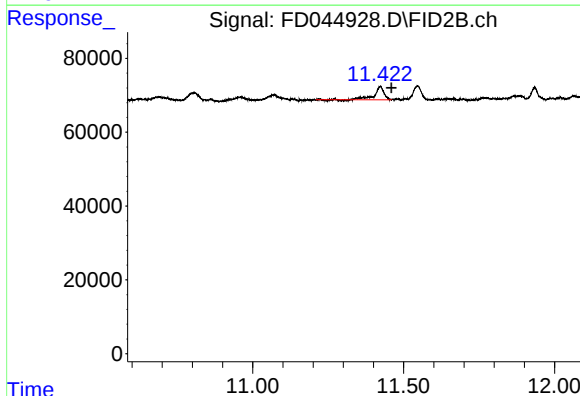


#11 ortho-Terphenyl (SURRE)

R.T.: 11.423 min  
Delta R.T.: -0.036 min  
Response: 76898  
Conc: 0.41 ug/ml

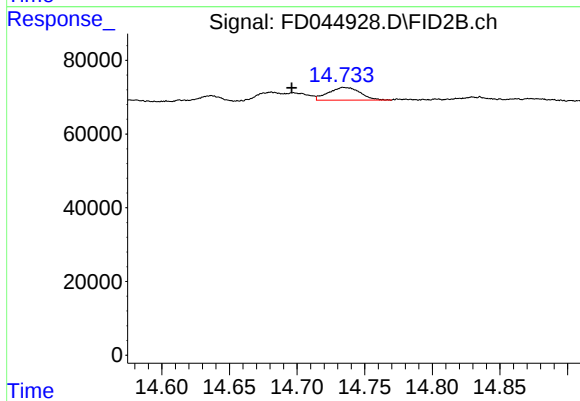

#15 Chrysene (C27.41)


R.T.: 14.736 min  
Delta R.T.: 0.039 min  
Response: 56414  
Conc: 0.38 ug/ml

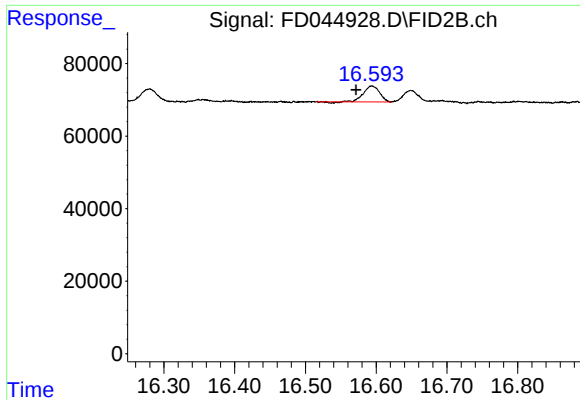

#18 Benzo[a]pyrene (C31.34)


R.T.: 16.594 min  
Delta R.T.: 0.022 min  
Response: 67717  
Conc: 0.48 ug/ml

Instrument :  
FID\_D  
ClientSampleId :

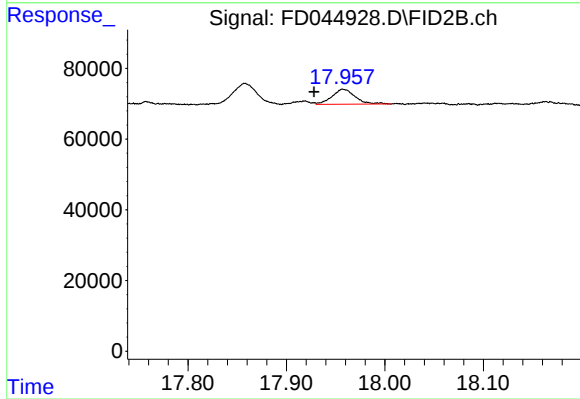

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 17.958 min  
Delta R.T.: 0.030 min  
Response: 68854  
Conc: 0.51 ug/ml

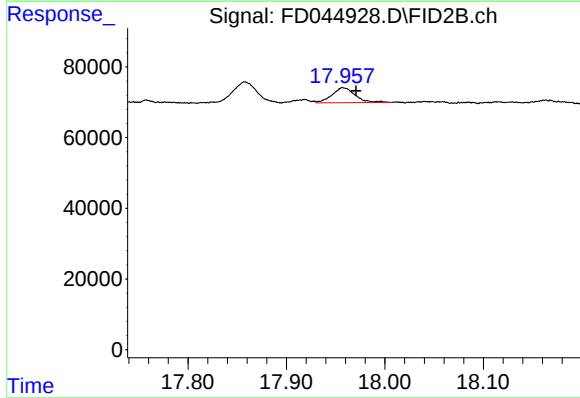

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 17.958 min  
Delta R.T.: -0.013 min  
Response: 68854  
Conc: 0.52 ug/ml