

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD020620AL\
 Data File : FD032292.D
 Signal(s) : FID2B.CH
 Acq On : 06 Feb 2020 7:43
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :
 MECL2

Integration File: autoint1.e
 Quant Time: Feb 07 05:58:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 020420.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 05 06:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) T n-Docosane (C22)	13.708	82842	0.597 ug/ml
15) T n-Hexacosane (C26)	15.825	93124	0.680 ug/ml
16) T n-Octacosane (C28)	16.772	120720	0.900 ug/ml
17) T n-Tricontane (C30)	17.656	111331	0.865 ug/ml
18) T n-Dotriacontane (C32)	18.495	227730	2.045 ug/ml
20) T n-Hexatriacontane (C36)	20.044	388793	4.402 ug/ml
22) T n-Tetracontane (C40)	21.619	439736	4.965 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD020620AL\
Data File : FD032292.D
Signal(s) : FID2B.CH
Acq On : 06 Feb 2020 7:43
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Feb 07 05:58:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 020420.M
Quant Title : GC Extractables
QLast Update : Wed Feb 05 06:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

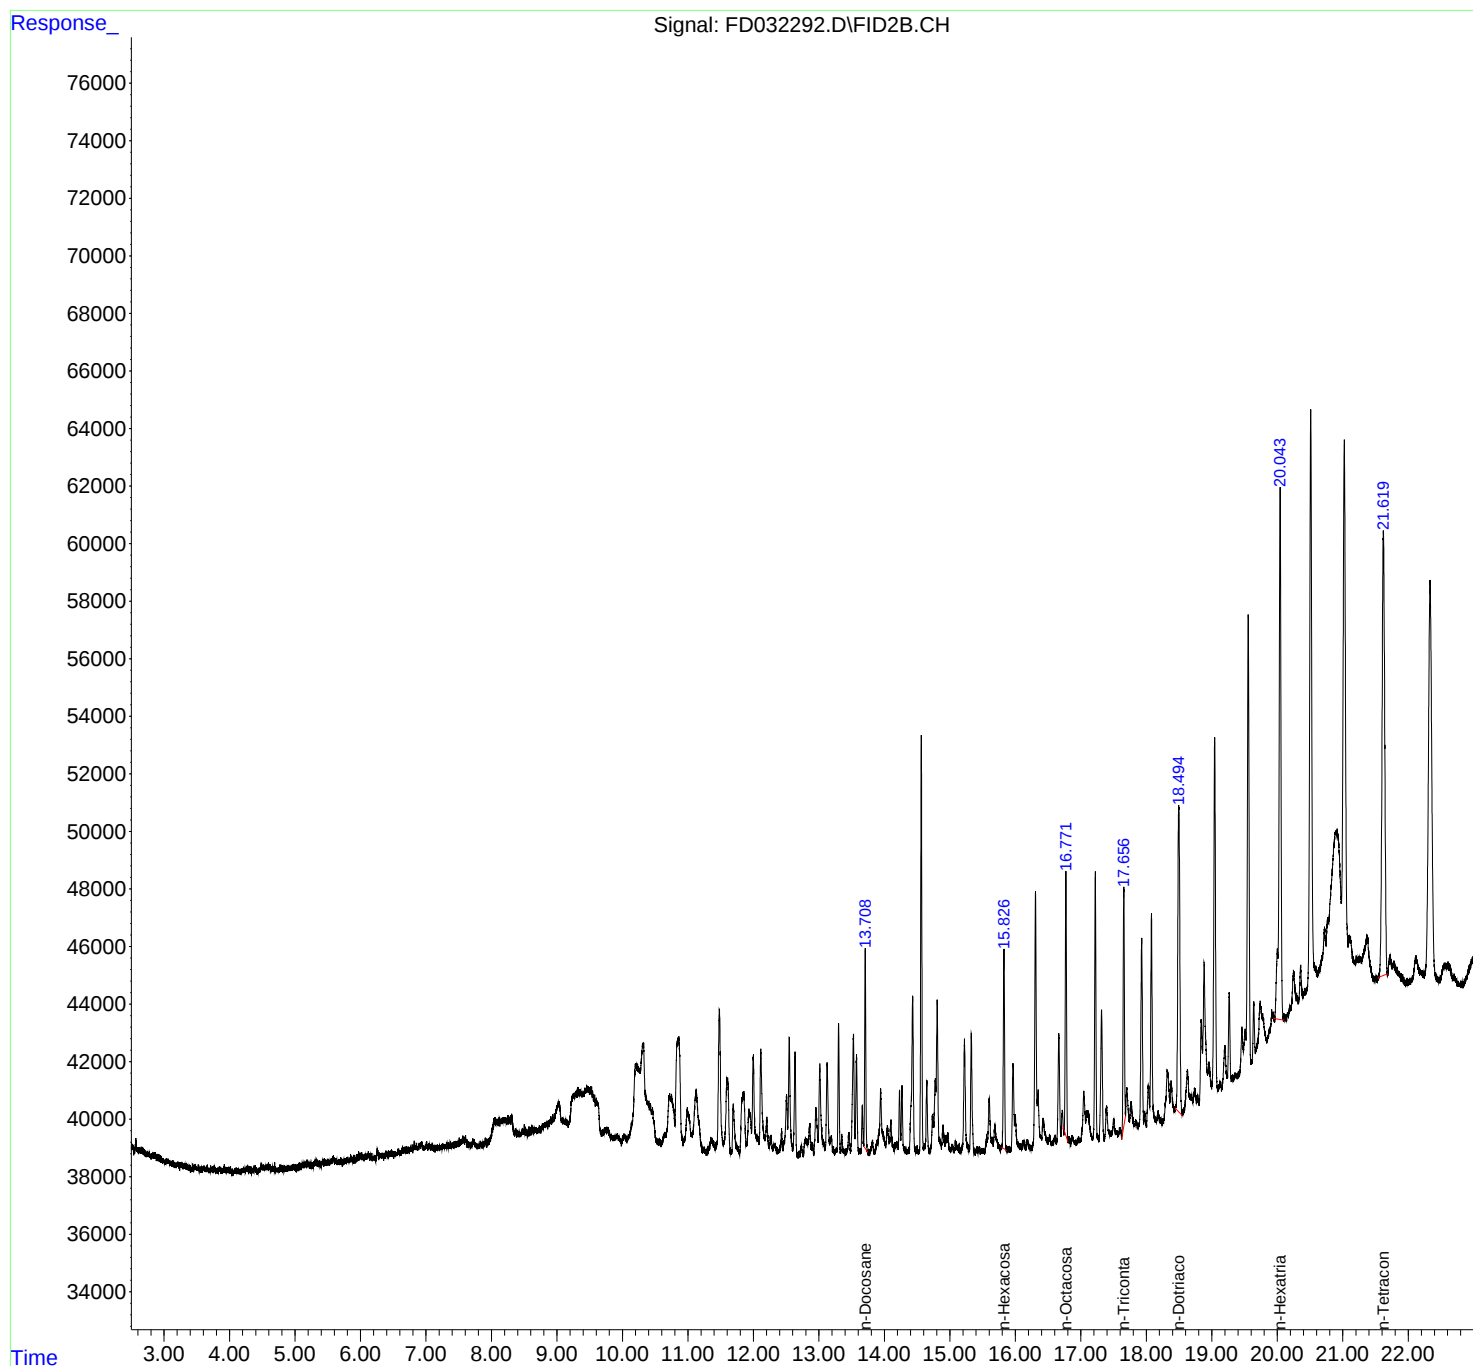


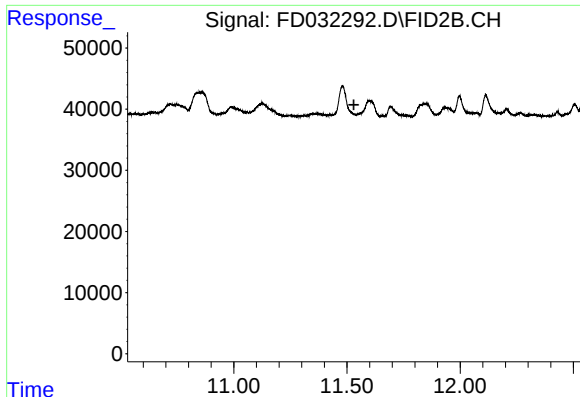

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.531 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :
MECL2

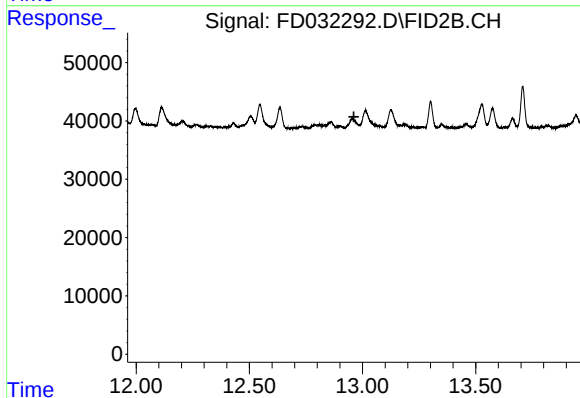


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.962 min
Response: 0
Conc: N.D.

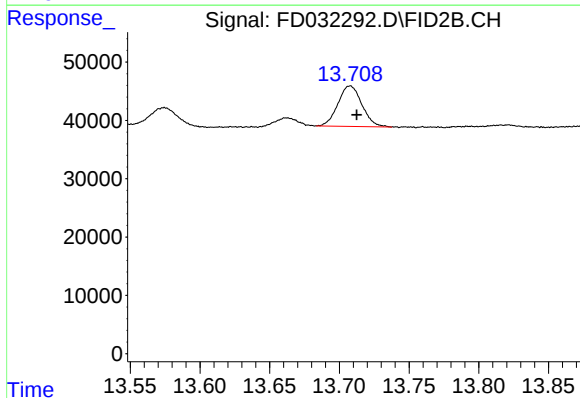


#13 n-Docosane (C22)

R.T.: 13.708 min
Delta R.T.: -0.005 min
Response: 82842
Conc: 0.60 ug/ml

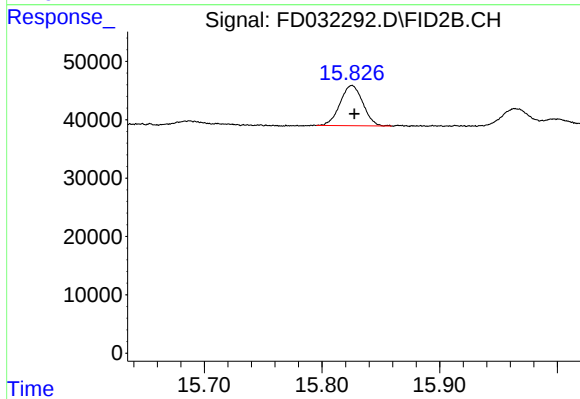

#15 n-Hexacosane (C26)


R.T.: 15.825 min
Delta R.T.: -0.002 min
Response: 93124
Conc: 0.68 ug/ml

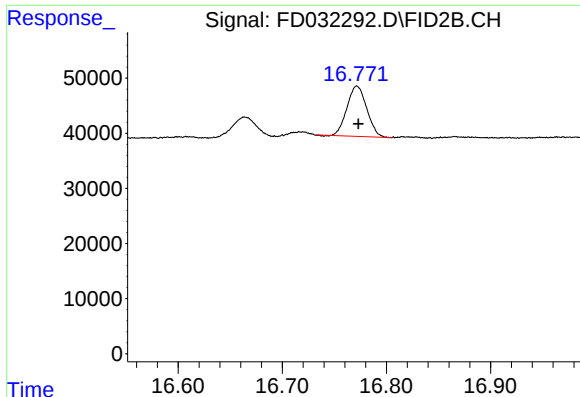

#16 n-Octacosane (C28)


R.T.: 16.772 min
Delta R.T.: -0.002 min
Response: 120720
Conc: 0.90 ug/ml

Instrument :
FID_D
ClientSampleId :
MECL2

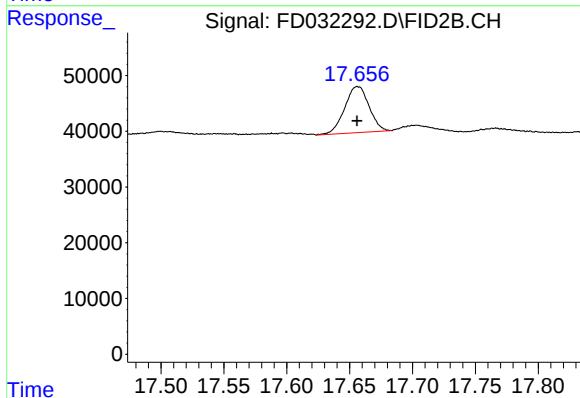


#17 n-Tricontane (C30)

R.T.: 17.656 min
Delta R.T.: 0.000 min
Response: 111331
Conc: 0.87 ug/ml

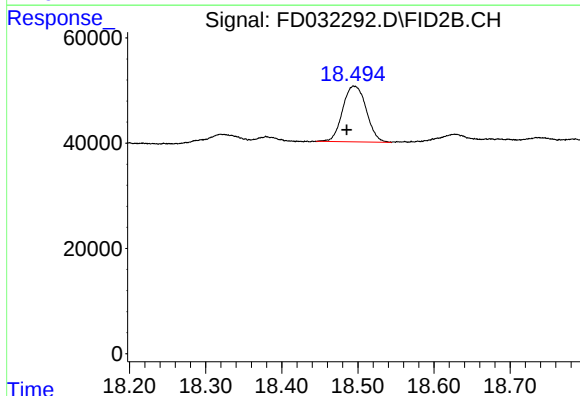


#18 n-Dotriacontane (C32)

R.T.: 18.495 min
Delta R.T.: 0.010 min
Response: 227730
Conc: 2.05 ug/ml

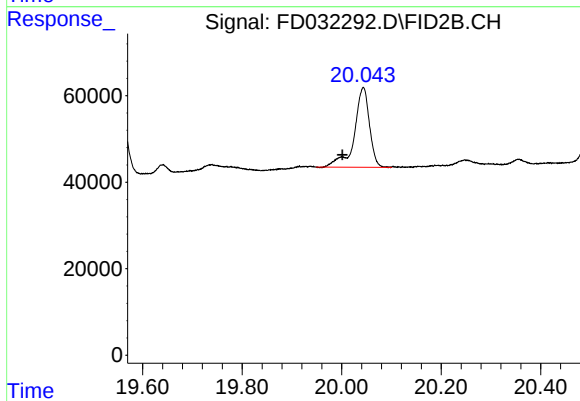

#20 n-Hexatriacontane (C36)

R.T.: 20.044 min
Delta R.T.: 0.042 min
Response: 388793
Conc: 4.40 ug/ml

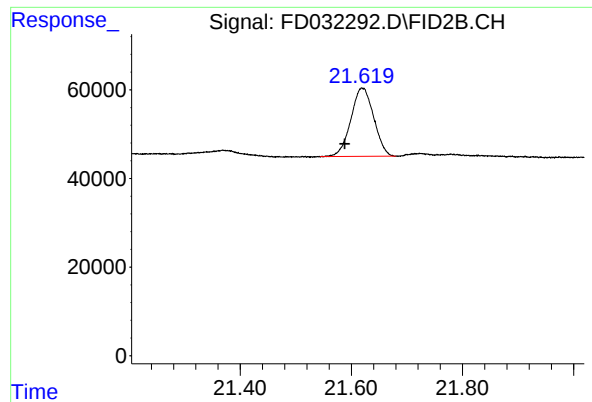

#22 n-Tetracontane (C40)

R.T.: 21.619 min
Delta R.T.: 0.031 min
Response: 439736
Conc: 4.97 ug/ml

Instrument :
FID_D
ClientSampleId :
MECL2