

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD022122AL\
 Data File : FD041218.D
 Signal(s) : FID2B.CH
 Acq On : 21 Feb 2022 17:00
 Operator : YP\AJ
 Sample : N1594-02
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :
 RO-CONCRETE-COMP-EPH-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/22/2022
 Supervised By :Ankita Jodhani 02/22/2022

Integration File: autoint1.e
 Quant Time: Feb 22 02:17:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 020822.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 09 03:32:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.236	1793320	64.163 ug/mlm
Spiked Amount	50.000	Recovery	= 128.33%
12) S 1-chlorooctadecane (S...	12.675	839880	40.118 ug/mlm
Spiked Amount	50.000	Recovery	= 80.24%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD022122AL\
Data File : FD041218.D
Signal(s) : FID2B.CH
Acq On : 21 Feb 2022 17:00
Operator : YP\AJ
Sample : N1594-02
Misc :
ALS Vial : 59 Sample Multiplier: 1


Instrument :
FID_D
ClientSampleId :
RO-CONCRETE-COMP-EPH-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/22/2022
Supervised By :Ankita Jodhani 02/22/2022

Integration File: autoint1.e
Quant Time: Feb 22 02:17:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 020822.M
Quant Title : GC Extractables
QLast Update : Wed Feb 09 03:32:15 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

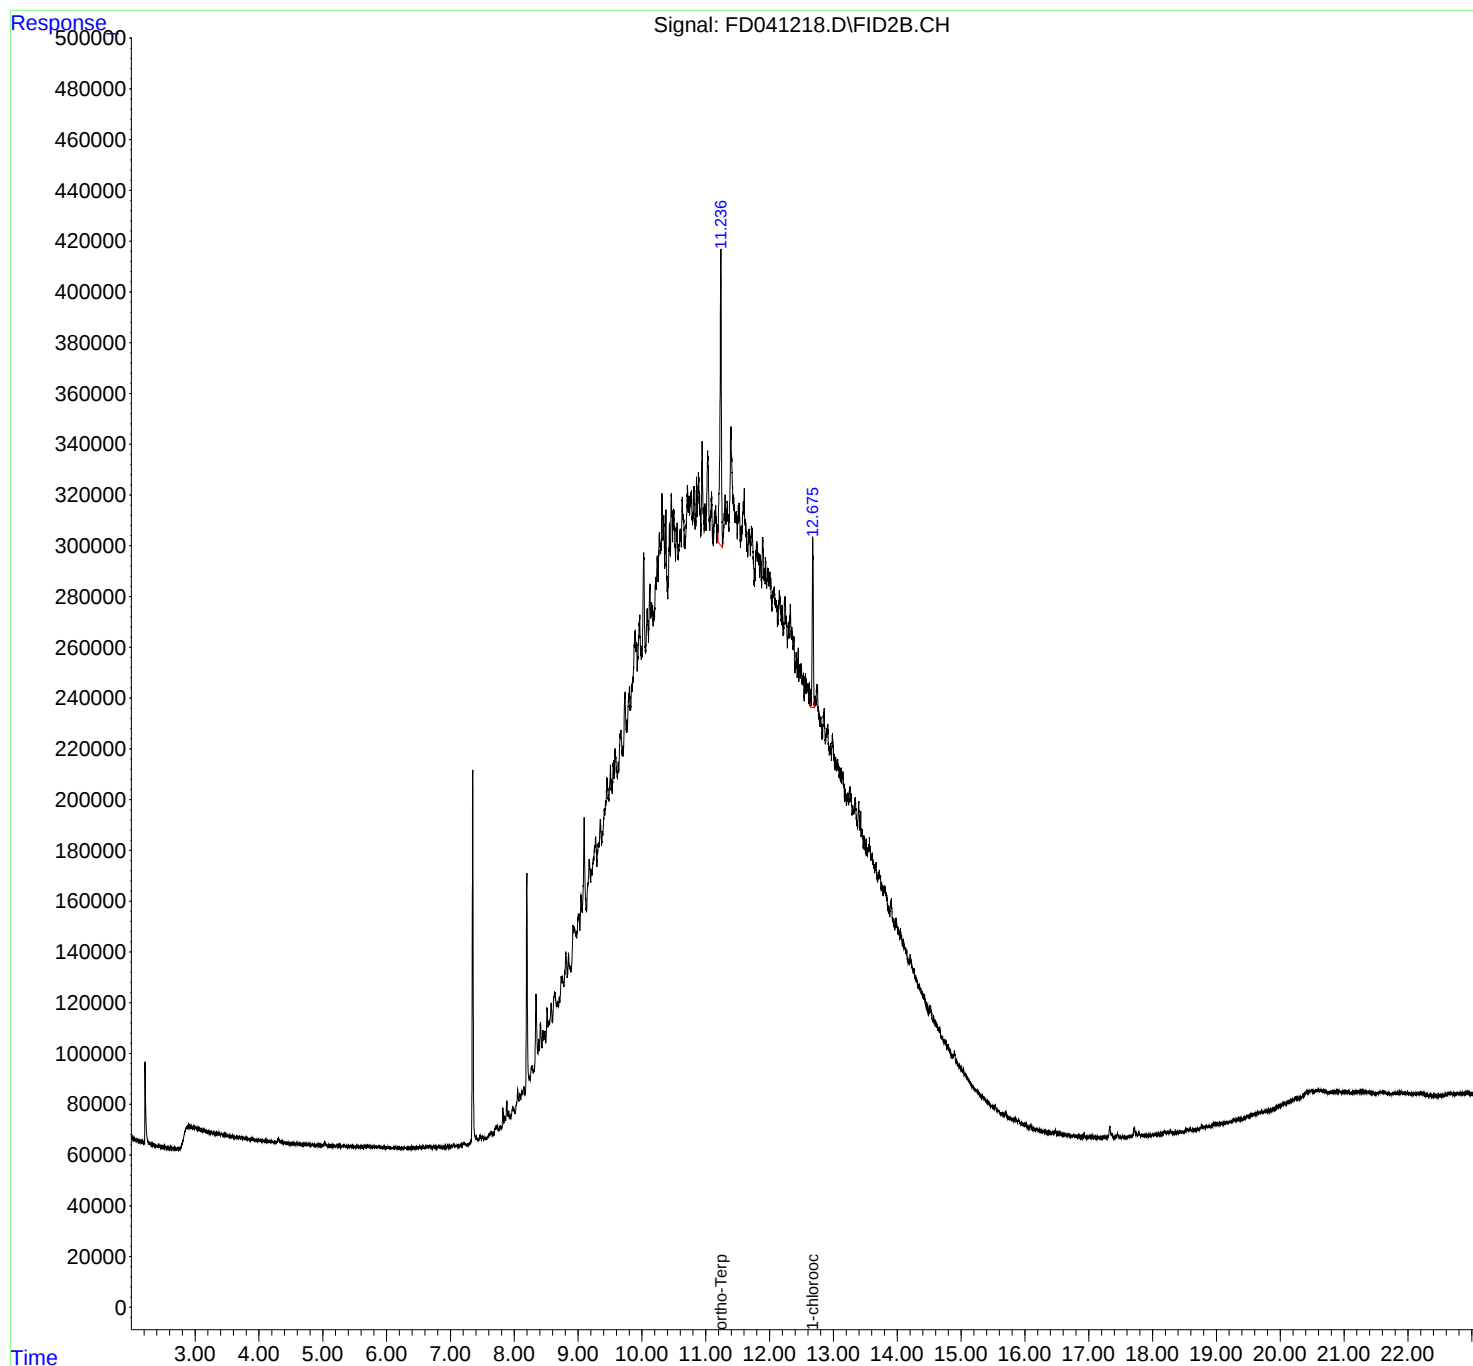

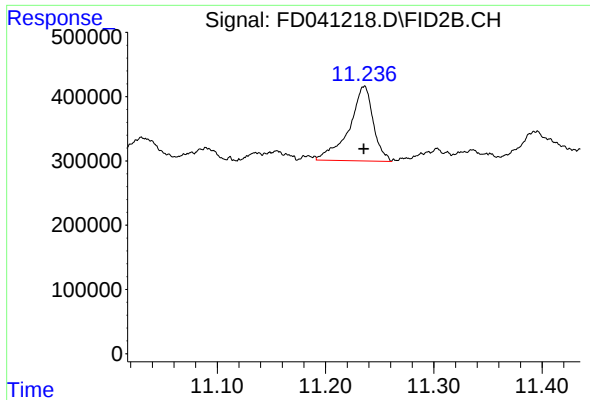


#9 ortho-Terphenyl (SURR)

R.T.: 11.236 min
Delta R.T.: 0.000 min
Response: 1793320
Conc: 64.16 ug/ml

Instrument :
FID_D
ClientSampleId :
RO-CONCRETE-COMP-EPH-2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/22/2022
Supervised By :Ankita Jodhani 02/22/2022

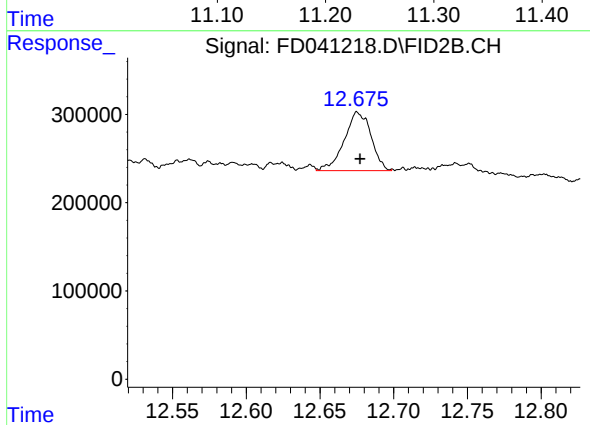

#12 1-chlorooctadecane (SURR)

R.T.: 12.675 min
Delta R.T.: -0.003 min
Response: 839880
Conc: 40.12 ug/ml m