

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD022224AR\
Data File : FD047269.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2024 08:24
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 23 03:39:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 020824.M
Quant Title : GC Extractables
QLast Update : Thu Feb 08 13:43:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) T Benzo[a]pyrene (C31.34)	16.495	45318	0.335 ug/ml
19) T Indeno[1,2,3-cd]pyren...	17.759f	42425	0.336 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD022224AR\
Data File : FD047269.D
Signal(s) : FID2B.ch
Acq On : 22 Feb 2024 08:24
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Feb 23 03:39:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 020824.M
Quant Title : GC Extractables
QLast Update : Thu Feb 08 13:43:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

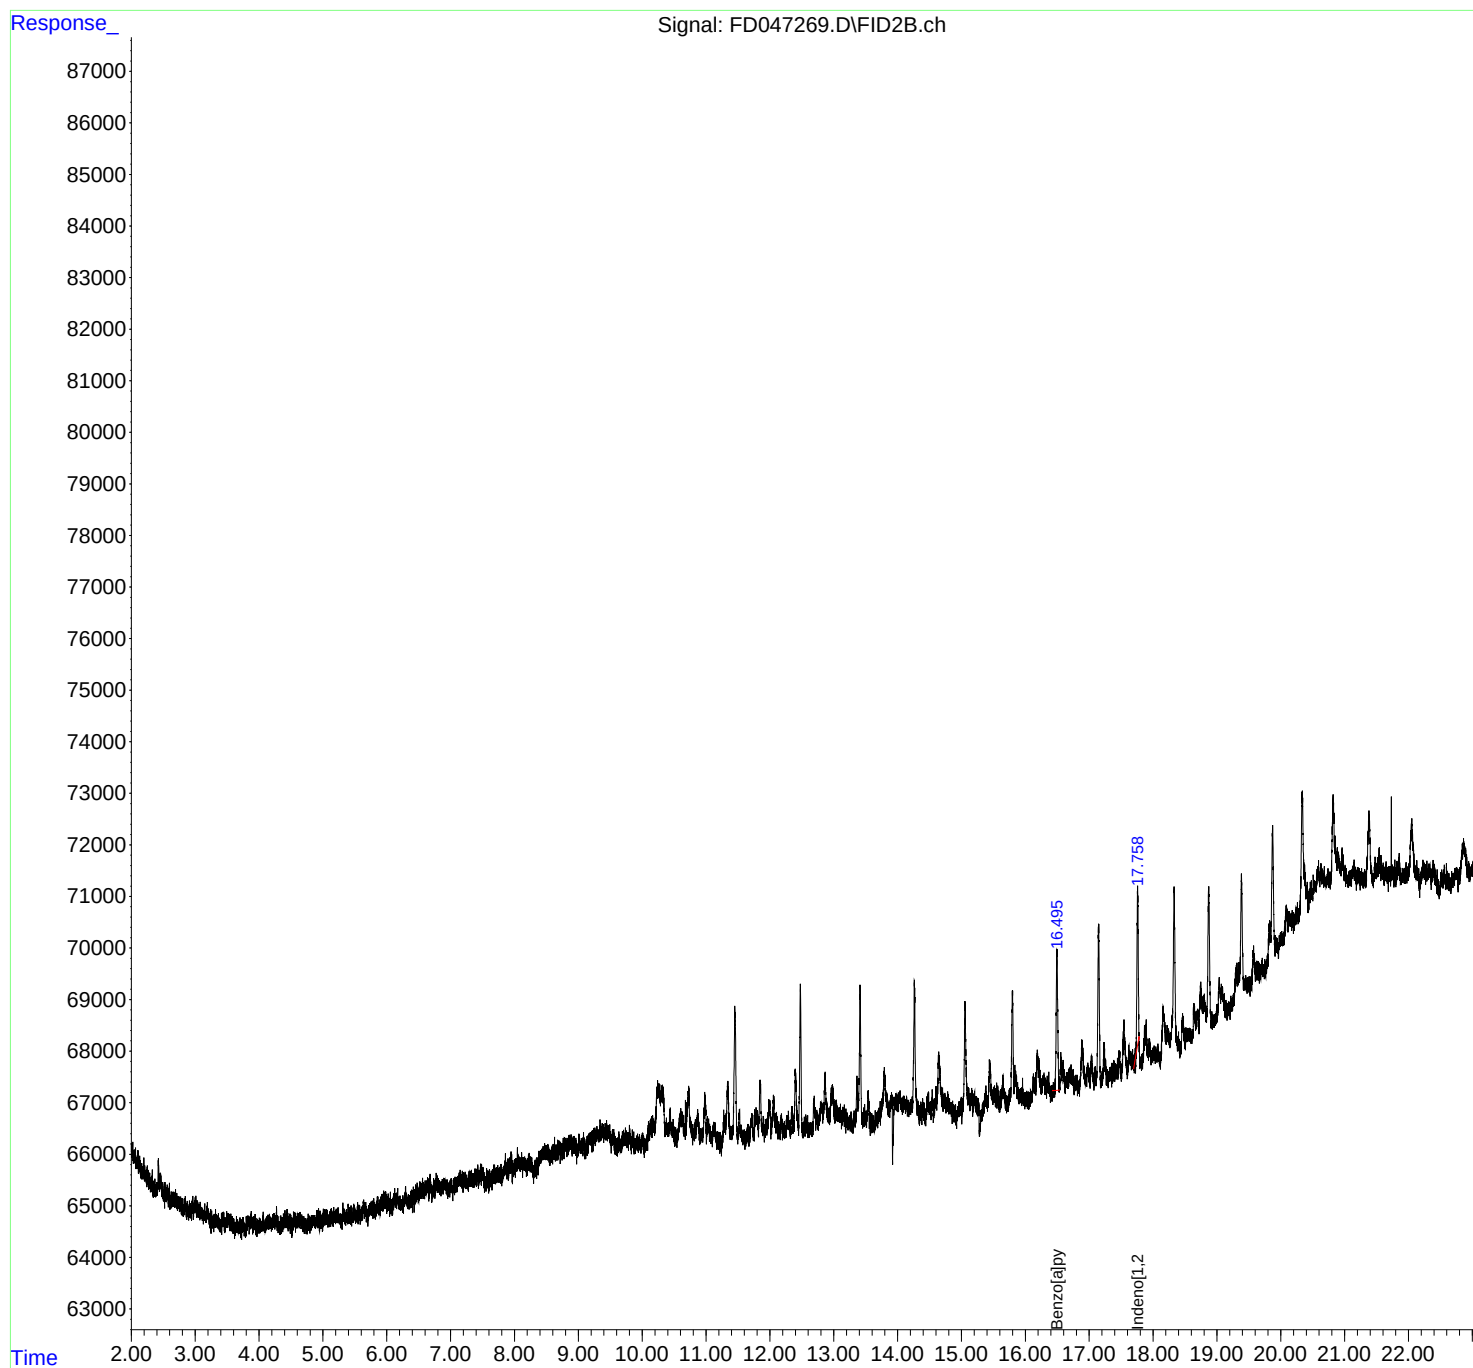


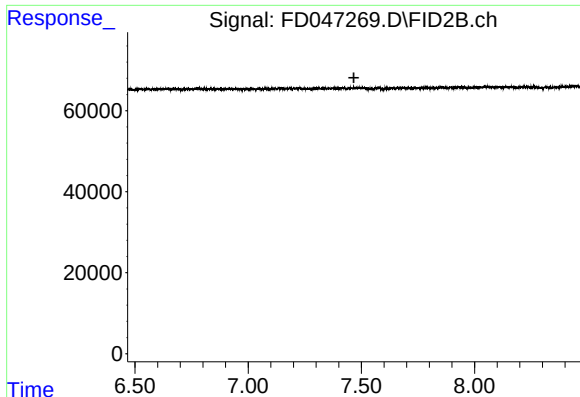

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T. : 7.467 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

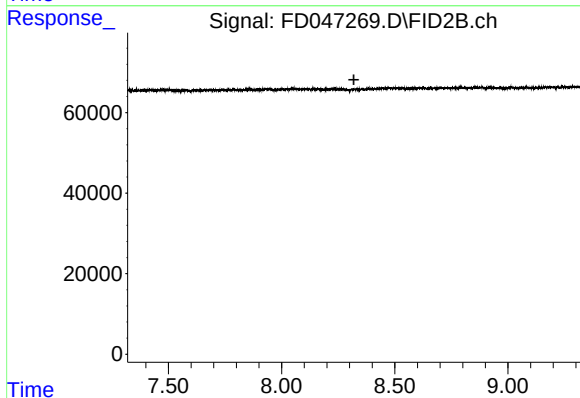


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 8.319 min
Response: 0
Conc: N.D.

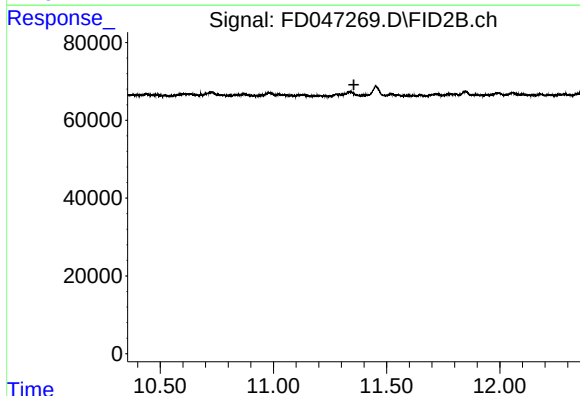


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.355 min
Response: 0
Conc: N.D.

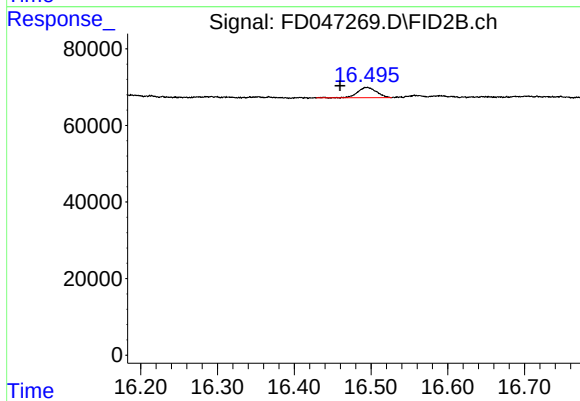

#18 Benzo[a]pyrene (C31.34)

R.T.: 16.495 min
Delta R.T.: 0.035 min
Response: 45318
Conc: 0.33 ug/ml

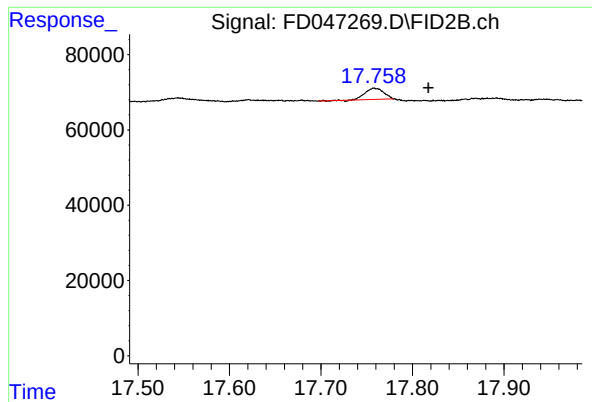

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 17.759 min
Delta R.T.: -0.059 min
Response: 42425
Conc: 0.34 ug/ml

Instrument :

FID_D

ClientSampleId :