

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030119\
 Data File : FB019982.D
 Signal(s) : FID2B.CH
 Acq On : 1 Mar 2019 5:10
 Operator : MJ/SJ
 Sample : 20 GRO STD
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 01 05:44:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
 Quant Title :
 QLast Update : Fri Mar 01 05:42:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.037	212385	20.000 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.893	582885	30.000 ng/ml
2) t 2,2,4-Trimethylpentane	7.651	559247	30.000 ng/ml
3) t n-Heptane	7.993	173430	10.000 ng/ml
4) t Benzene	8.129	200741	10.000 ng/ml
6) t Toluene	10.884	545871	30.000 ng/ml
7) t Ethylbenzene	13.336	217744	10.000 ng/ml
8) t m-Xylene	13.469	449742	20.000 ng/ml
9) t O-Xylene	14.200	448440	20.000 ng/ml
10) t 1,2,4-Trimethylbenzene	16.487	439569	20.000 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030119\
Data File : FB019982.D
Signal(s) : FID2B.CH
Acq On : 1 Mar 2019 5:10
Operator : MJ/SJ
Sample : 20 GRO STD
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 01 05:44:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
Quant Title :
QLast Update : Fri Mar 01 05:42:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

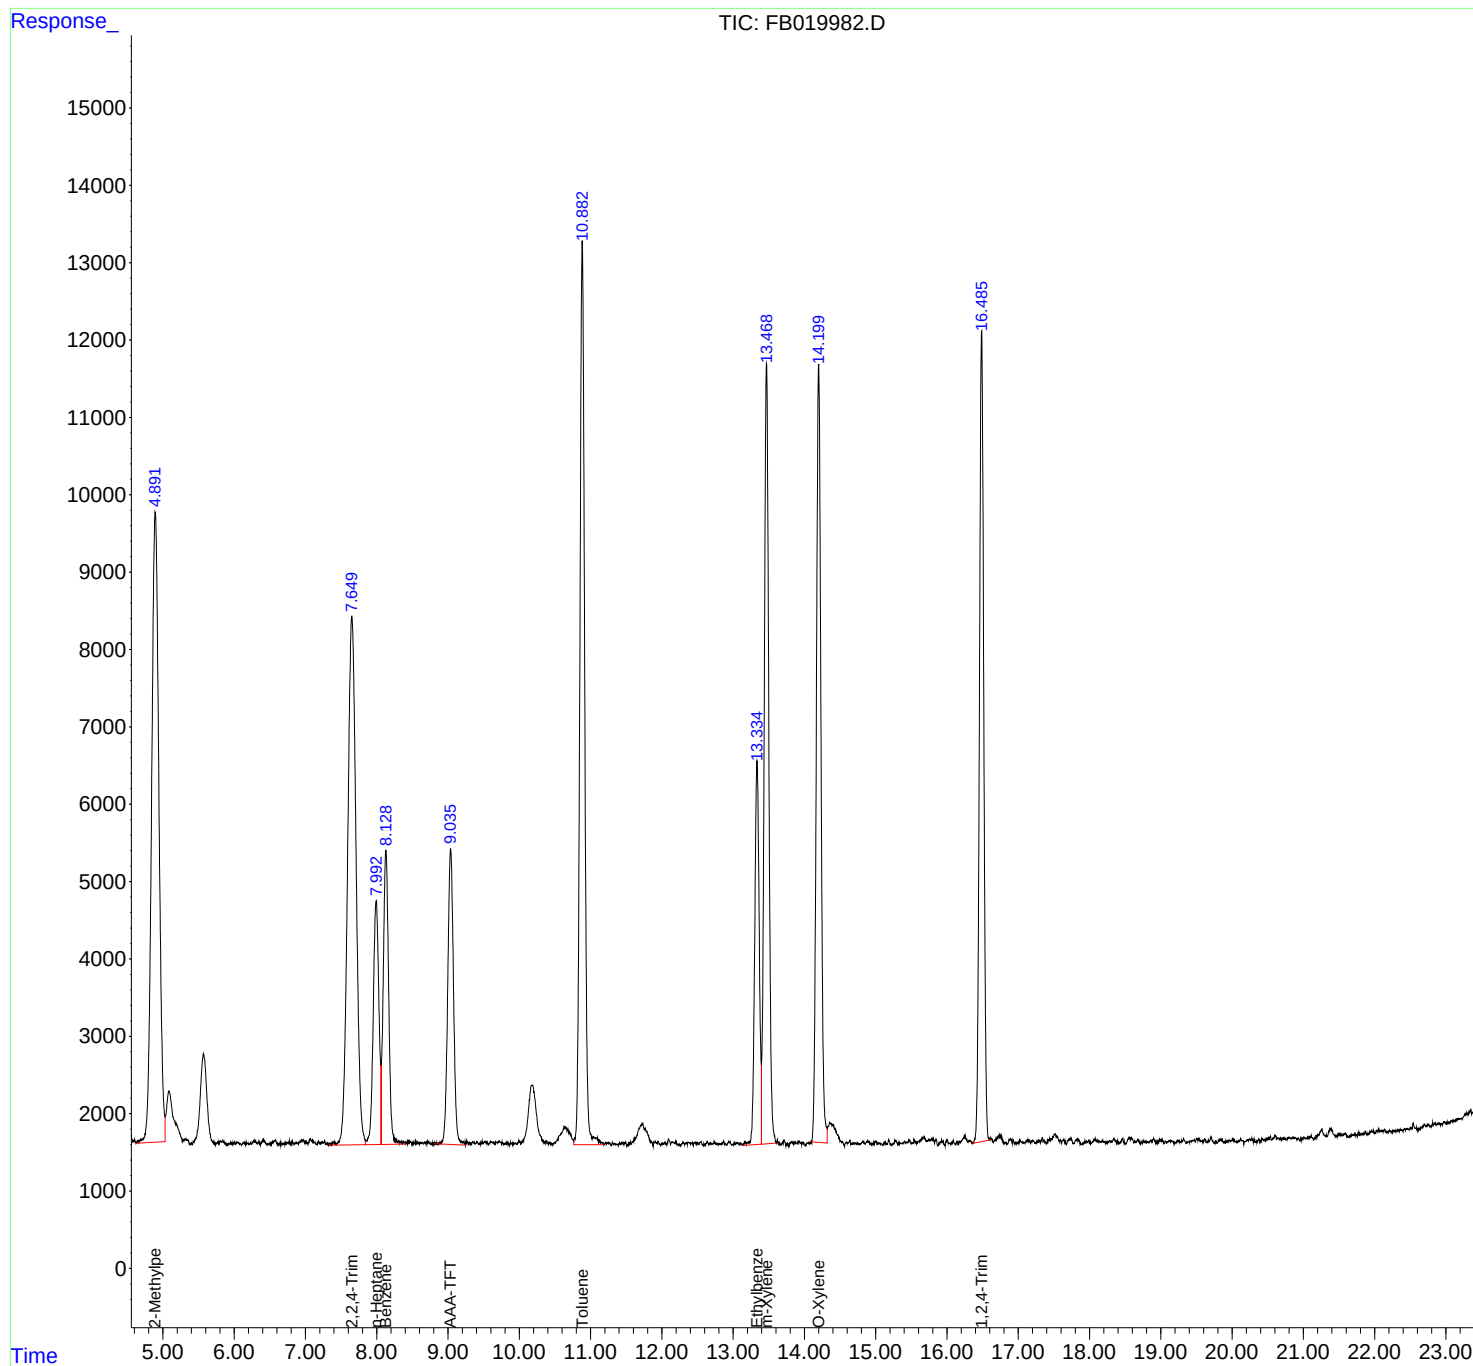


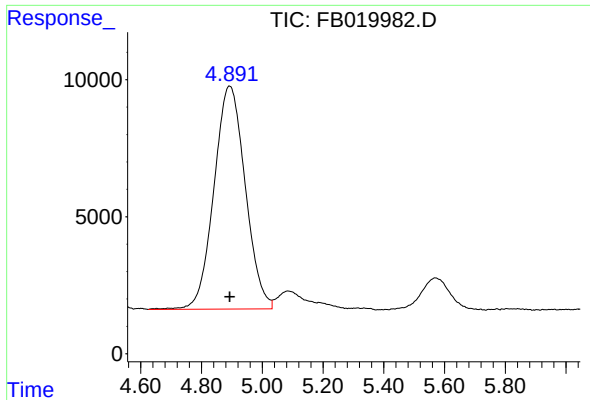

#1 2-Methylpentane


R.T.: 4.893 min
Delta R.T.: 0.000 min
Response: 582885
Conc: 30.00 ng/ml

Instrument :
FID_D
ClientSampleId :

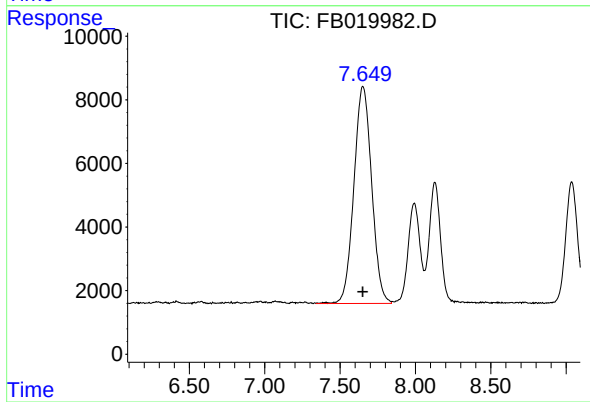


#2 2,2,4-Trimethylpentane

R.T.: 7.651 min
Delta R.T.: 0.000 min
Response: 559247
Conc: 30.00 ng/ml

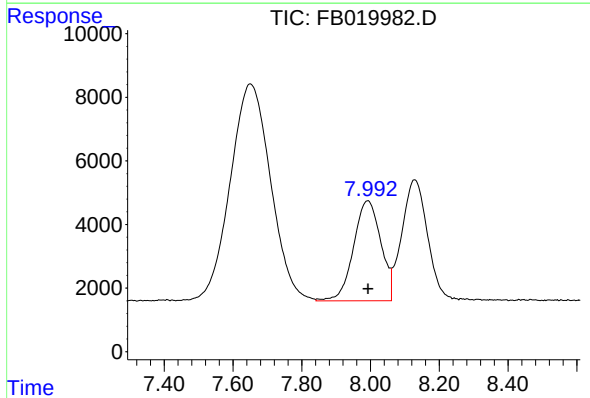


#3 n-Heptane

R.T.: 7.993 min
Delta R.T.: 0.000 min
Response: 173430
Conc: 10.00 ng/ml

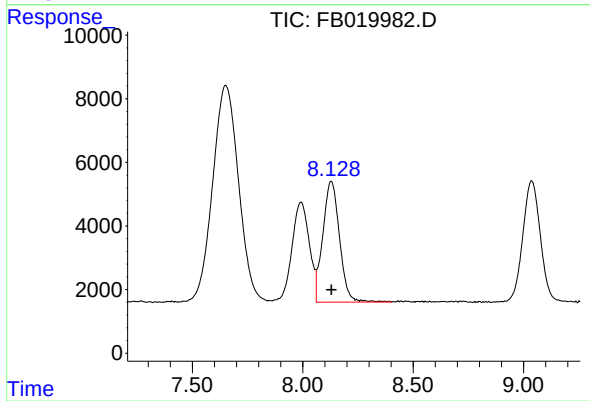

#4 Benzene


R.T.: 8.129 min
Delta R.T.: 0.000 min
Response: 200741
Conc: 10.00 ng/ml

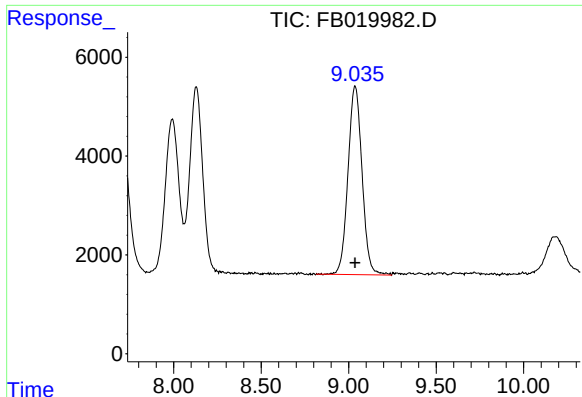

#5 AAA-TFT


R.T.: 9.037 min
Delta R.T.: 0.000 min
Response: 212385
Conc: 20.00 ng/ml

Instrument :
FID_D
ClientSampleId :

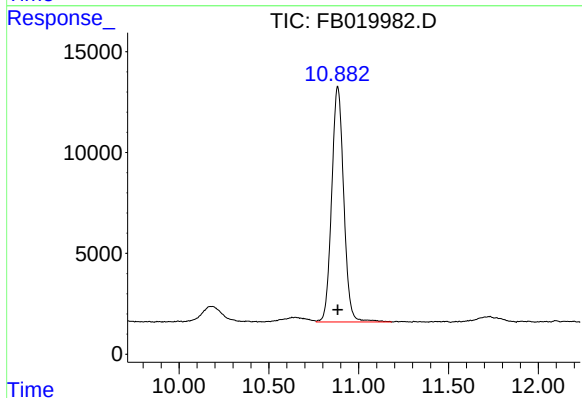


#6 Toluene

R.T.: 10.884 min
Delta R.T.: 0.000 min
Response: 545871
Conc: 30.00 ng/ml

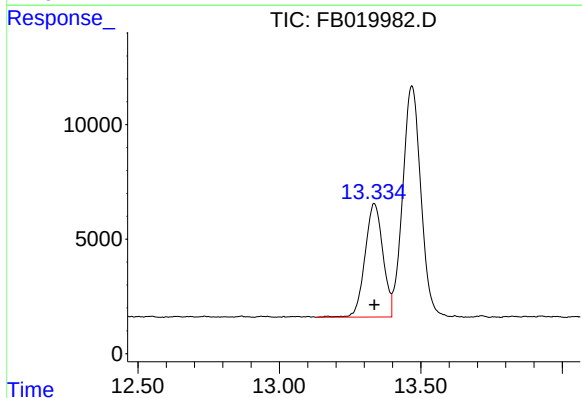


#7 Ethylbenzene

R.T.: 13.336 min
Delta R.T.: 0.000 min
Response: 217744
Conc: 10.00 ng/ml

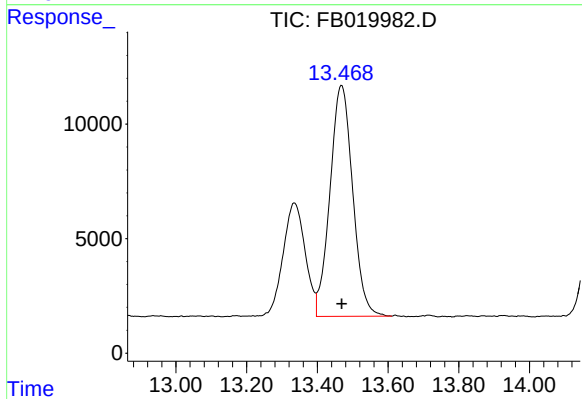

#8 m-Xylene


R.T.: 13.469 min
Delta R.T.: 0.000 min
Response: 449742
Conc: 20.00 ng/ml

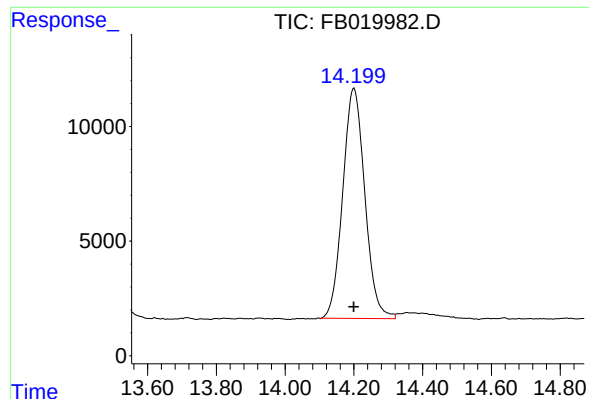

#9 O-Xylene

R.T.: 14.200 min
Delta R.T.: 0.000 min
Response: 448440
Conc: 20.00 ng/ml

Instrument :
FID_D
ClientSampleId :

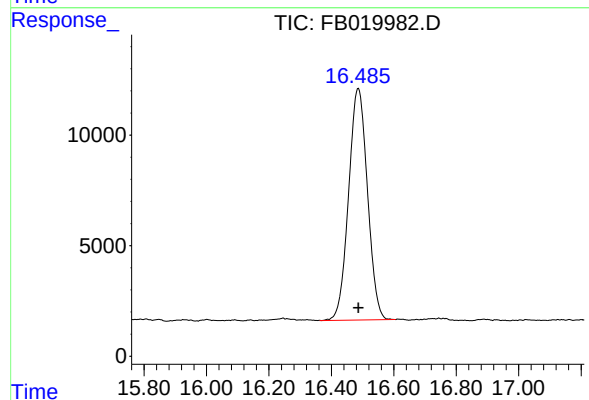

#10 1,2,4-Trimethylbenzene

R.T.: 16.487 min
Delta R.T.: 0.000 min
Response: 439569
Conc: 20.00 ng/ml