

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030119\
 Data File : FB019983.D
 Signal(s) : FID2B.CH
 Acq On : 1 Mar 2019 5:40
 Operator : MJ/SJ
 Sample : 50 GRO STD
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 01 05:59:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
 Quant Title :
 QLast Update : Fri Mar 01 05:42:31 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.074	533802	47.623 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.003	1619193	78.570 ng/ml
2) t 2,2,4-Trimethylpentane	7.709	1565717	78.369 ng/ml
3) t n-Heptane	8.043	476793	25.653 ng/ml
4) t Benzene	8.182	546149	26.101 ng/ml
6) t Toluene	10.907	1479956	77.691 ng/ml
7) t Ethylbenzene	13.346	584311	25.616 ng/ml
8) t m-Xylene	13.479	1208239	51.346 ng/ml
9) t O-Xylene	14.209	1195336	51.127 ng/ml
10) t 1,2,4-Trimethylbenzene	16.491	1166143	50.472 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030119\
Data File : FB019983.D
Signal(s) : FID2B.CH
Acq On : 1 Mar 2019 5:40
Operator : MJ/SJ
Sample : 50 GRO STD
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 01 05:59:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
Quant Title :
QLast Update : Fri Mar 01 05:42:31 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

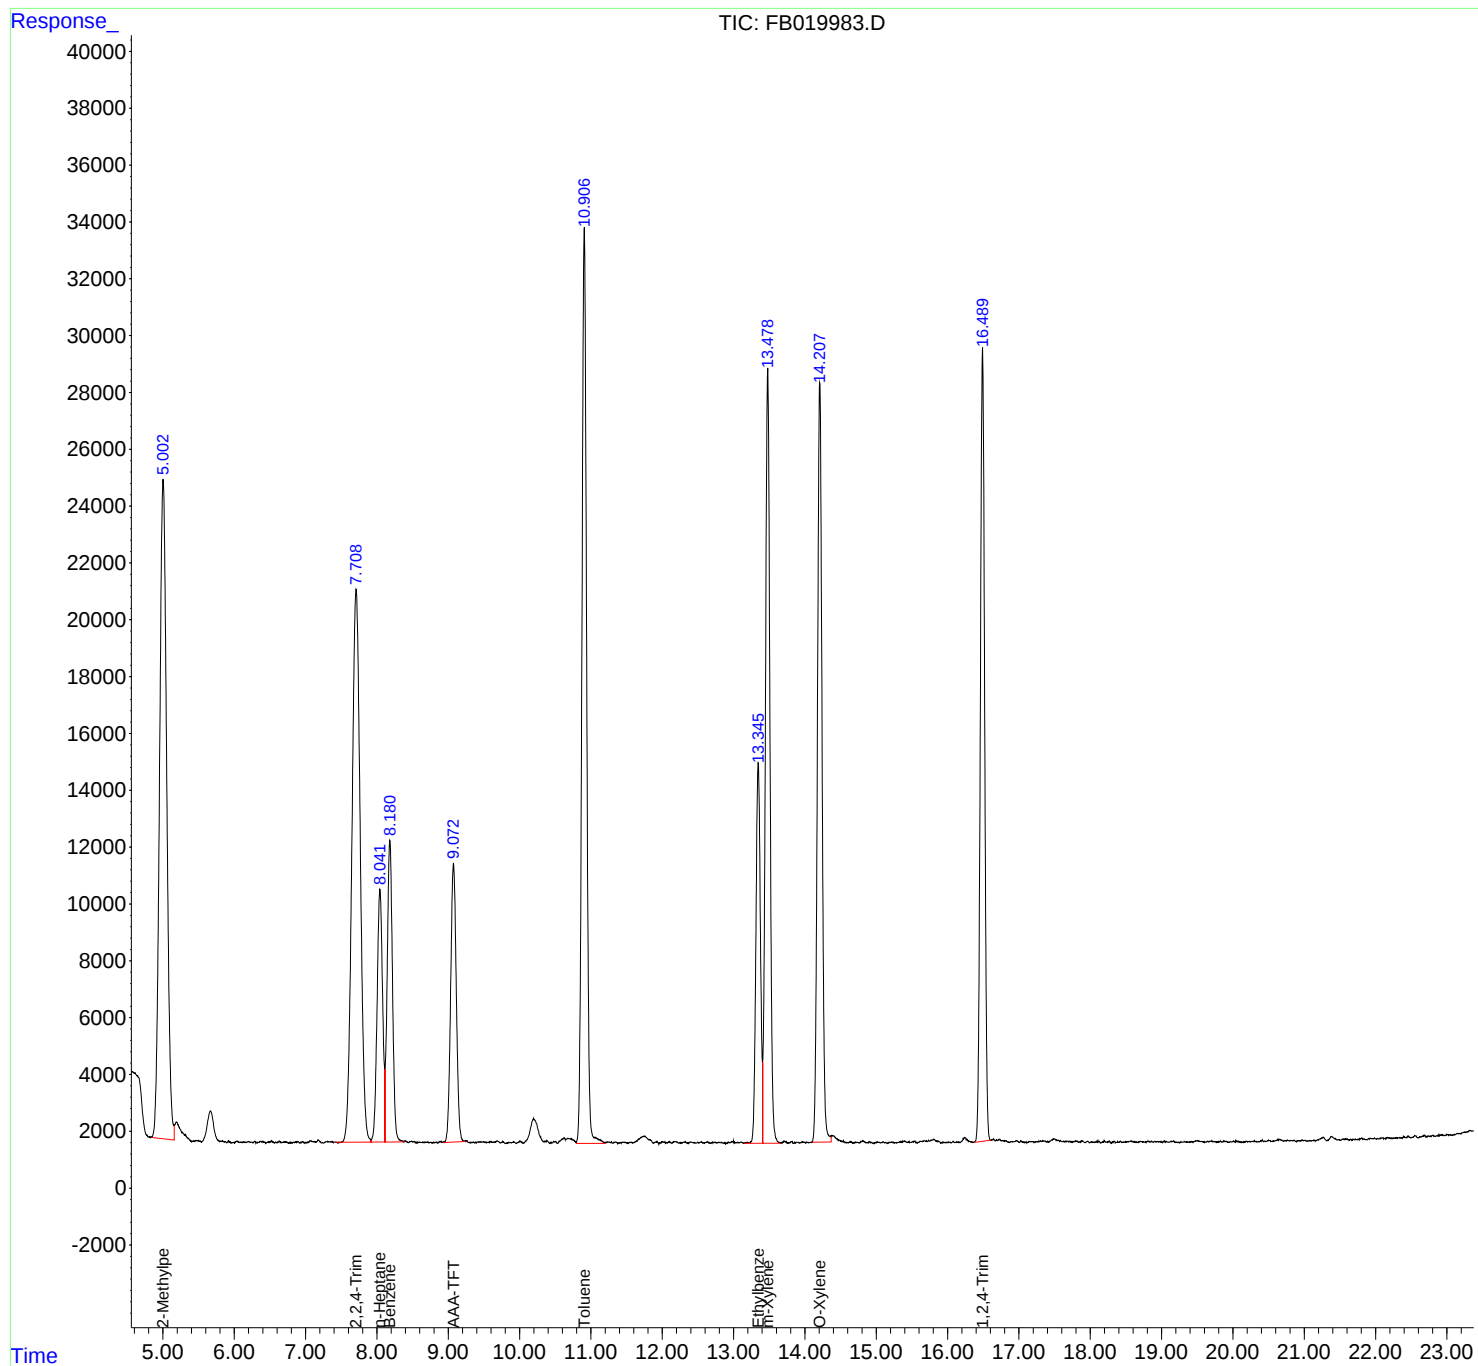


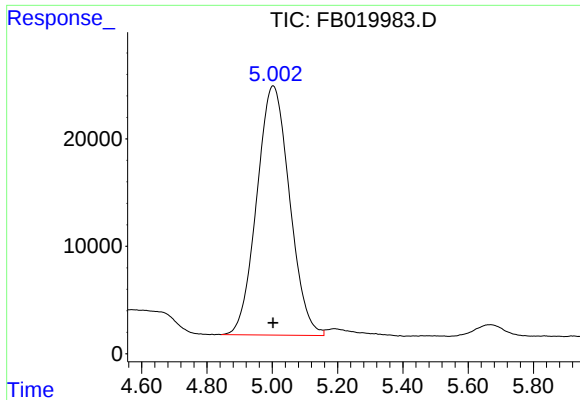

#1 2-Methylpentane


R.T.: 5.003 min
Delta R.T.: 0.001 min
Response: 1619193
Conc: 78.57 ng/ml

Instrument :
FID_D
ClientSampleId :

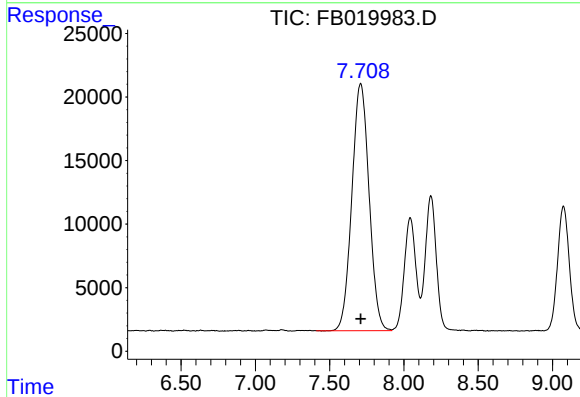


#2 2,2,4-Trimethylpentane

R.T.: 7.709 min
Delta R.T.: 0.000 min
Response: 1565717
Conc: 78.37 ng/ml

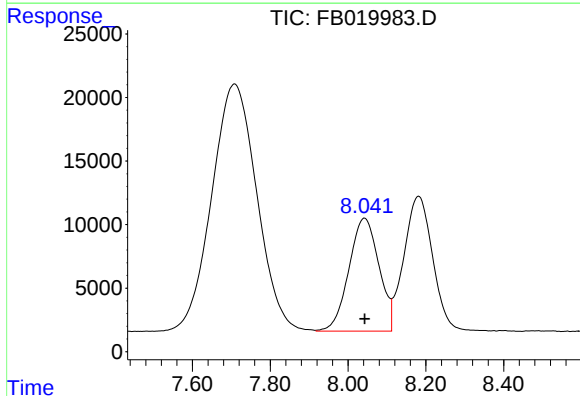


#3 n-Heptane

R.T.: 8.043 min
Delta R.T.: 0.000 min
Response: 476793
Conc: 25.65 ng/ml

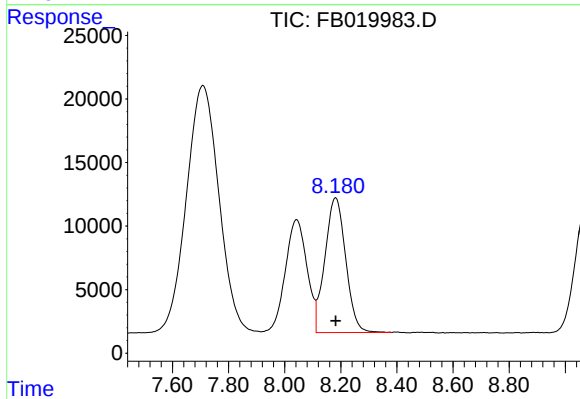

#4 Benzene


R.T.: 8.182 min
Delta R.T.: 0.000 min
Response: 546149
Conc: 26.10 ng/ml

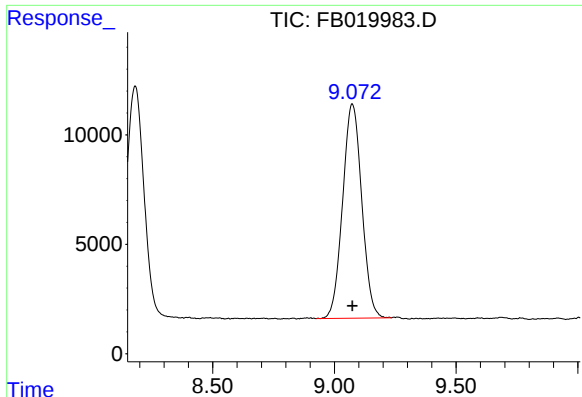

#5 AAA-TFT


R.T.: 9.074 min
Delta R.T.: 0.000 min
Response: 533802
Conc: 47.62 ng/ml

Instrument :
FID_D
ClientSampleId :

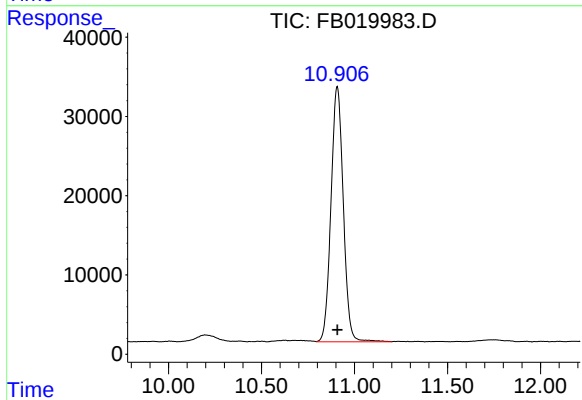


#6 Toluene

R.T.: 10.907 min
Delta R.T.: 0.000 min
Response: 1479956
Conc: 77.69 ng/ml

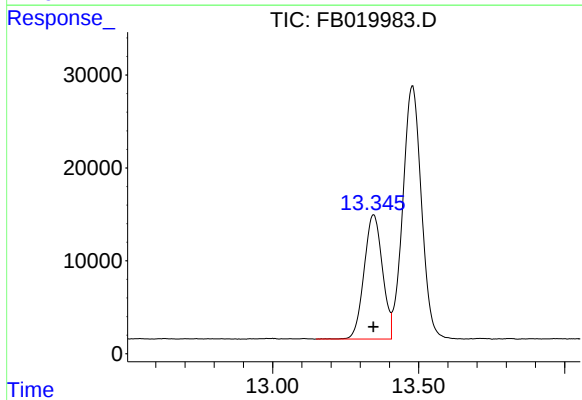


#7 Ethylbenzene

R.T.: 13.346 min
Delta R.T.: 0.000 min
Response: 584311
Conc: 25.62 ng/ml

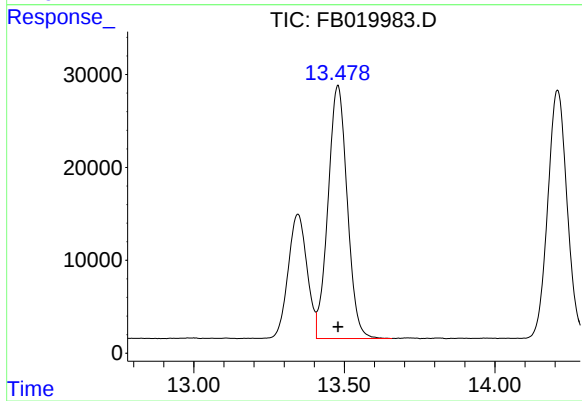

#8 m-Xylene


R.T.: 13.479 min
Delta R.T.: 0.000 min
Response: 1208239
Conc: 51.35 ng/ml

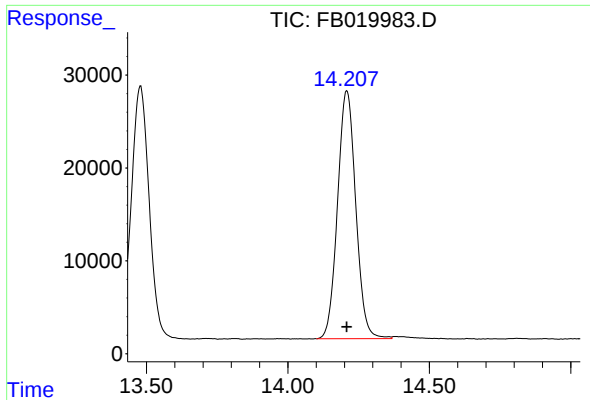

#9 O-Xylene

R.T.: 14.209 min
Delta R.T.: 0.000 min
Response: 1195336
Conc: 51.13 ng/ml

Instrument :
FID_D
ClientSampleId :

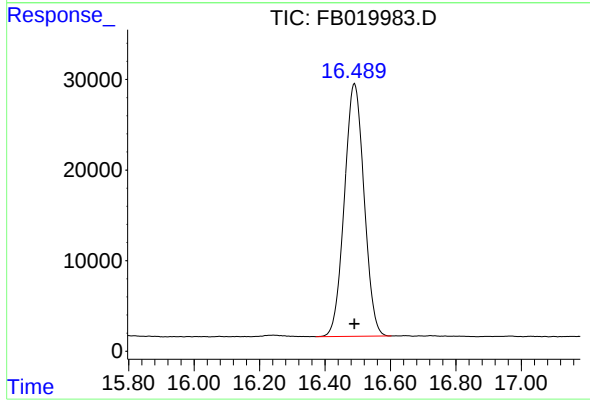

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min
Delta R.T.: 0.000 min
Response: 1166143
Conc: 50.47 ng/ml