

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030119\
 Data File : FB019984.D
 Signal(s) : FID2B.CH
 Acq On : 1 Mar 2019 6:10
 Operator : MJ/SJ
 Sample : 100 GRO STD
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 01 06:28:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
 Quant Title :
 QLast Update : Fri Mar 01 06:27:56 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.036	1119525	99.902 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.891	3225367	155.046 ng/ml
2) t 2,2,4-Trimethylpentane	7.651	3112138	154.582 ng/ml
3) t n-Heptane	7.992	945663	50.701 ng/ml
4) t Benzene	8.129	1055852	50.368 ng/ml
6) t Toluene	10.884	2784456	146.921 ng/ml
7) t Ethylbenzene	13.336	1115939	49.134 ng/ml
8) t m-Xylene	13.469	2311354	98.574 ng/ml
9) t O-Xylene	14.201	2290024	98.353 ng/ml
10) t 1,2,4-Trimethylbenzene	16.487	2270081	98.596 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB030119\
Data File : FB019984.D
Signal(s) : FID2B.CH
Acq On : 1 Mar 2019 6:10
Operator : MJ/SJ
Sample : 100 GRO STD
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 01 06:28:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030119.M
Quant Title :
QLast Update : Fri Mar 01 06:27:56 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

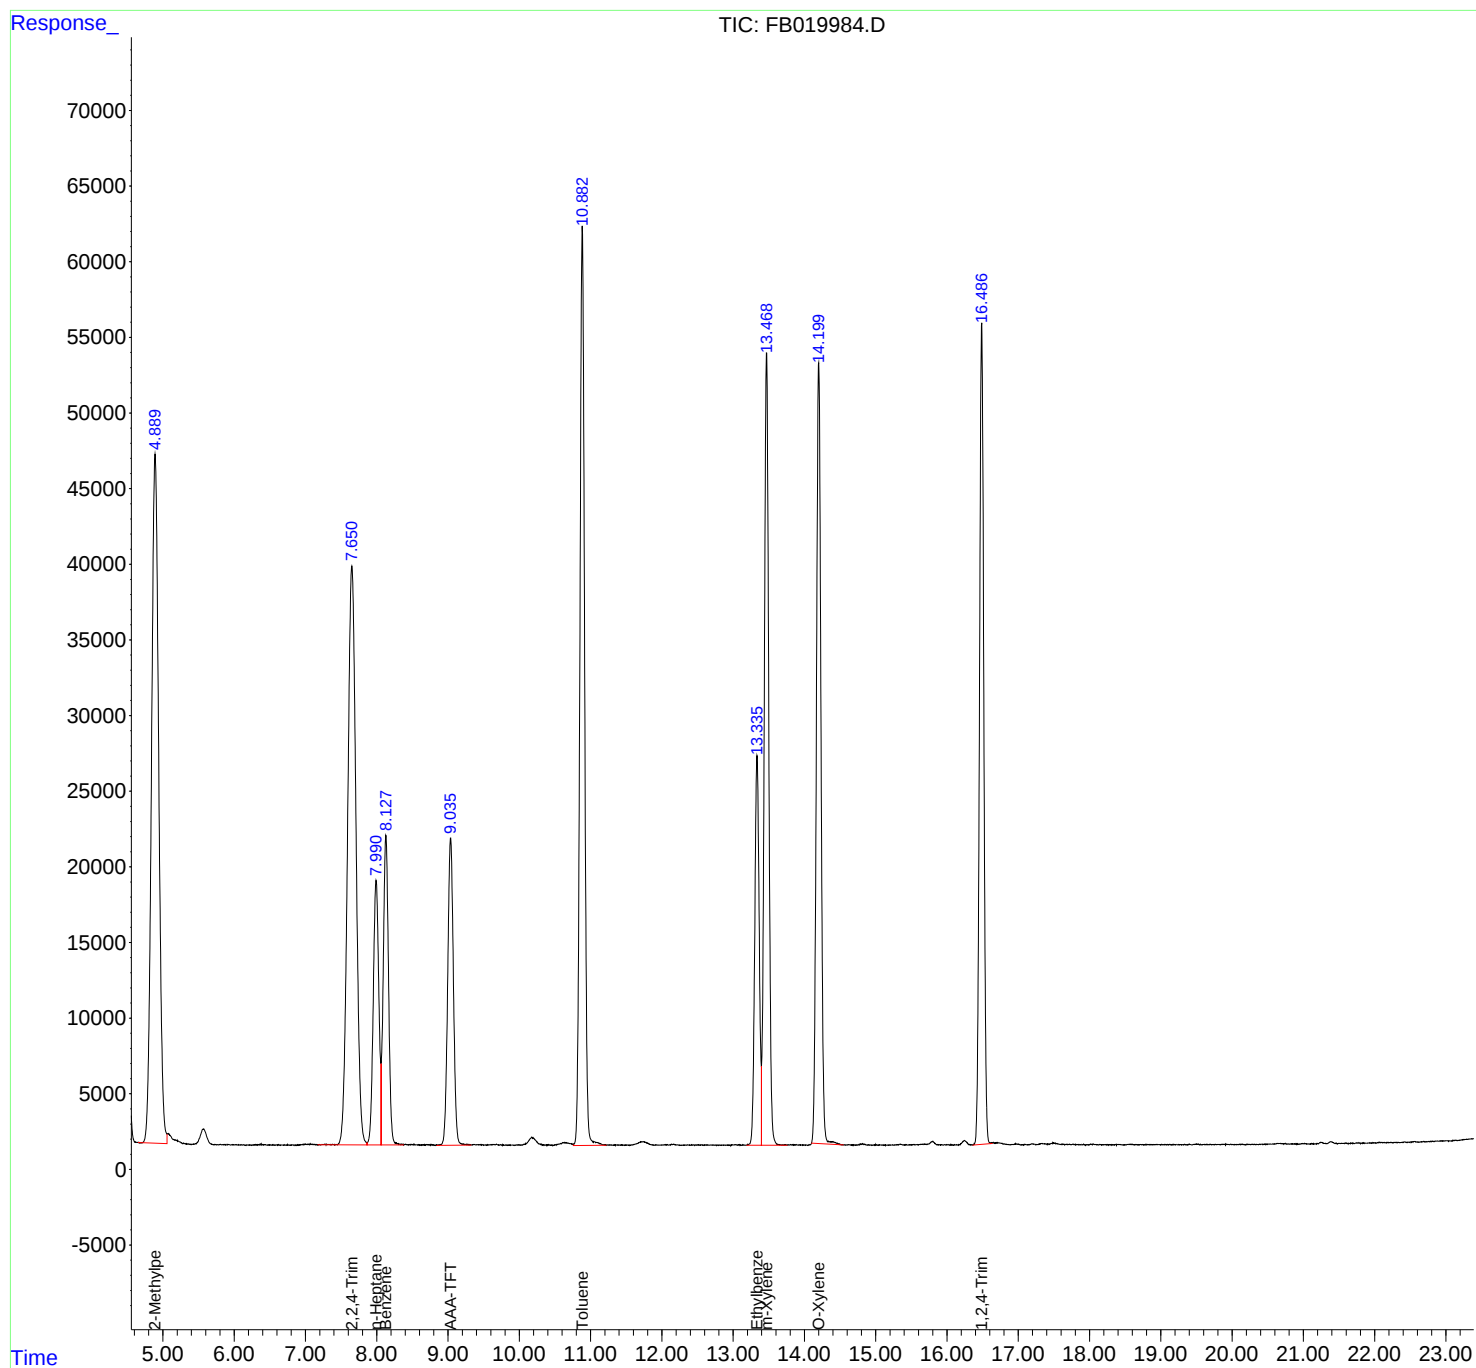


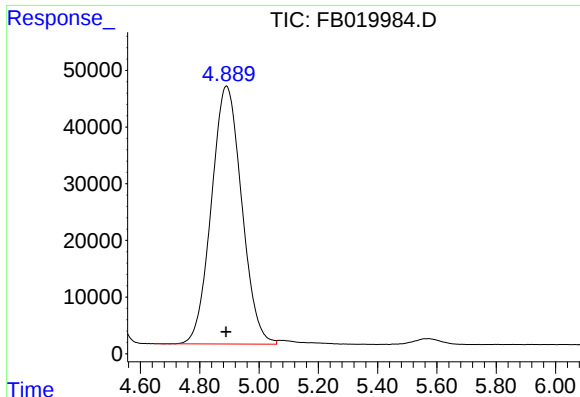

#1 2-Methylpentane


R.T.: 4.891 min
Delta R.T.: 0.002 min
Response: 3225367
Conc: 155.05 ng/ml

Instrument :
FID_D
ClientSampleId :

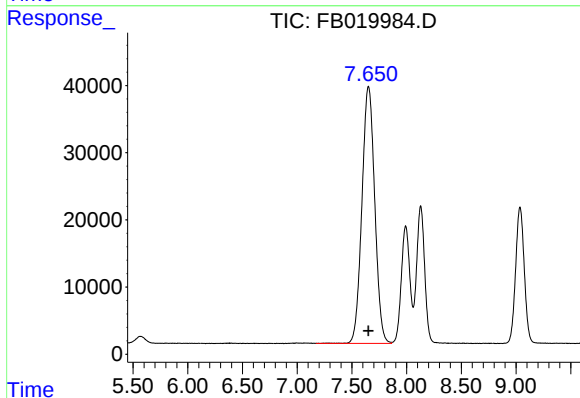


#2 2,2,4-Trimethylpentane

R.T.: 7.651 min
Delta R.T.: 0.000 min
Response: 3112138
Conc: 154.58 ng/ml

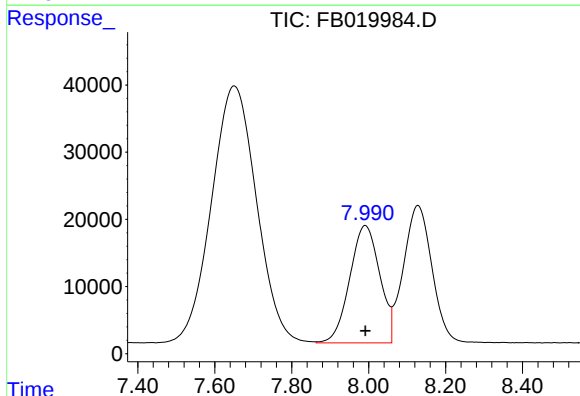


#3 n-Heptane

R.T.: 7.992 min
Delta R.T.: 0.000 min
Response: 945663
Conc: 50.70 ng/ml

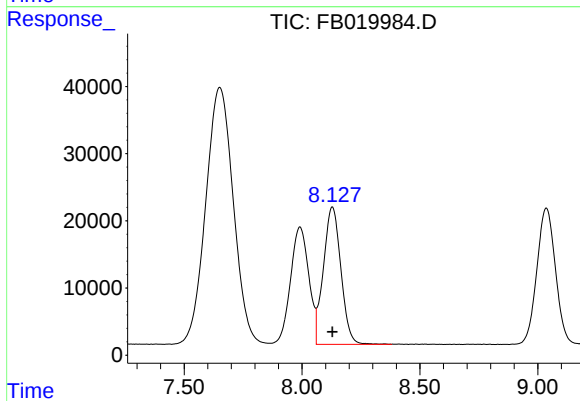

#4 Benzene


R.T.: 8.129 min
Delta R.T.: 0.000 min
Response: 1055852
Conc: 50.37 ng/ml

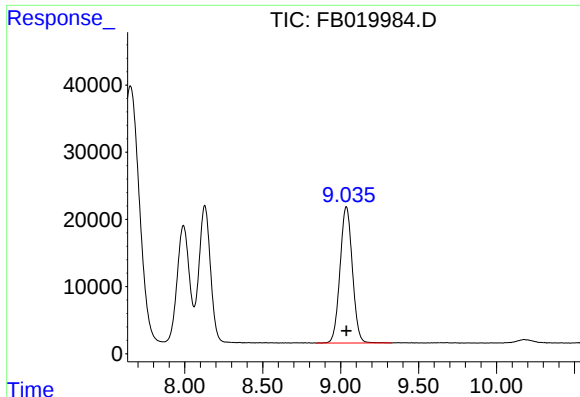

#5 AAA-TFT


R.T.: 9.036 min
Delta R.T.: 0.000 min
Response: 1119525
Conc: 99.90 ng/ml

Instrument :
FID_D
ClientSampleId :

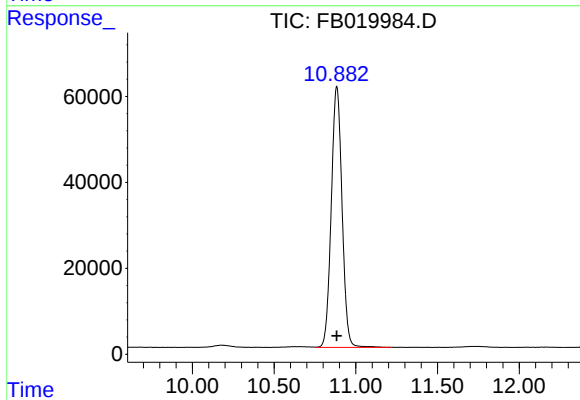


#6 Toluene

R.T.: 10.884 min
Delta R.T.: 0.000 min
Response: 2784456
Conc: 146.92 ng/ml

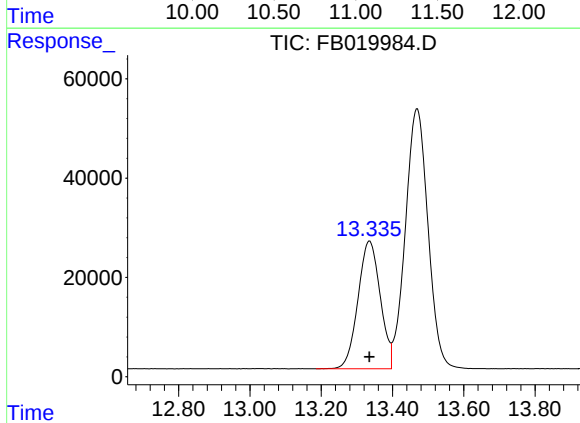


#7 Ethylbenzene

R.T.: 13.336 min
Delta R.T.: 0.000 min
Response: 1115939
Conc: 49.13 ng/ml

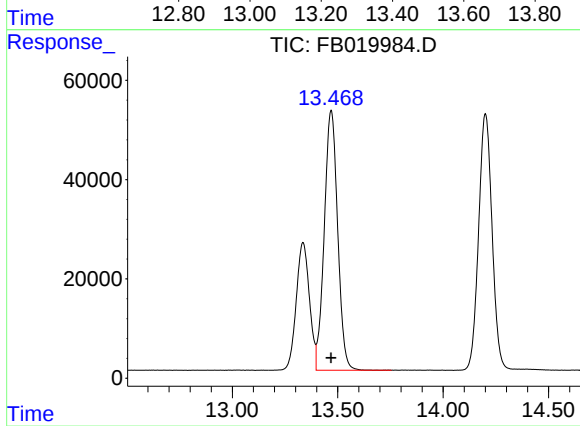

#8 m-Xylene


R.T.: 13.469 min
Delta R.T.: 0.000 min
Response: 2311354
Conc: 98.57 ng/ml

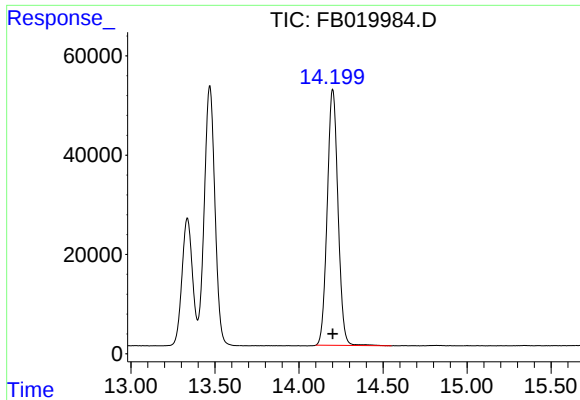

#9 O-Xylene

R.T.: 14.201 min
Delta R.T.: 0.000 min
Response: 2290024
Conc: 98.35 ng/ml

Instrument :
FID_D
ClientSampleId :

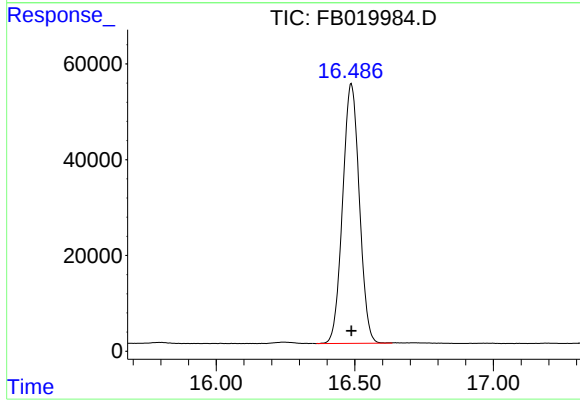

#10 1,2,4-Trimethylbenzene

R.T.: 16.487 min
Delta R.T.: 0.000 min
Response: 2270081
Conc: 98.60 ng/ml