

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD022819AR\
 Data File : FD028011.D
 Signal(s) : FID2B.CH
 Acq On : 28 Feb 2019 20:32
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Mar 01 04:09:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 022819.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 01 04:06:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

12) T	Fluoranthene (C21.85)	12.213	53426	0.492 ug/ml
14) T	Benzo[a]anthracene (C...	14.338f	314293	3.105 ug/ml
15) T	Chrysene (C27.41)	14.460	69582	0.675 ug/ml
16) T	benzo[b]fluoranthene ...	15.992f	147855	1.403 ug/ml
17) T	Bnezo[k]fluoranthene ...	15.992	147855	1.373 ug/ml
20) T	Dibenz[a,h]anthracene...	17.756f	176302	1.750 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD022819AR\
Data File : FD028011.D
Signal(s) : FID2B.CH
Acq On : 28 Feb 2019 20:32
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 01 04:09:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 022819.M
Quant Title : GC Extractables
QLast Update : Fri Mar 01 04:06:35 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

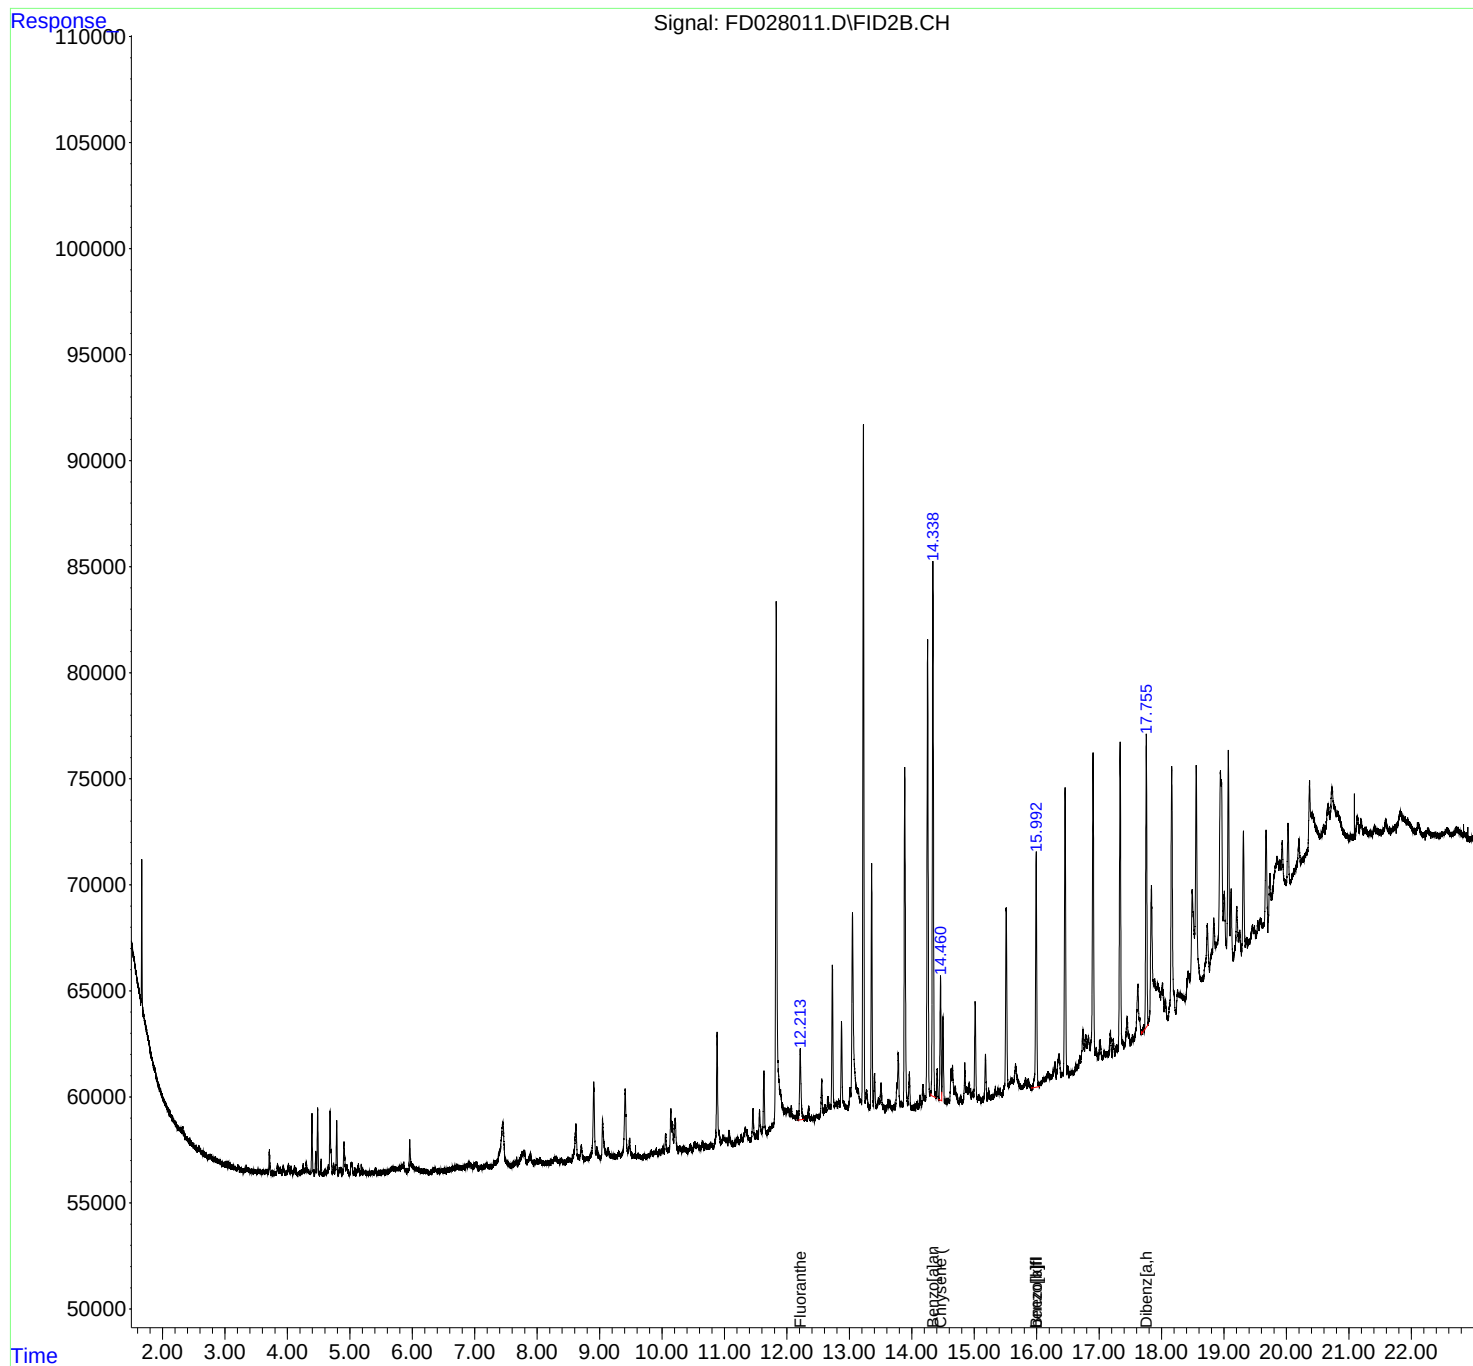


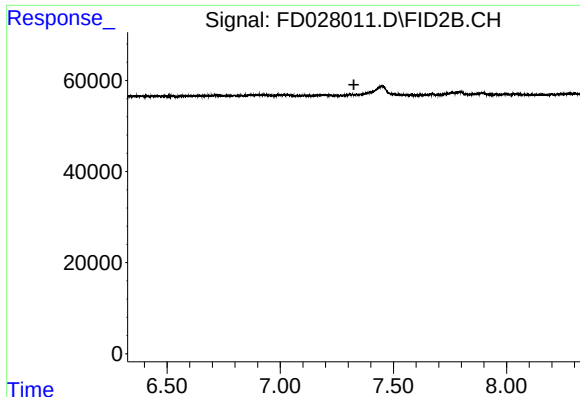

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T. : 7.325 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :
I.BLK

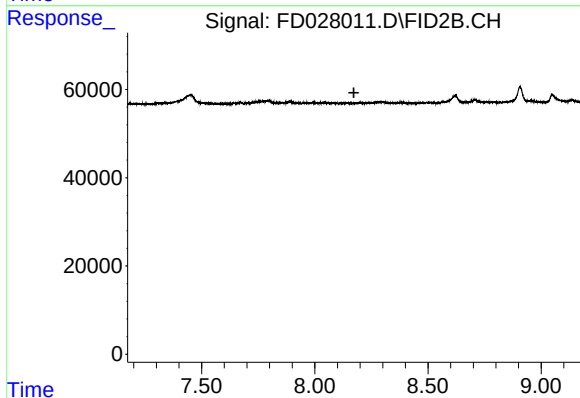


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 8.173 min
Response: 0
Conc: N.D.

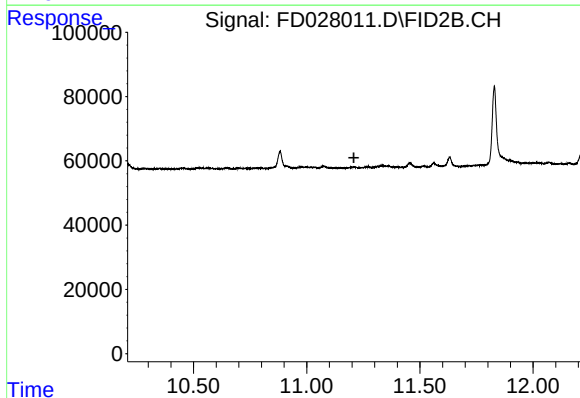


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.208 min
Response: 0
Conc: N.D.

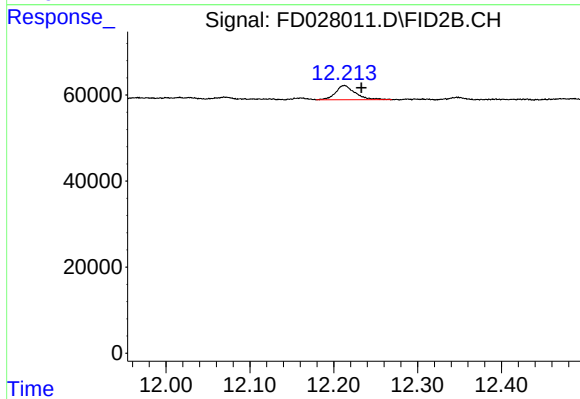

#12 Fluoranthene (C21.85)


R.T.: 12.213 min
Delta R.T.: -0.021 min
Response: 53426
Conc: 0.49 ug/ml

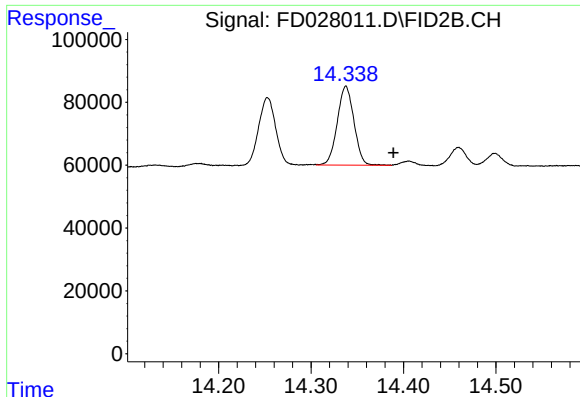

#14 Benzo[a]anthracene (C26.37)


R.T.: 14.338 min
Delta R.T.: -0.051 min
Response: 314293
Conc: 3.11 ug/ml

Instrument :
FID_D
ClientSampleId :
I.BLK

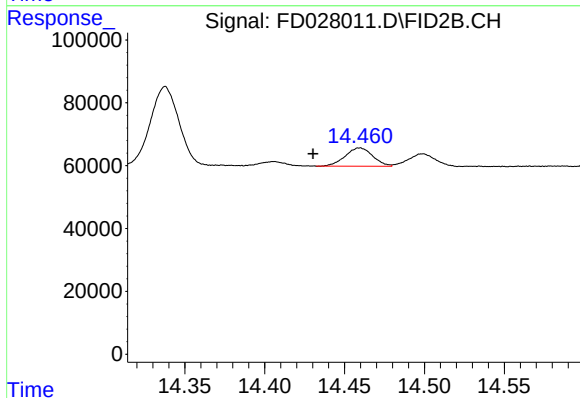


#15 Chrysene (C27.41)

R.T.: 14.460 min
Delta R.T.: 0.029 min
Response: 69582
Conc: 0.67 ug/ml

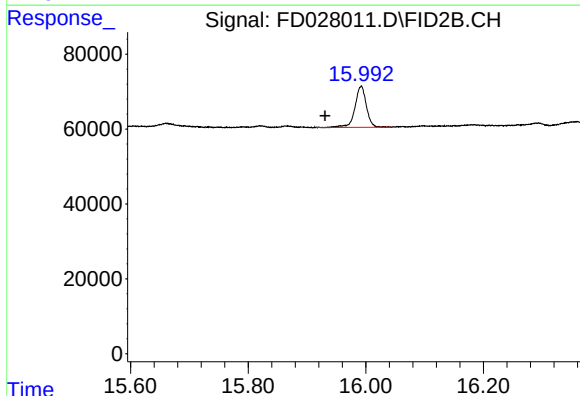


#16 benzo[b]fluoranthene (C30.41)

R.T.: 15.992 min
Delta R.T.: 0.061 min
Response: 147855
Conc: 1.40 ug/ml

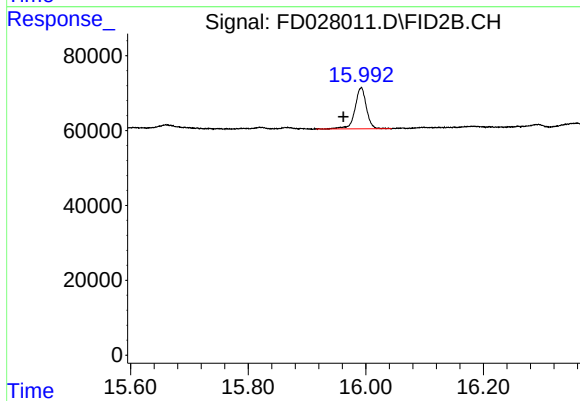

#17 Bnezo[k]fluoranthene (C30.14)

R.T.: 15.992 min
Delta R.T.: 0.030 min
Response: 147855
Conc: 1.37 ug/ml

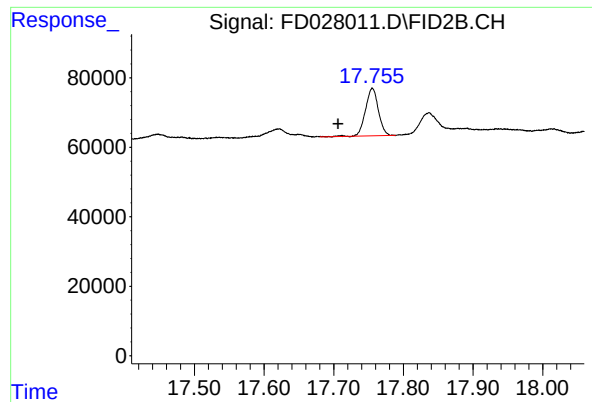

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 17.756 min
Delta R.T.: 0.049 min
Response: 176302
Conc: 1.75 ug/ml

Instrument :
FID_D
ClientSampleId :
I.BLK