

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD030123AR\
 Data File : FD045190.D
 Signal(s) : FID2B.ch
 Acq On : 01 Mar 2023 07:59
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 01 15:42:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 030123.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 01 14:05:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

14) T	Benzo[a]anthracene (C...	14.673	66524	0.522 ug/ml
15) T	Chrysene (C27.41)	14.673	66524	0.510 ug/ml
17) T	Bnezo[k]fluoranthene ...	16.273	55329	0.438 ug/ml
19) T	Indeno[1,2,3-cd]pyren...	17.949	139558	1.167 ug/ml
20) T	Dibenz[a,h]anthracene...	17.949	139558	1.157 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD030123AR\
Data File : FD045190.D
Signal(s) : FID2B.ch
Acq On : 01 Mar 2023 07:59
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 01 15:42:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aromatic EPH 030123.M
Quant Title : GC Extractables
QLast Update : Wed Mar 01 14:05:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

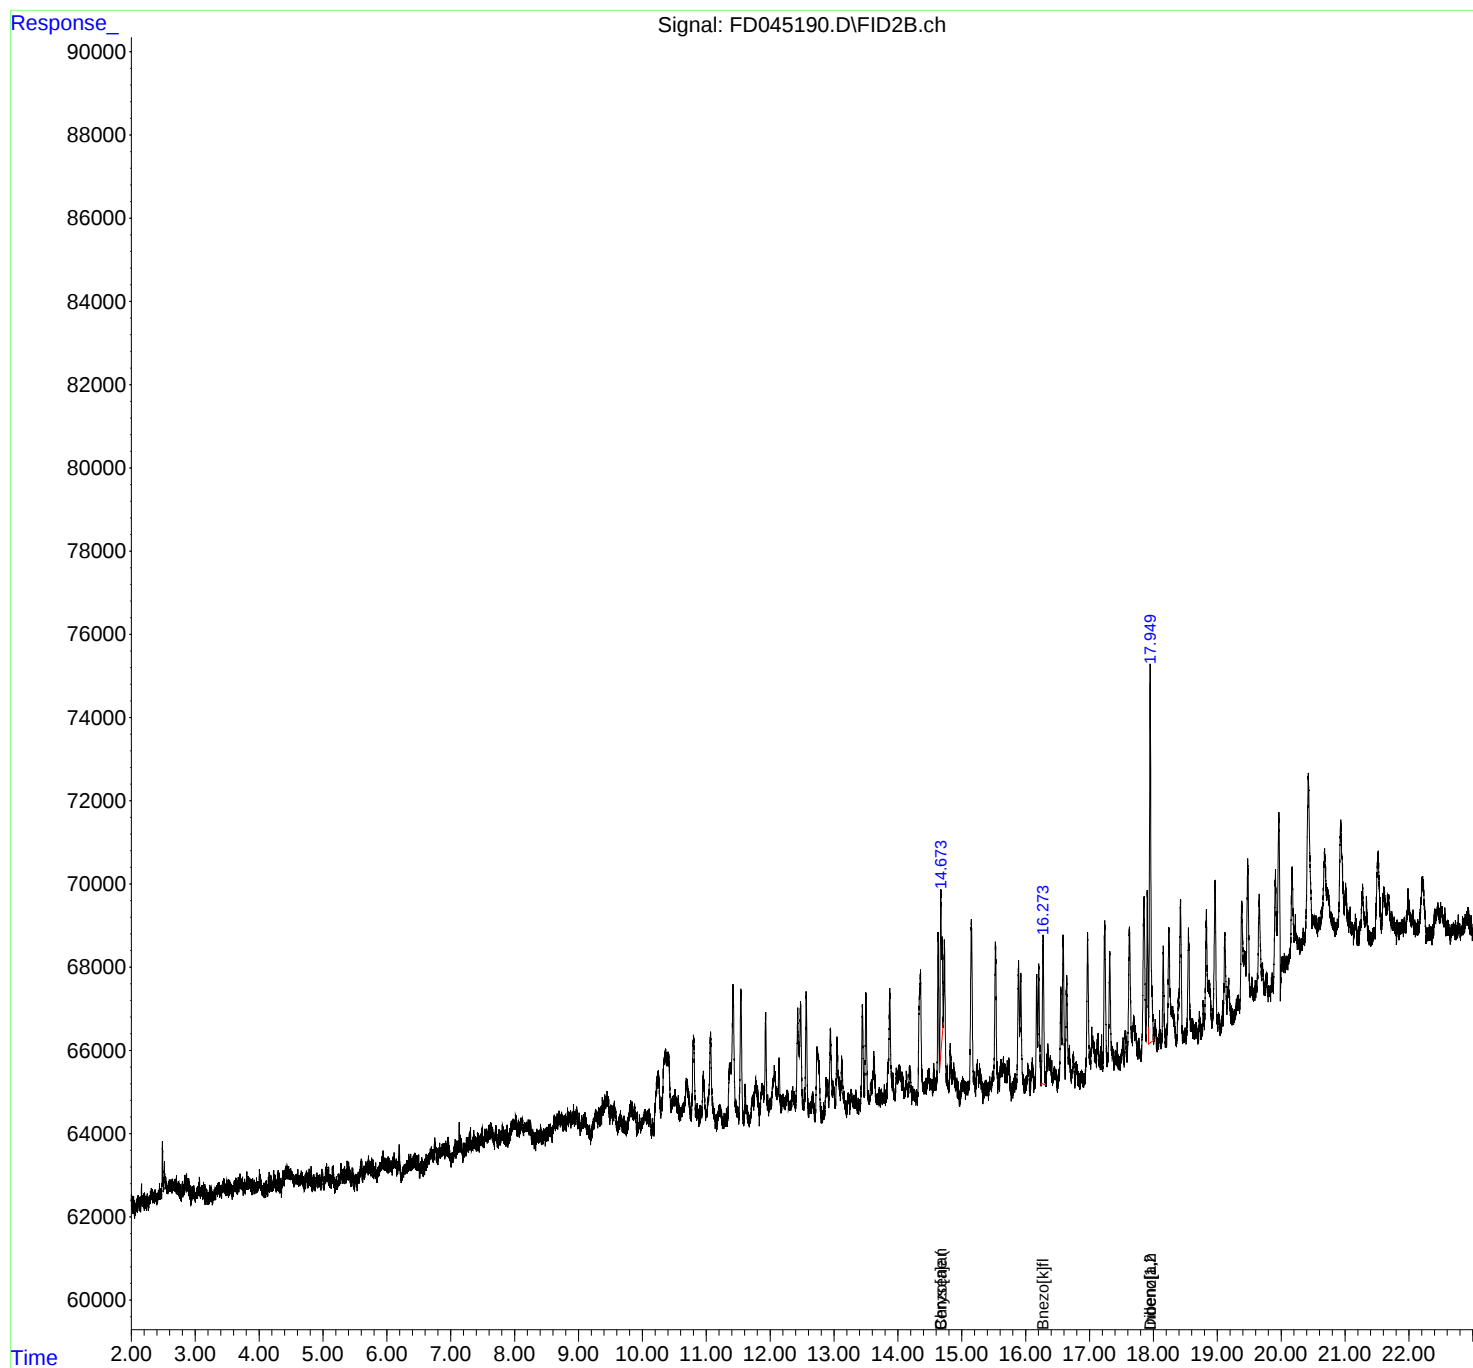


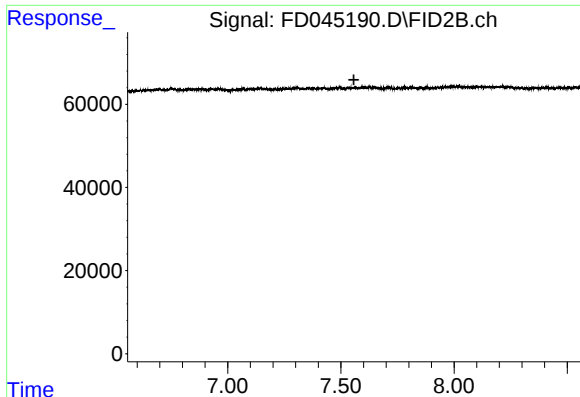

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T. : 7.558 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

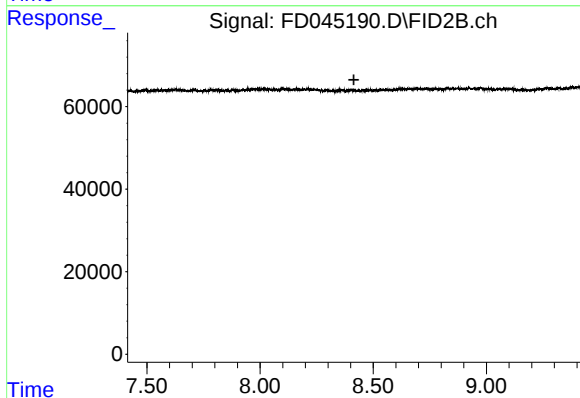


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 8.415 min
Response: 0
Conc: N.D.

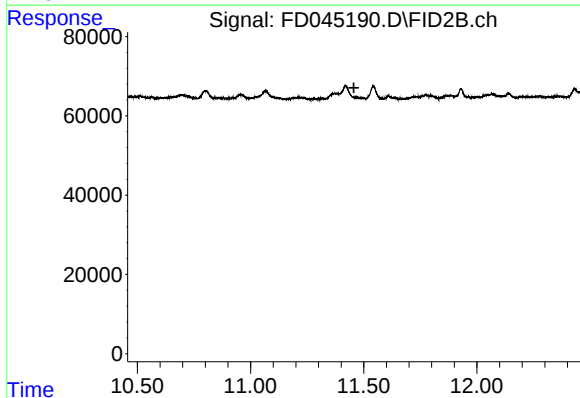


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.457 min
Response: 0
Conc: N.D.

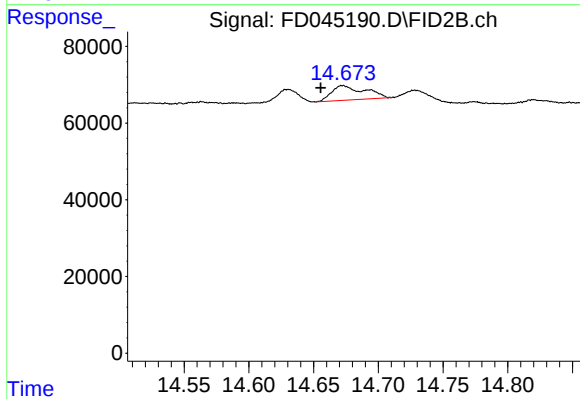

#14 Benzo[a]anthracene (C26.37)


R.T.: 14.673 min
Delta R.T.: 0.017 min
Response: 66524
Conc: 0.52 ug/ml

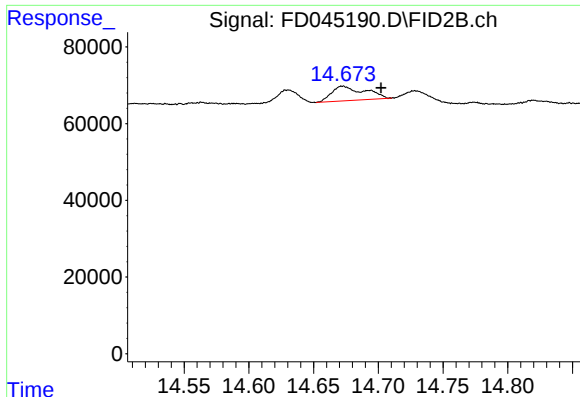

#15 Chrysene (C27.41)


R.T.: 14.673 min
Delta R.T.: -0.029 min
Response: 66524
Conc: 0.51 ug/ml

Instrument :
FID_D
ClientSampleId :

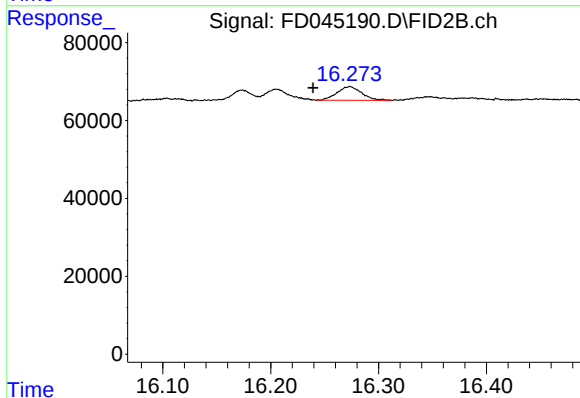


#17 Bnezo[k]fluoranthene (C30.14)

R.T.: 16.273 min
Delta R.T.: 0.034 min
Response: 55329
Conc: 0.44 ug/ml

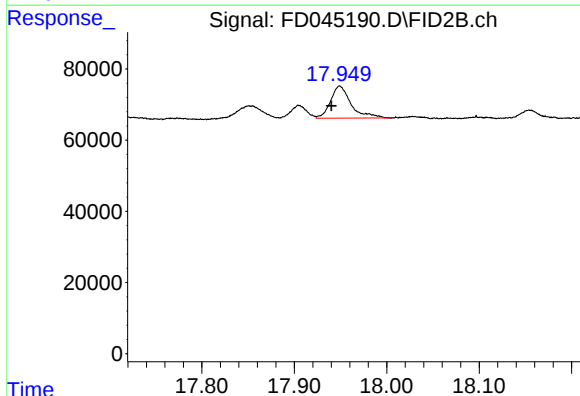

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 17.949 min
Delta R.T.: 0.009 min
Response: 139558
Conc: 1.17 ug/ml

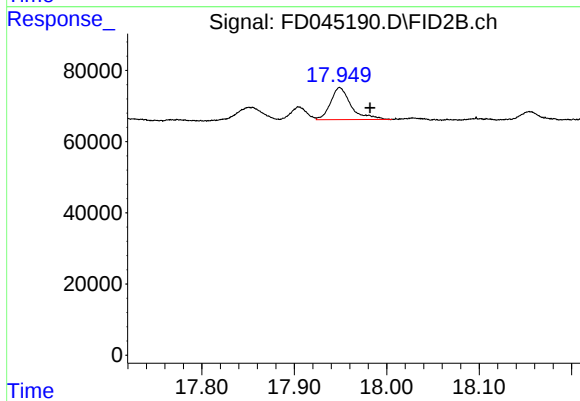

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 17.949 min
Delta R.T.: -0.033 min
Response: 139558
Conc: 1.16 ug/ml