

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD030222AL\
 Data File : FD041345.D
 Signal(s) : FID2B.CH
 Acq On : 02 Mar 2022 9:01
 Operator : UA/NP
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 03 01:11:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 022322.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 24 01:21:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.238	130140	0.838 ug/ml
11) T	n-Heneicosane (C21)	12.860	538600	3.440 ug/ml
13) T	n-Docosane (C22)	13.434	76194	0.487 ug/ml
14) T	n-Tetracosane (C24)	14.532	50936	0.325 ug/ml
15) T	n-Hexacosane (C26)	15.548	66693	0.434 ug/ml
16) T	n-Octacosane (C28)	16.492	54883	0.369 ug/ml
17) T	n-Tricontane (C30)	17.374	56809	0.404 ug/ml
18) T	n-Dotriacontane (C32)	18.201	28174	0.221 ug/ml
19) T	n-Tetratriacontane (C34)	18.985	41078	0.361 ug/ml
20) T	n-Hexatriacontane (C36)	19.727	943	0.009 ug/ml
21) T	n-Octatriacontane (C38)	20.359f	61494	0.648 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD030222AL\
Data File : FD041345.D
Signal(s) : FID2B.CH
Acq On : 02 Mar 2022 9:01
Operator : UA/NP
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 03 01:11:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 022322.M
Quant Title : GC Extractables
QLast Update : Thu Feb 24 01:21:33 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

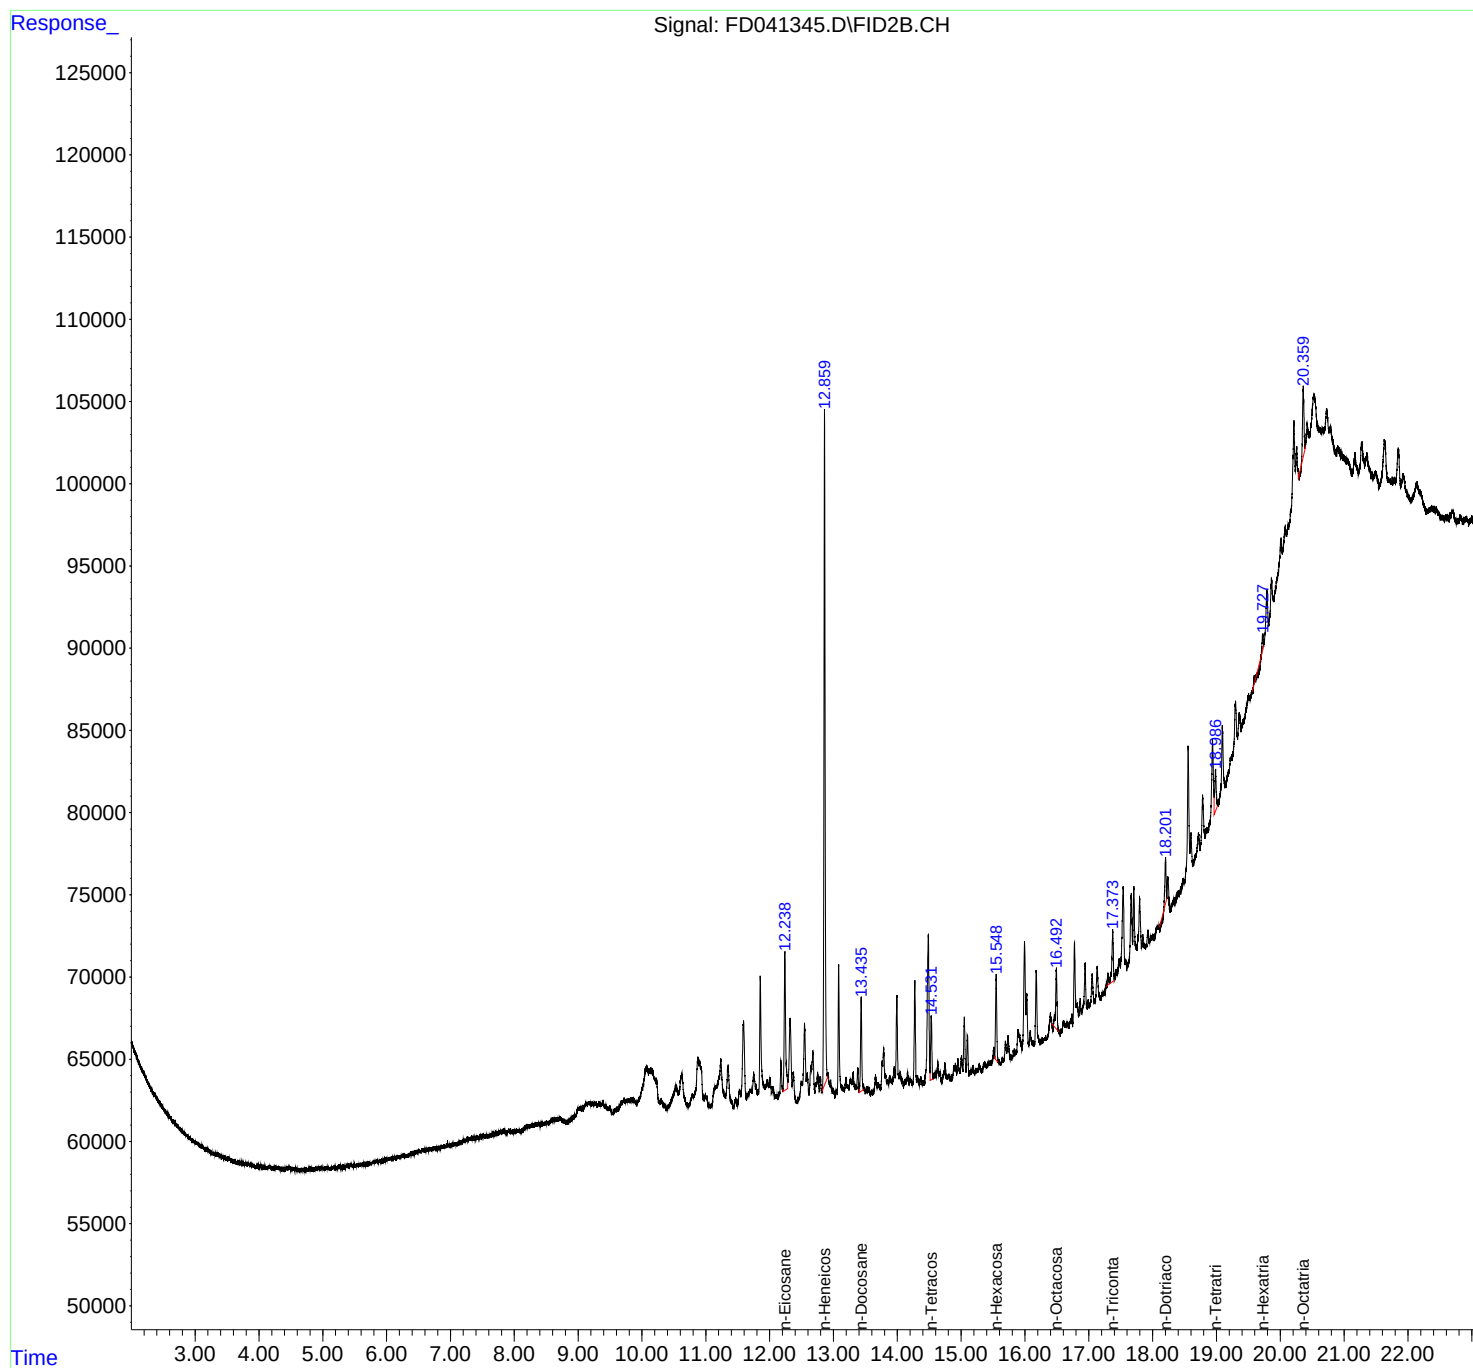


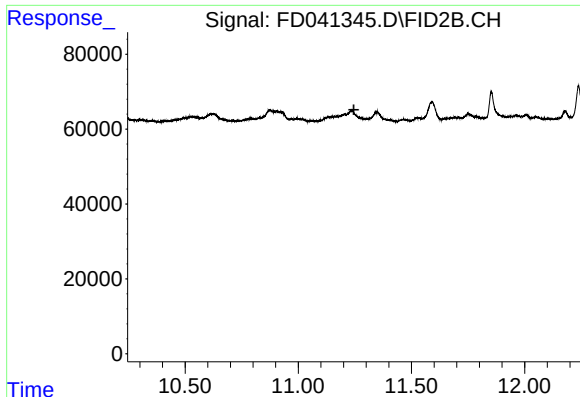

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.246 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

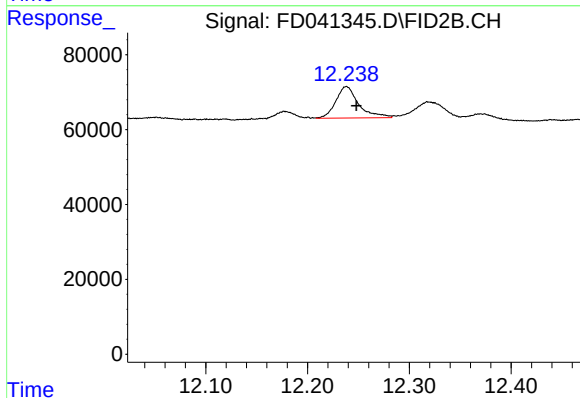


#10 n-Eicosane (C20)

R.T.: 12.238 min
Delta R.T.: -0.010 min
Response: 130140
Conc: 0.84 ug/ml

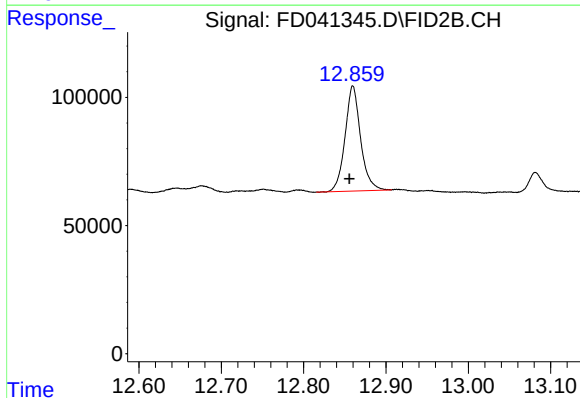


#11 n-Heneicosane (C21)

R.T.: 12.860 min
Delta R.T.: 0.004 min
Response: 538600
Conc: 3.44 ug/ml

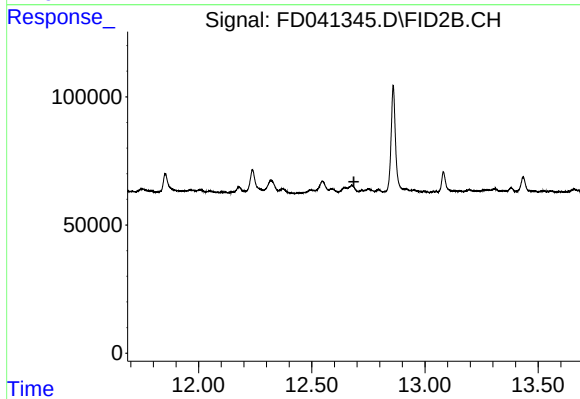

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T. : 12.686 min
Response: 0
Conc: N.D.

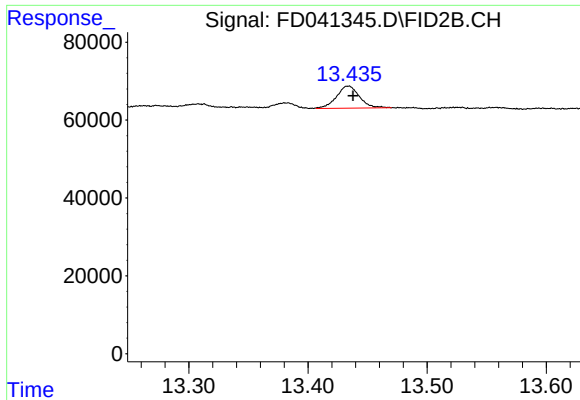

#13 n-Docosane (C22)


R.T.: 13.434 min
Delta R.T.: -0.004 min
Response: 76194
Conc: 0.49 ug/ml

Instrument :
FID_D
ClientSampleId :

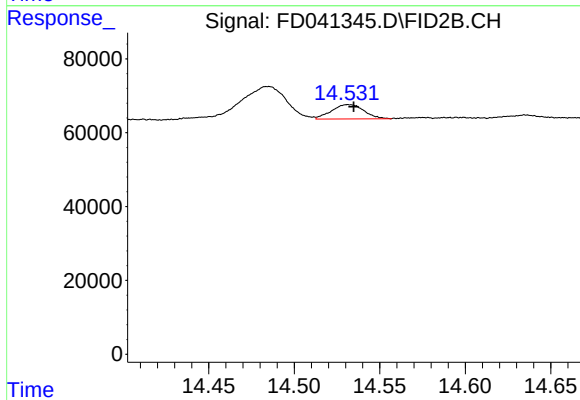


#14 n-Tetracosane (C24)

R.T.: 14.532 min
Delta R.T.: -0.003 min
Response: 50936
Conc: 0.32 ug/ml

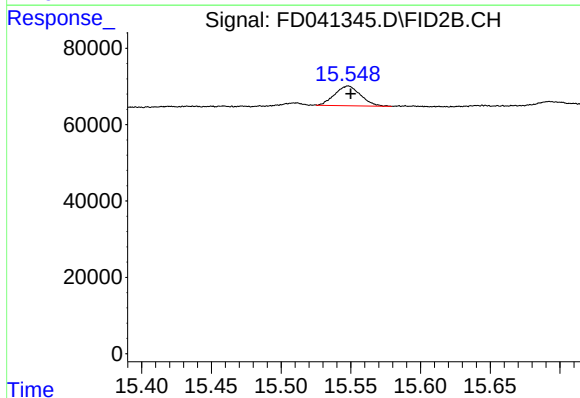


#15 n-Hexacosane (C26)

R.T.: 15.548 min
Delta R.T.: -0.002 min
Response: 66693
Conc: 0.43 ug/ml

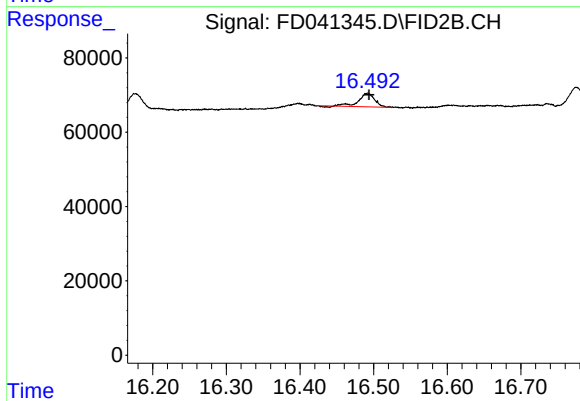

#16 n-Octacosane (C28)


R.T.: 16.492 min
Delta R.T.: -0.003 min
Response: 54883
Conc: 0.37 ug/ml

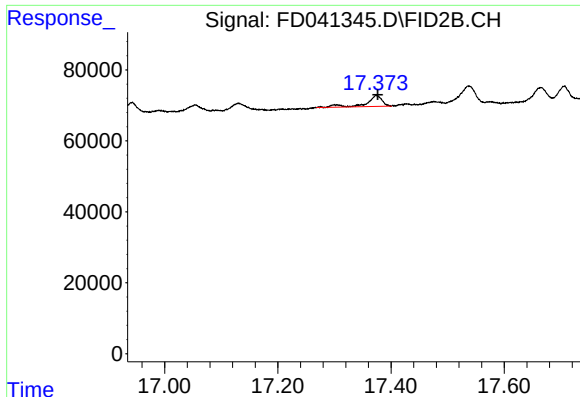

#17 n-Tricontane (C30)


R.T.: 17.374 min
Delta R.T.: -0.002 min
Response: 56809
Conc: 0.40 ug/ml

Instrument :
FID_D
ClientSampleId :

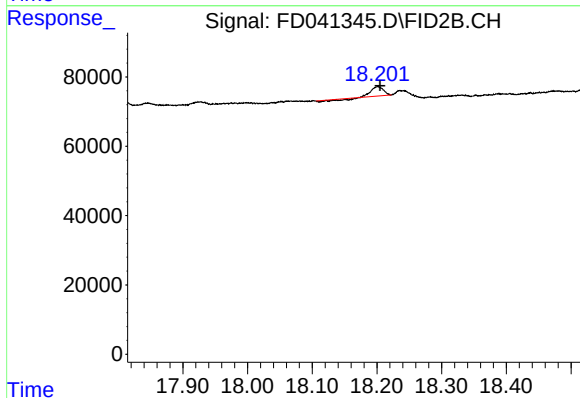


#18 n-Dotriacontane (C32)

R.T.: 18.201 min
Delta R.T.: -0.003 min
Response: 28174
Conc: 0.22 ug/ml

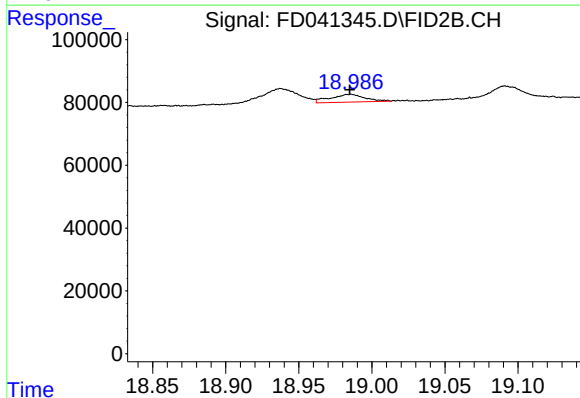


#19 n-Tetratriacontane (C34)

R.T.: 18.985 min
Delta R.T.: 0.000 min
Response: 41078
Conc: 0.36 ug/ml

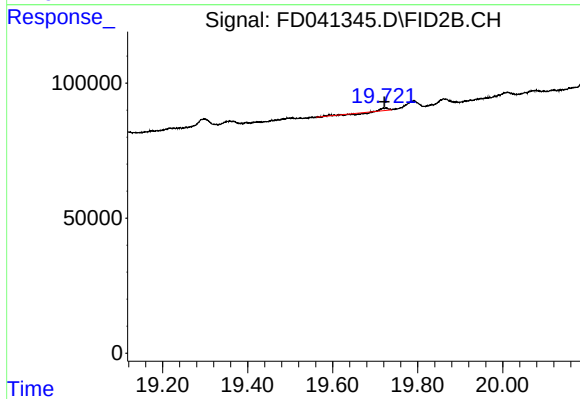

#20 n-Hexatriacontane (C36)

R.T.: 19.727 min
Delta R.T.: 0.005 min
Response: 943
Conc: 0.01 ug/ml

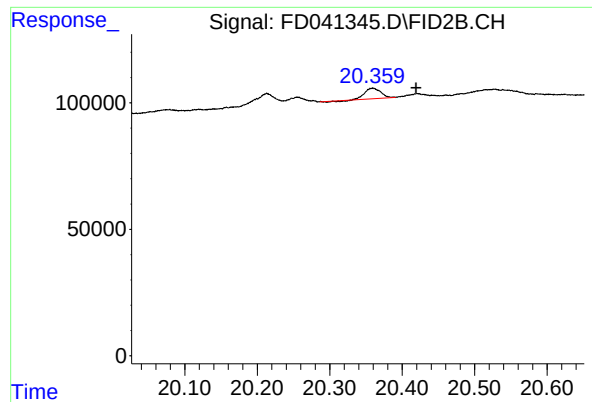

#21 n-Octatriacontane (C38)

R.T.: 20.359 min
Delta R.T.: -0.060 min
Response: 61494
Conc: 0.65 ug/ml

Instrument :
FID_D
ClientSampleId :