

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD030322AL\
 Data File : FD041367.D
 Signal(s) : FID2B.CH
 Acq On : 03 Mar 2022 9:12
 Operator : UA/NP
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 04 02:06:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 022322.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 24 01:21:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.238	38882	0.250 ug/ml
11) T n-Heneicosane (C21)	12.858	300700	1.920 ug/ml
14) T n-Tetracosane (C24)	14.485f	66690	0.425 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD030322AL\
Data File : FD041367.D
Signal(s) : FID2B.CH
Acq On : 03 Mar 2022 9:12
Operator : UA/NP
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 04 02:06:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 022322.M
Quant Title : GC Extractables
QLast Update : Thu Feb 24 01:21:33 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

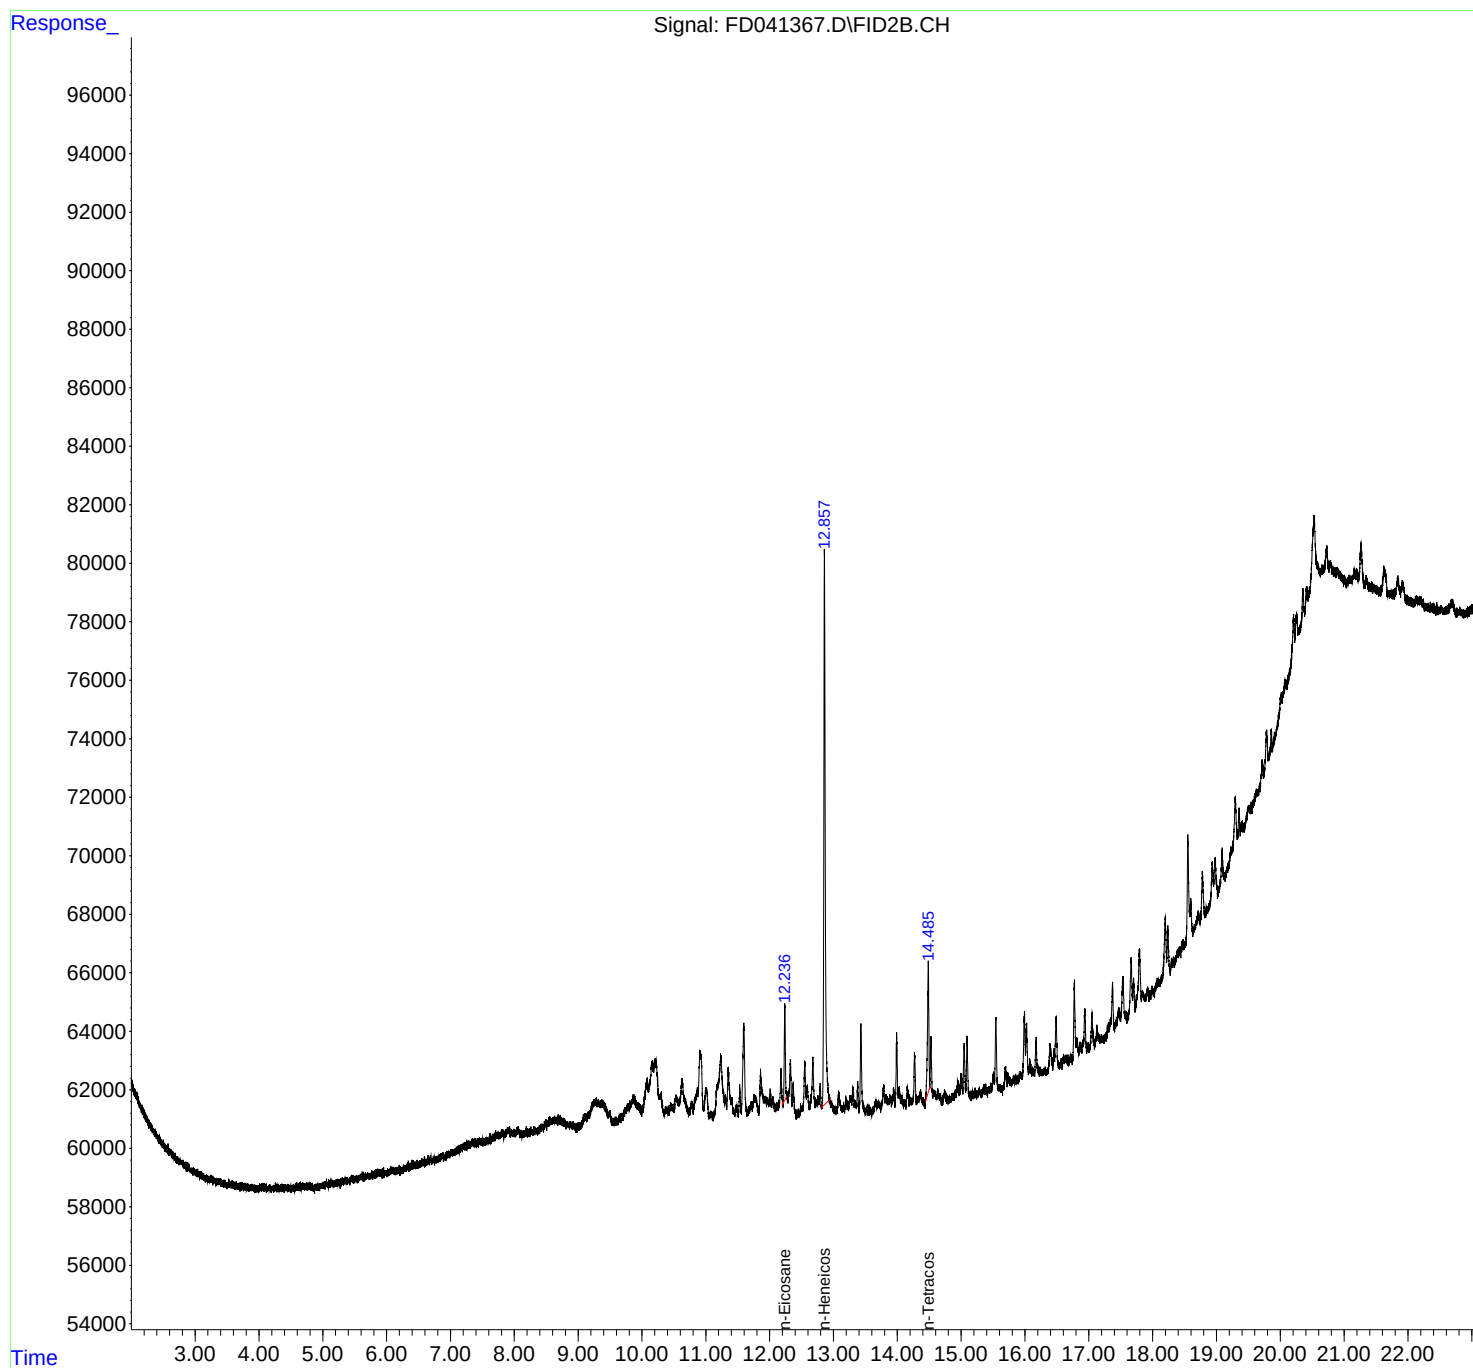


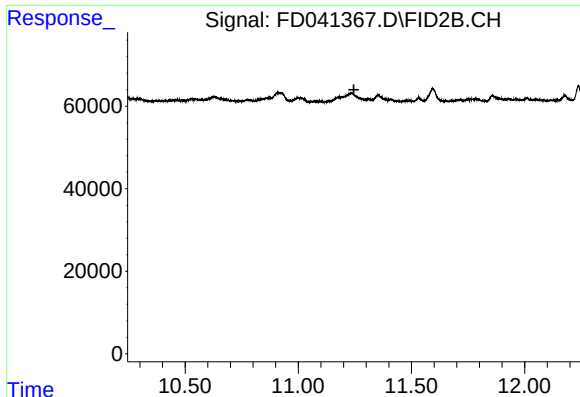

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.246 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

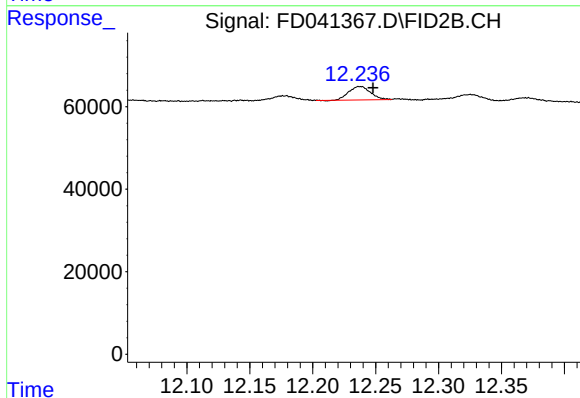


#10 n-Eicosane (C20)

R.T.: 12.238 min
Delta R.T.: -0.010 min
Response: 38882
Conc: 0.25 ug/ml

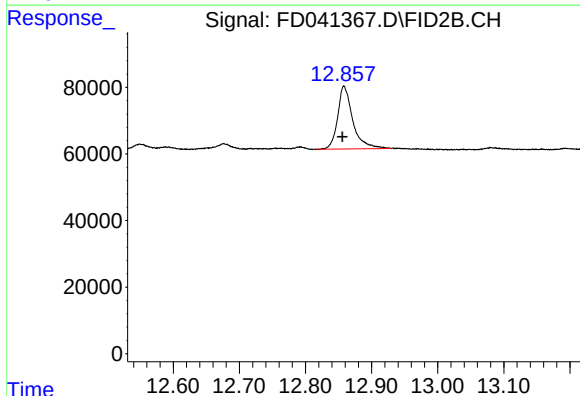


#11 n-Heneicosane (C21)

R.T.: 12.858 min
Delta R.T.: 0.002 min
Response: 300700
Conc: 1.92 ug/ml

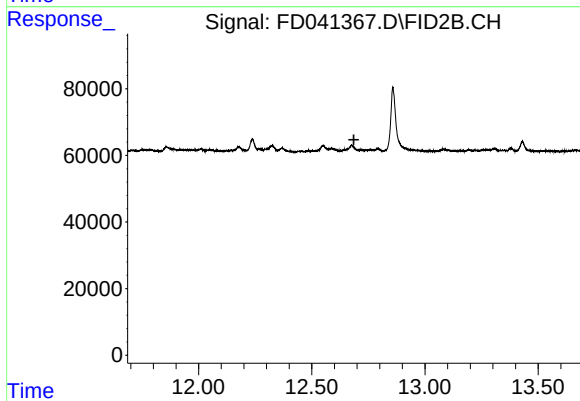

#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.686 min
Response: 0
Conc: N.D.

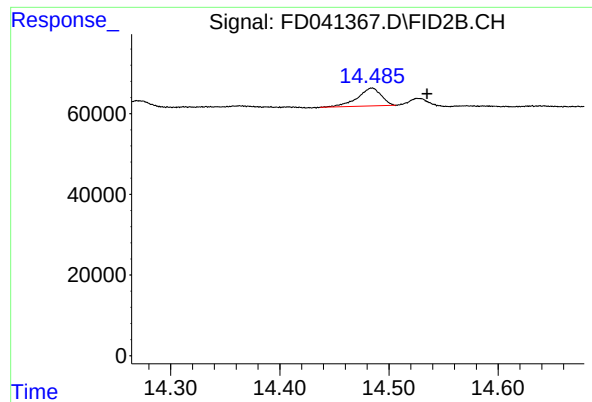

#14 n-Tetracosane (C24)

R.T.: 14.485 min
Delta R.T.: -0.050 min
Response: 66690
Conc: 0.43 ug/ml

Instrument :

FID_D

ClientSampleId :