

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD030322AL\
 Data File : FD041377.D
 Signal(s) : FID2B.CH
 Acq On : 03 Mar 2022 17:33
 Operator : UA/NP
 Sample : N1751-06
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 04 02:08:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 022322.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 24 01:21:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.244	5771730	33.274 ug/ml
Spiked Amount 50.000		Recovery =	66.55%
12) S 1-chlorooctadecane (S...	12.683	4526627	33.435 ug/ml
Spiked Amount 50.000		Recovery =	66.87%
Target Compounds			
10) T n-Eicosane (C20)	12.269	519104	3.344 ug/ml
14) T n-Tetracosane (C24)	14.589f	50907	0.325 ug/ml
16) T n-Octacosane (C28)	16.455	72521	0.487 ug/ml
21) T n-Octatriacontane (C38)	20.414	13677	0.144 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD030322AL\
Data File : FD041377.D
Signal(s) : FID2B.CH
Acq On : 03 Mar 2022 17:33
Operator : UA/NP
Sample : N1751-06
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 04 02:08:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 022322.M
Quant Title : GC Extractables
QLast Update : Thu Feb 24 01:21:33 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

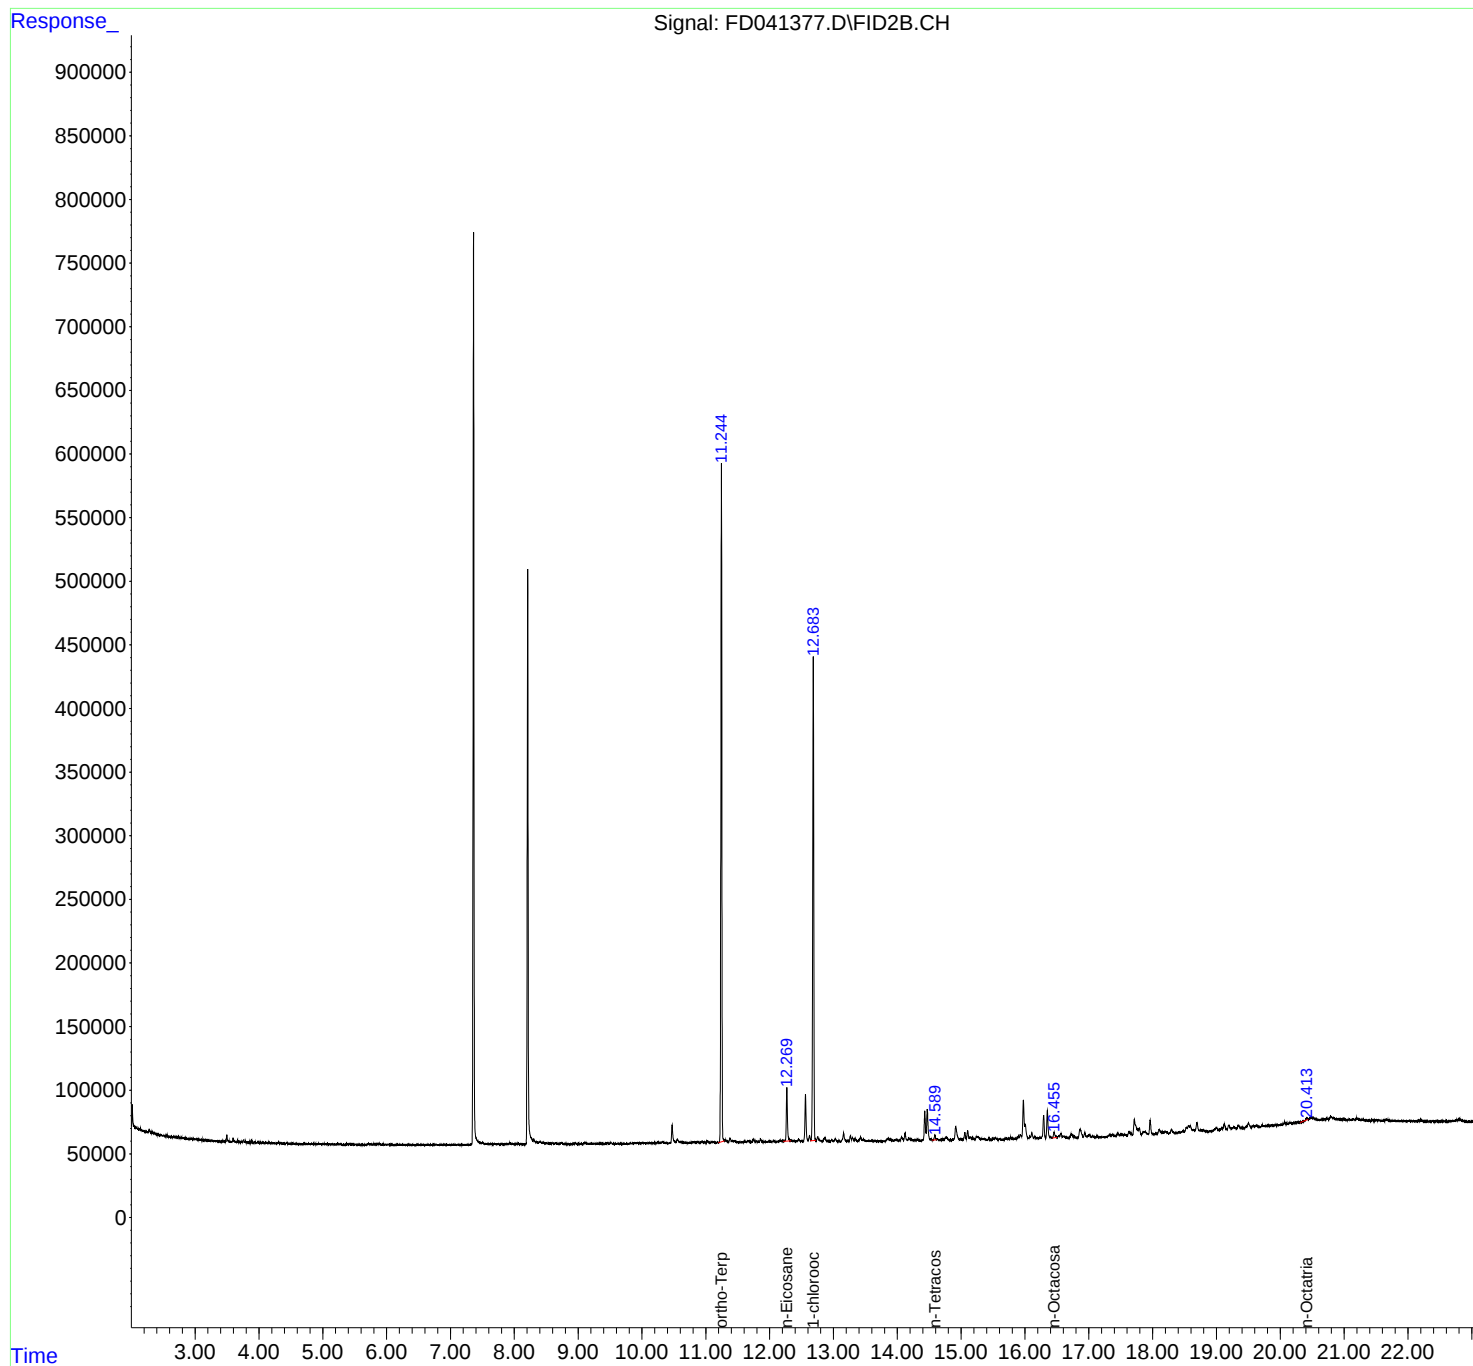


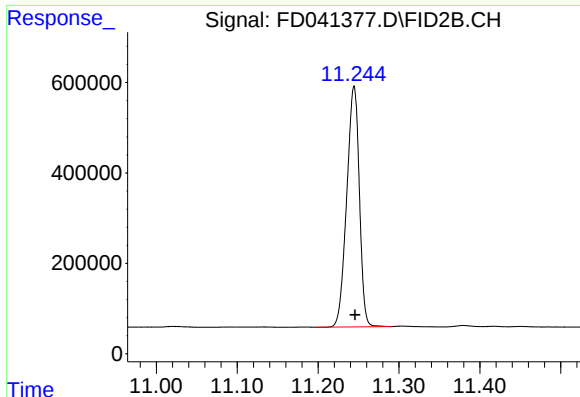

#9 ortho-Terphenyl (SURR)


R.T.: 11.244 min
Delta R.T.: -0.001 min
Response: 5771730
Conc: 33.27 ug/ml

Instrument :
FID_D
ClientSampleId :

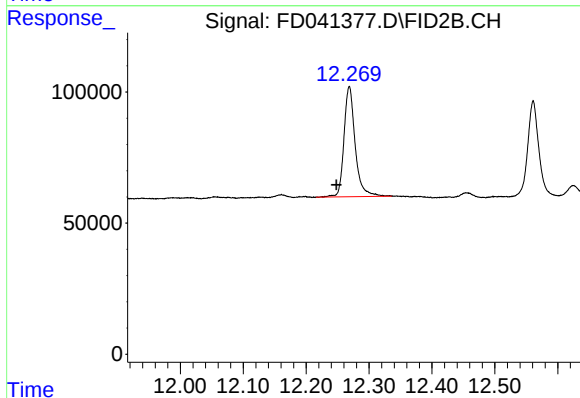


#10 n-Eicosane (C20)

R.T.: 12.269 min
Delta R.T.: 0.021 min
Response: 519104
Conc: 3.34 ug/ml

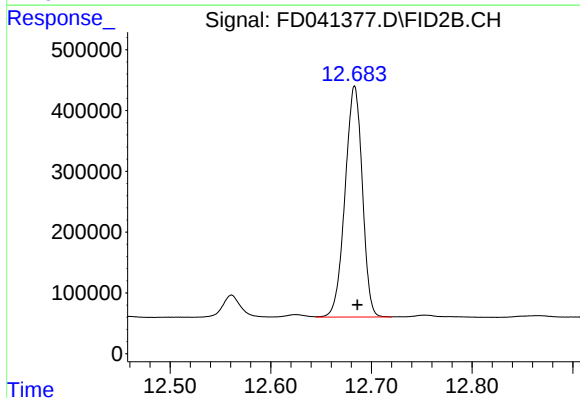


#12 1-chlorooctadecane (SURR)

R.T.: 12.683 min
Delta R.T.: -0.003 min
Response: 4526627
Conc: 33.44 ug/ml

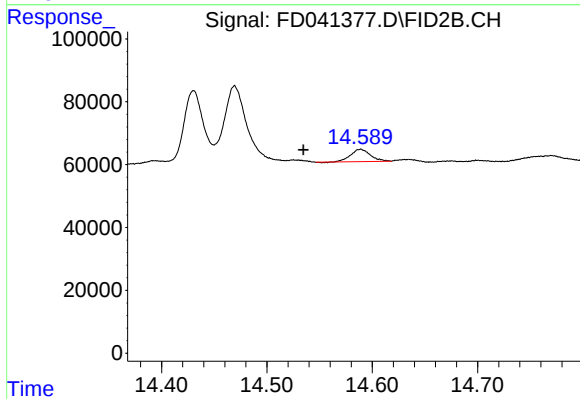

#14 n-Tetracosane (C24)


R.T.: 14.589 min
Delta R.T.: 0.054 min
Response: 50907
Conc: 0.32 ug/ml

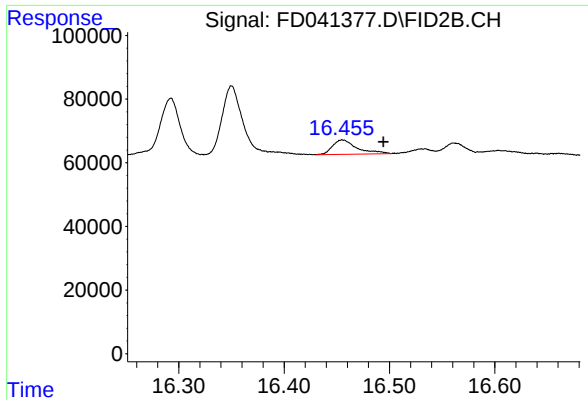

#16 n-Octacosane (C28)

R.T.: 16.455 min
Delta R.T.: -0.039 min
Response: 72521
Conc: 0.49 ug/ml

Instrument :
FID_D
ClientSampleId :

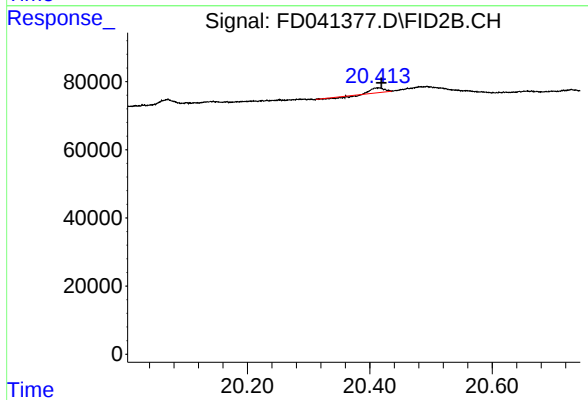

#21 n-Octatriacontane (C38)

R.T.: 20.414 min
Delta R.T.: -0.005 min
Response: 13677
Conc: 0.14 ug/ml