

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD030519AL\
 Data File : FD028133.D
 Signal(s) : FID2B.CH
 Acq On : 06 Mar 2019 9:22
 Operator : AJ\SJ
 Sample : K1596-01
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :
 COMP-13

Integration File: autoint1.e
 Quant Time: Mar 06 12:27:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 030519.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 06 03:32:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.206	3116711	22.395 ug/ml
Spiked Amount 50.000		Recovery =	44.79%
12) S 1-chlorooctadecane (S...	12.649	2385832	22.213 ug/ml
Spiked Amount 50.000		Recovery =	44.43%
Target Compounds			
10) T n-Eicosane (C20)	12.228	104876	0.973 ug/ml
16) T n-Octacosane (C28)	16.450	97874	0.987 ug/ml
17) T n-Tricontane (C30)	17.334	115654	1.225 ug/ml
19) T n-Tetratriacontane (C34)	18.928	121035	1.626 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD030519AL\
Data File : FD028133.D
Signal(s) : FID2B.CH
Acq On : 06 Mar 2019 9:22
Operator : AJ\SJ
Sample : K1596-01
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :
COMP-13

Integration File: autoint1.e
Quant Time: Mar 06 12:27:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Alaphatic EPH 030519.M
Quant Title : GC Extractables
QLast Update : Wed Mar 06 03:32:11 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

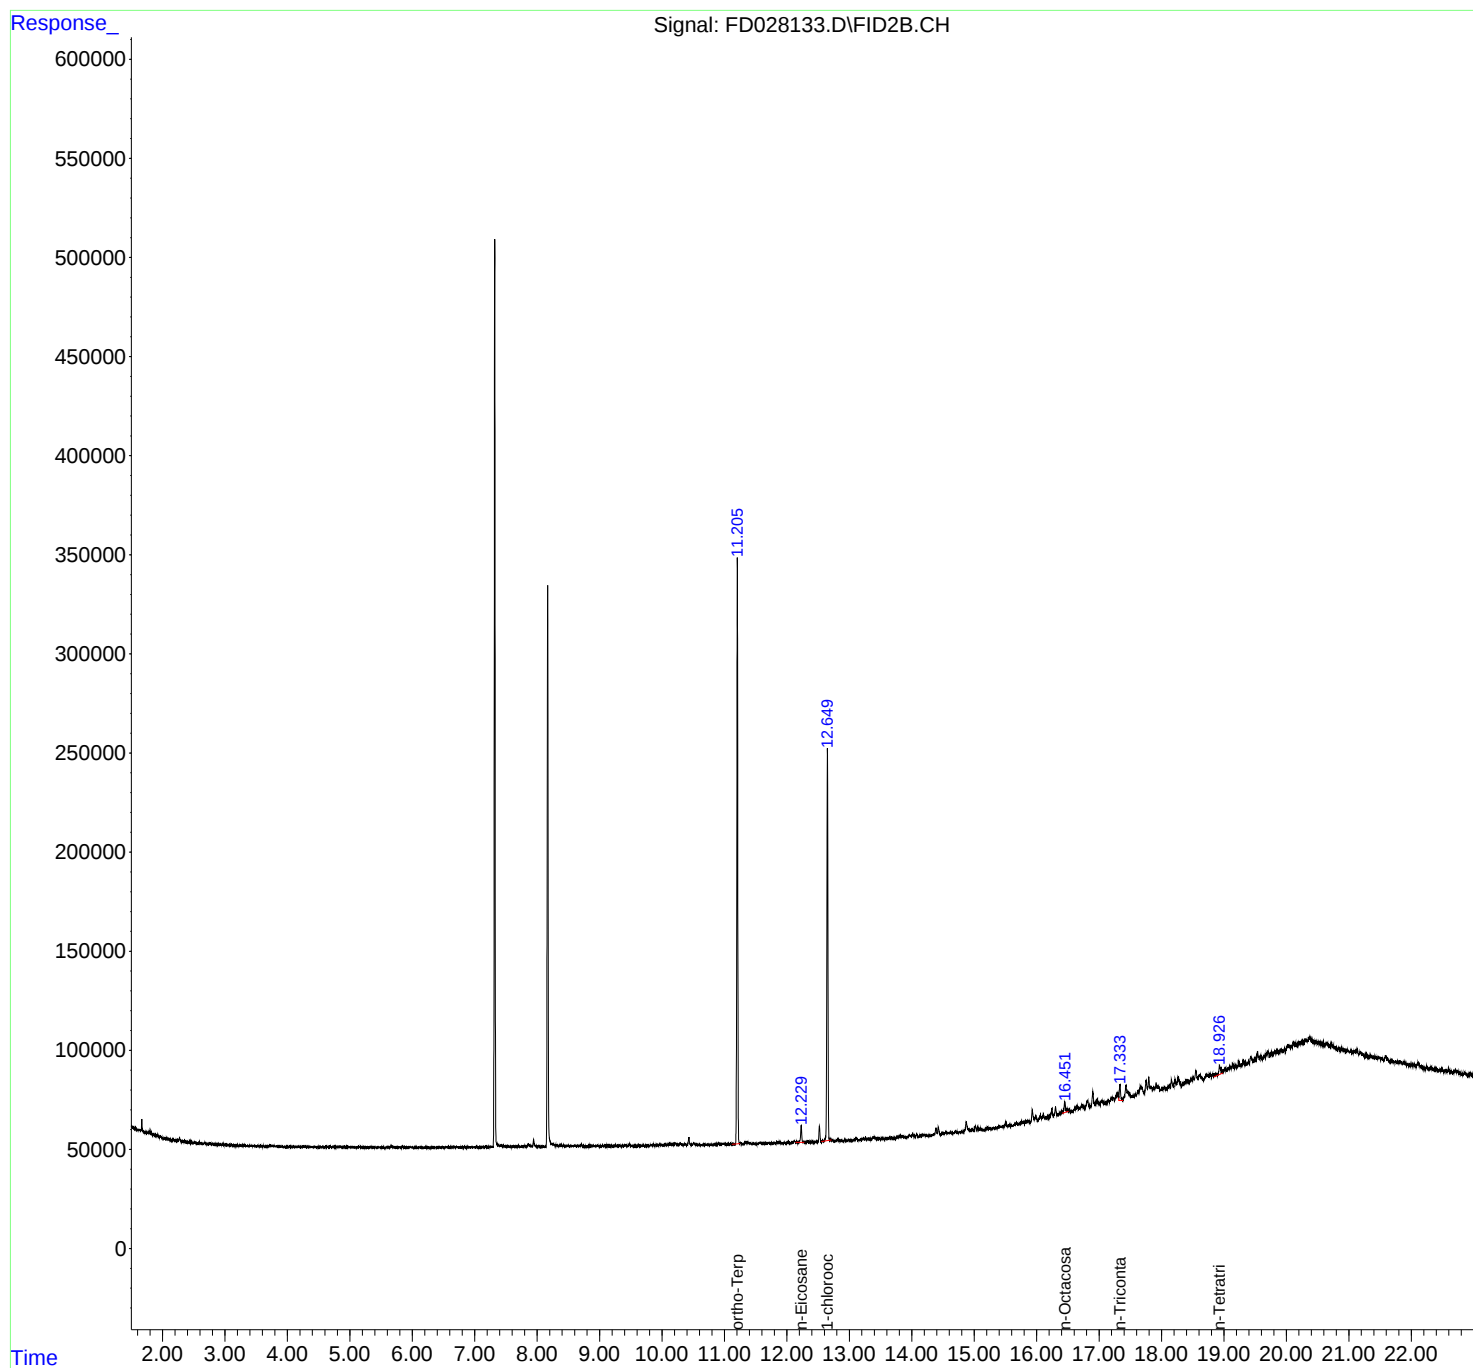


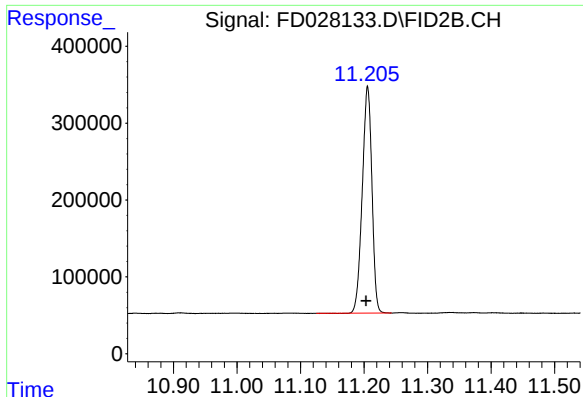

#9 ortho-Terphenyl (SURR)


R.T.: 11.206 min
Delta R.T.: 0.002 min
Response: 3116711
Conc: 22.39 ug/ml

Instrument :
FID_D
ClientSampleId :
COMP-13

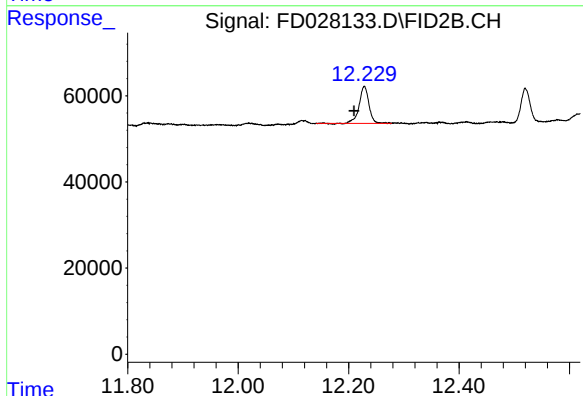


#10 n-Eicosane (C20)

R.T.: 12.228 min
Delta R.T.: 0.019 min
Response: 104876
Conc: 0.97 ug/ml

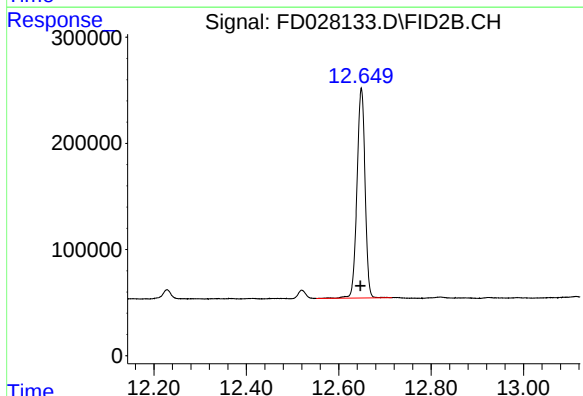


#12 1-chlorooctadecane (SURR)

R.T.: 12.649 min
Delta R.T.: 0.002 min
Response: 2385832
Conc: 22.21 ug/ml

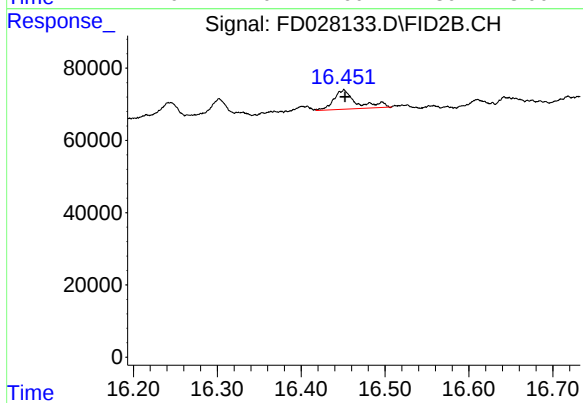

#16 n-Octacosane (C28)


R.T.: 16.450 min
Delta R.T.: -0.002 min
Response: 97874
Conc: 0.99 ug/ml

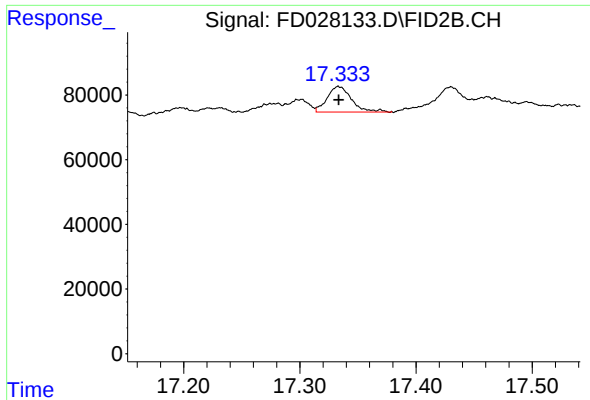

#17 n-Tricontane (C30)

R.T.: 17.334 min
Delta R.T.: 0.000 min
Response: 115654
Conc: 1.22 ug/ml

Instrument :
FID_D
ClientSampleId :
COMP-13

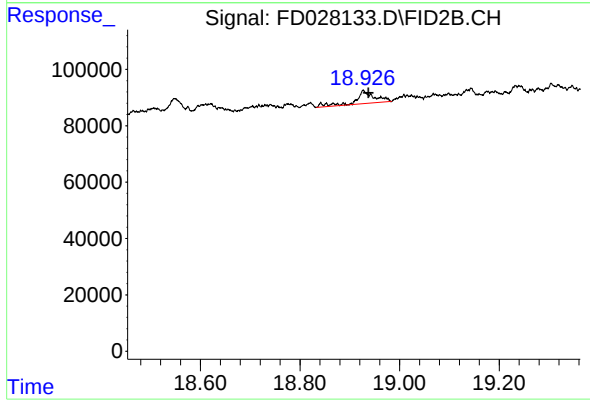

#19 n-Tetratriacontane (C34)

R.T.: 18.928 min
Delta R.T.: -0.010 min
Response: 121035
Conc: 1.63 ug/ml