

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD030922AL\
 Data File : FD041455.D
 Signal(s) : FID2B.CH
 Acq On : 09 Mar 2022 13:55
 Operator : UA/NP
 Sample : I.BLK
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_D
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 10 02:13:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 022322.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 24 01:21:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

18) T	n-Dotriacontane (C32)	18.216	69857	0.549 ug/ml
19) T	n-Tetratriacontane (C34)	18.992	21677	0.190 ug/ml
20) T	n-Hexatriacontane (C36)	19.729	19600	0.191 ug/ml
21) T	n-Octatriacontane (C38)	20.417	8396	0.088 ug/ml
22) T	n-Tetracontane (C40)	21.171	38111	0.402 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD030922AL\
Data File : FD041455.D
Signal(s) : FID2B.CH
Acq On : 09 Mar 2022 13:55
Operator : UA/NP
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 10 02:13:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 022322.M
Quant Title : GC Extractables
QLast Update : Thu Feb 24 01:21:33 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

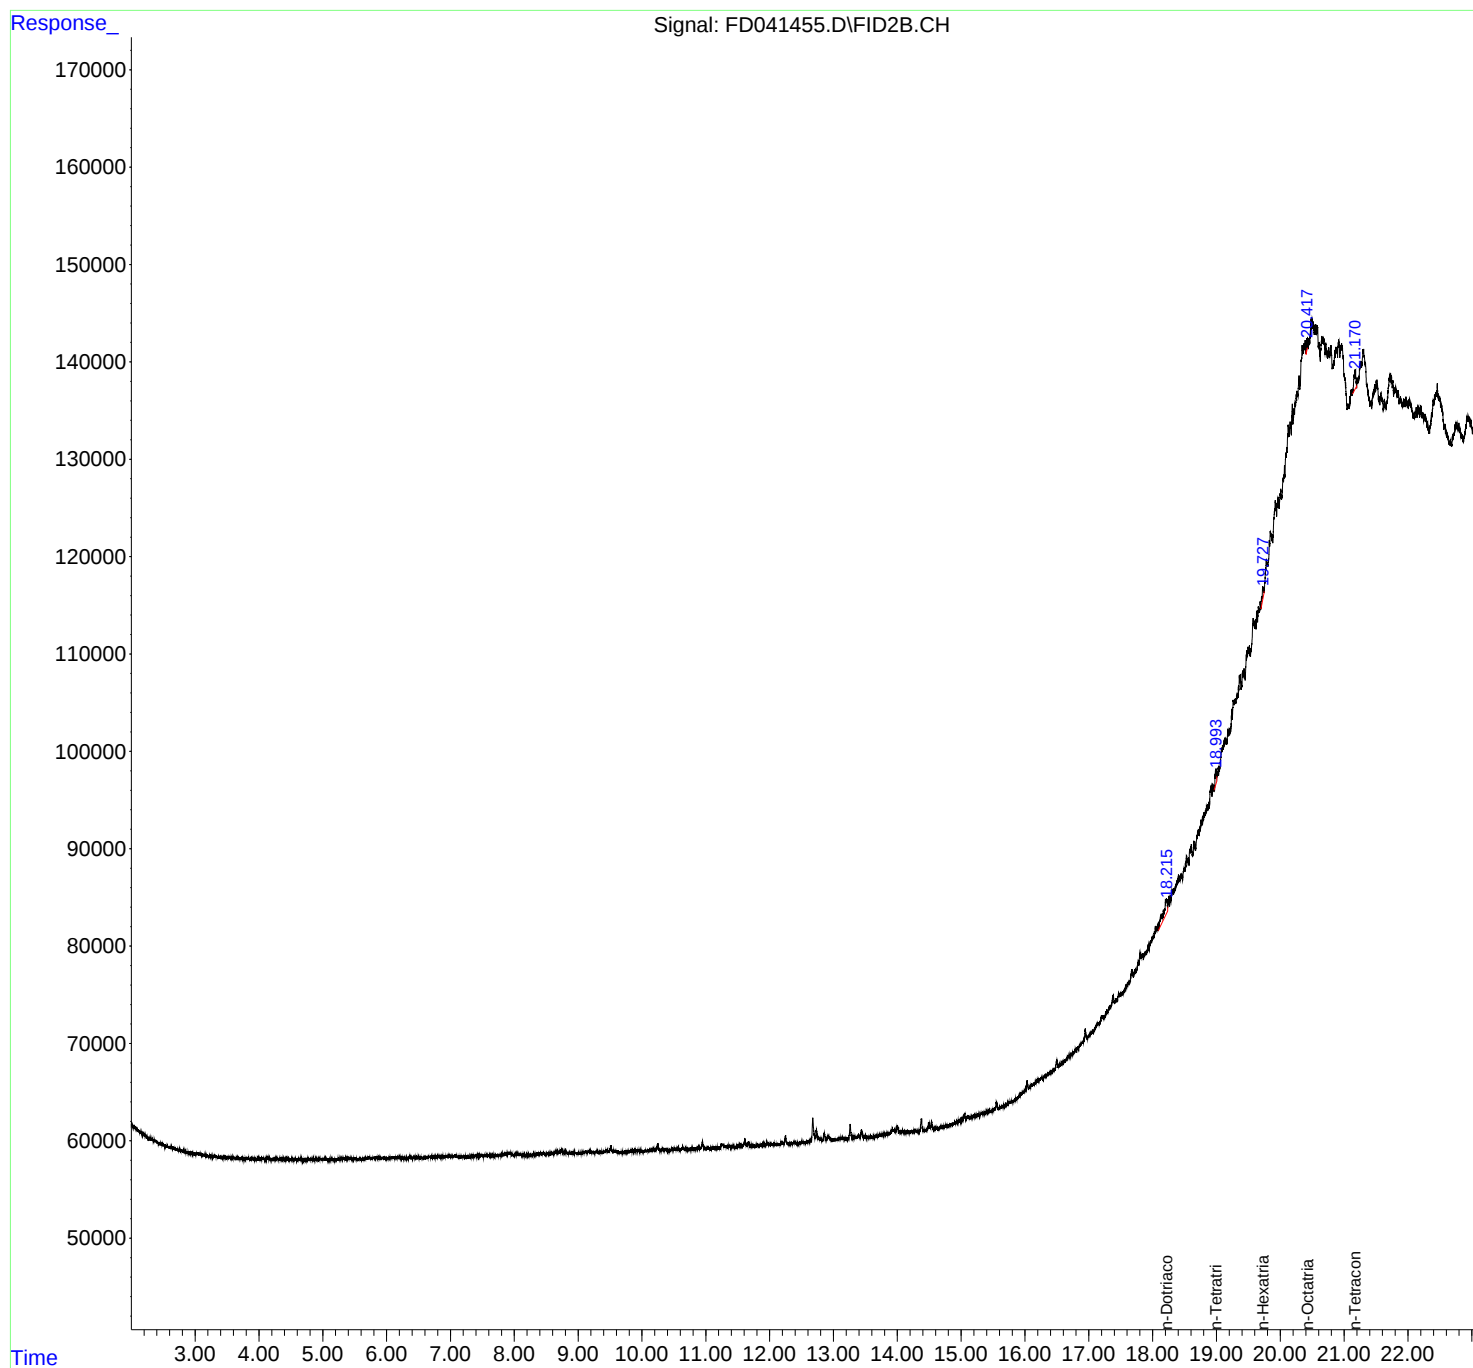


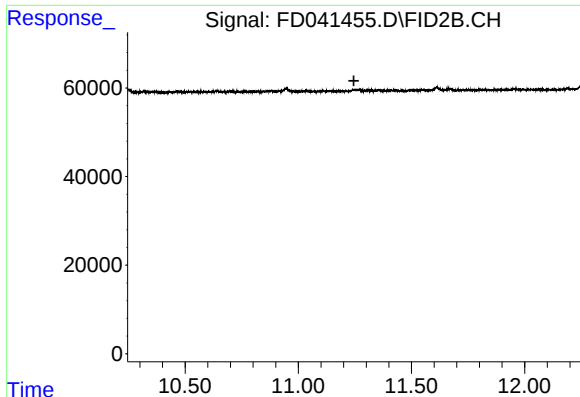

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.246 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

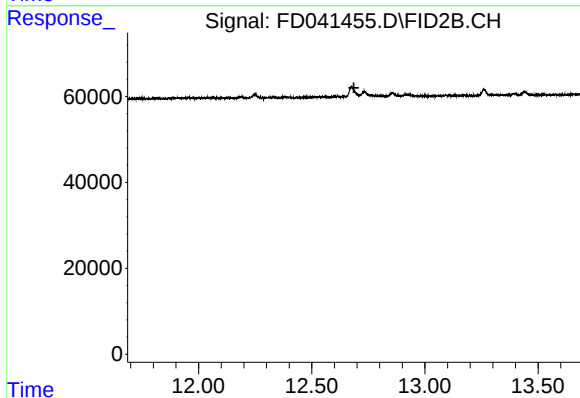


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.686 min
Response: 0
Conc: N.D.

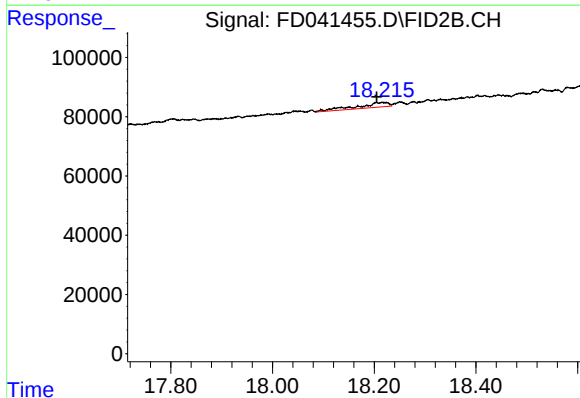


#18 n-Dotriacontane (C32)

R.T.: 18.216 min
Delta R.T.: 0.011 min
Response: 69857
Conc: 0.55 ug/ml

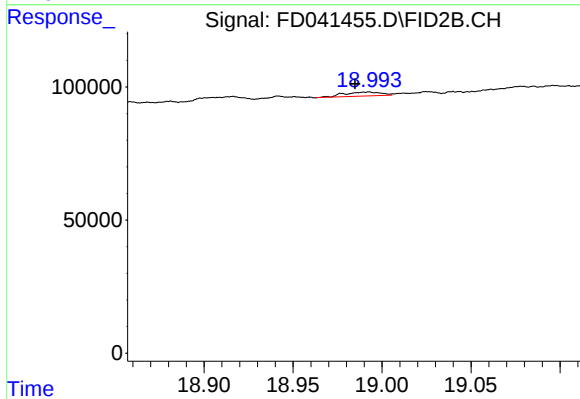

#19 n-Tetratriacontane (C34)


R.T.: 18.992 min
Delta R.T.: 0.007 min
Response: 21677
Conc: 0.19 ug/ml

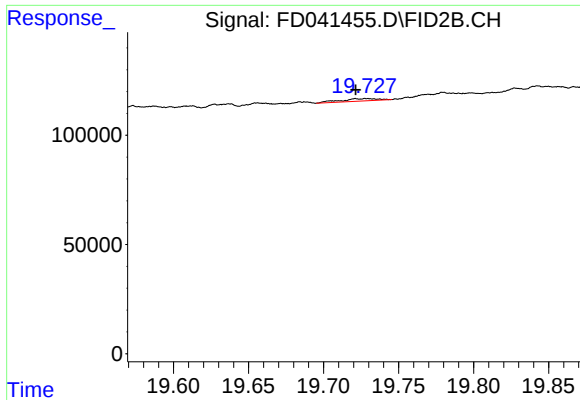

#20 n-Hexatriacontane (C36)


R.T.: 19.729 min
Delta R.T.: 0.008 min
Response: 19600
Conc: 0.19 ug/ml

Instrument :
FID_D
ClientSampleId :

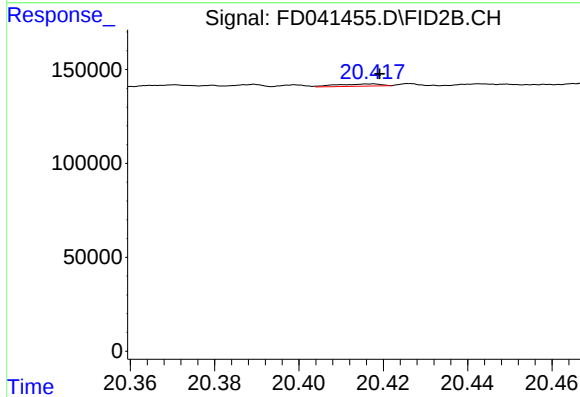

#21 n-Octatriacontane (C38)

R.T.: 20.417 min
Delta R.T.: -0.002 min
Response: 8396
Conc: 0.09 ug/ml

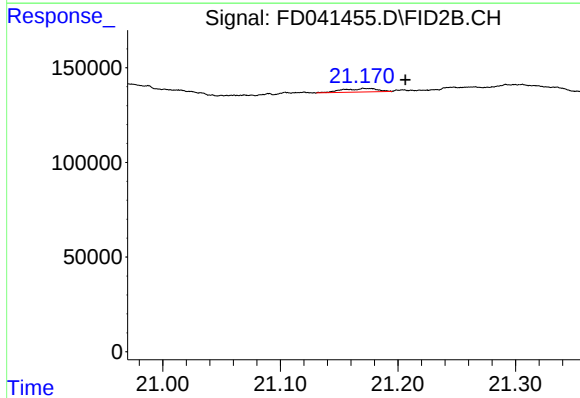

#22 n-Tetracontane (C40)

R.T.: 21.171 min
Delta R.T.: -0.035 min
Response: 38111
Conc: 0.40 ug/ml