

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF031822\  
 Data File : FF010092.D  
 Signal(s) : FID2B.ch  
 Acq On : 19 Mar 2022 00:38  
 Operator : AJ\MA  
 Sample : RT MARKER  
 Misc :  
 ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e  
 Quant Time: Mar 19 01:23:45 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF031022.M  
 Quant Title :  
 QLast Update : Thu Mar 10 12:46:01 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| Target Compounds            |        |          |              |
| 3) N-DODECANE               | 6.450  | 3597529  | 20.922 ug/ml |
| 12) N-OCTACOSANE            | 16.867 | 3032616  | 18.948 ug/ml |
| 14) N-DOTRIACONTANE         | 18.603 | 200490   | 1.373 ug/ml  |
| 16) N-HEXATRIACONTANE       | 20.155 | 164243   | 1.321 ug/ml  |
| 18) N-TETRACONTANE          | 21.808 | 653601   | 6.369 ug/ml  |
| -----                       |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF031822\  
Data File : FF010092.D  
Signal(s) : FID2B.ch  
Acq On : 19 Mar 2022 00:38  
Operator : AJ\MA  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Mar 19 01:23:45 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF031022.M  
Quant Title :  
QLast Update : Thu Mar 10 12:46:01 2022  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

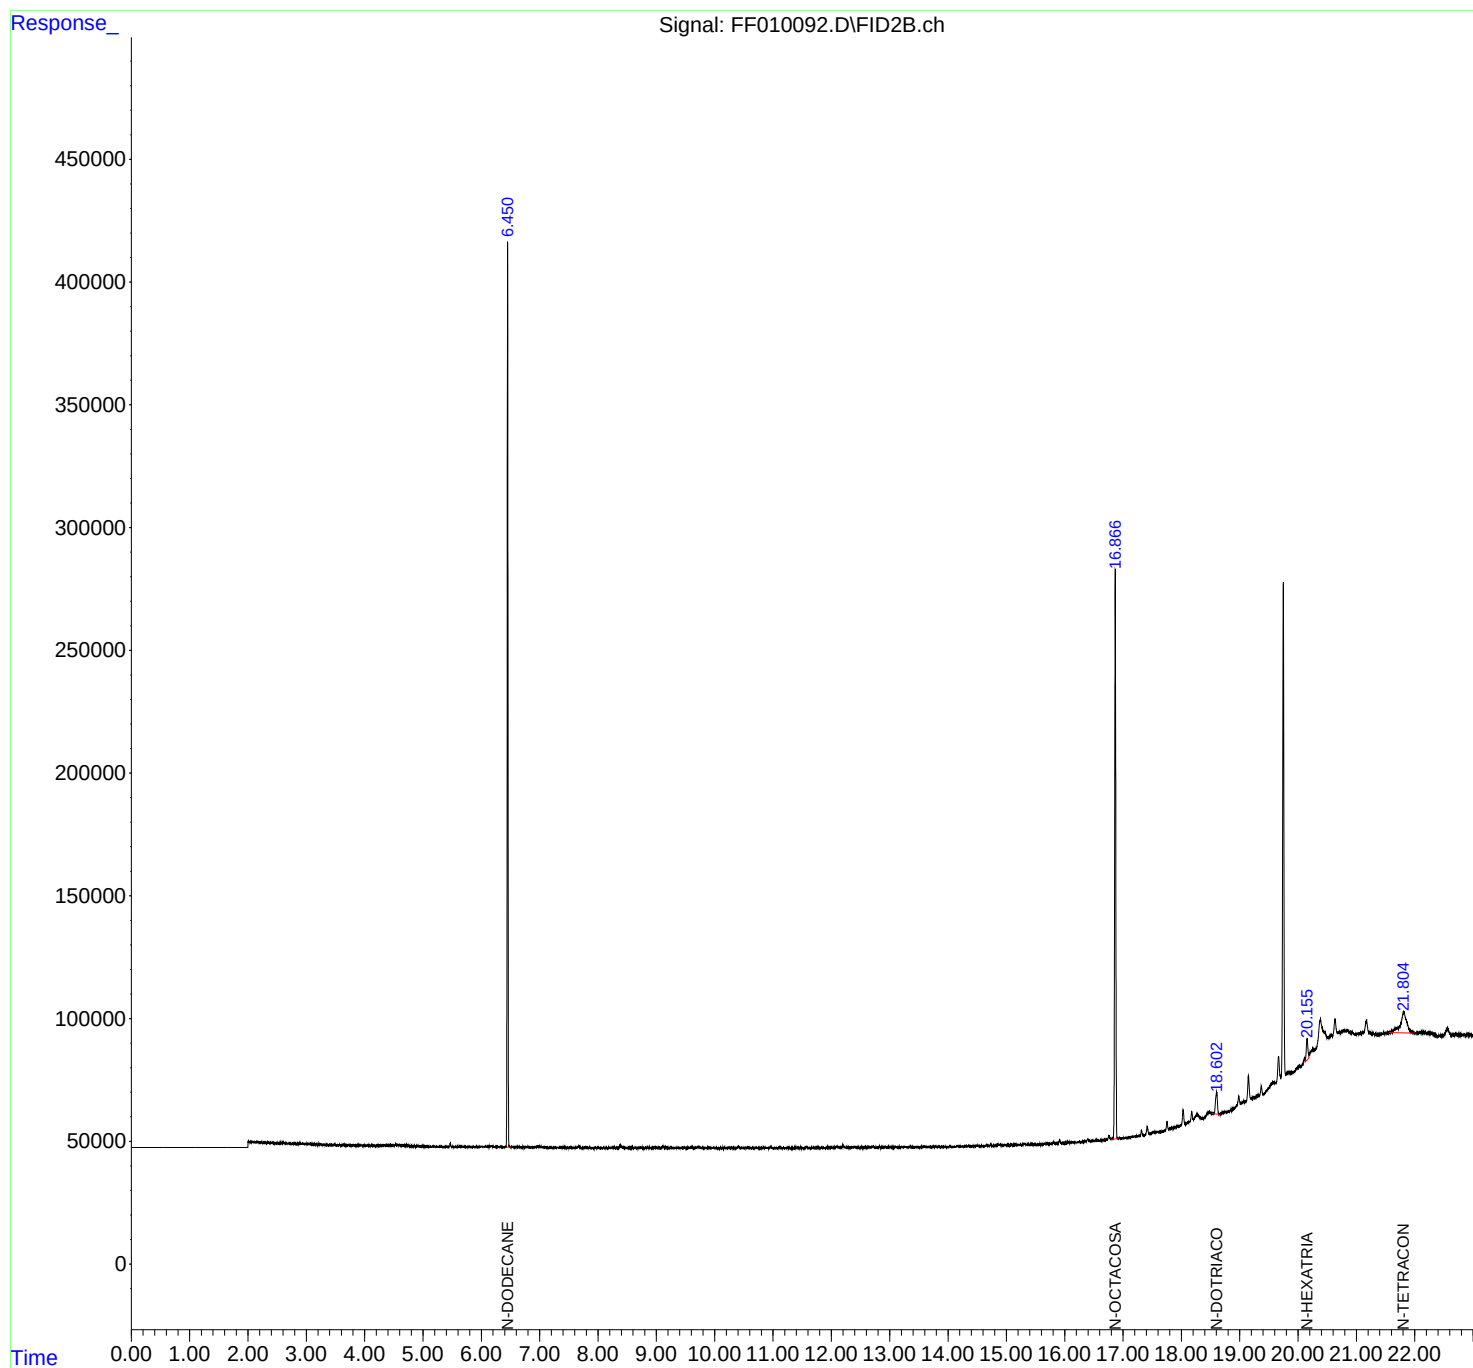

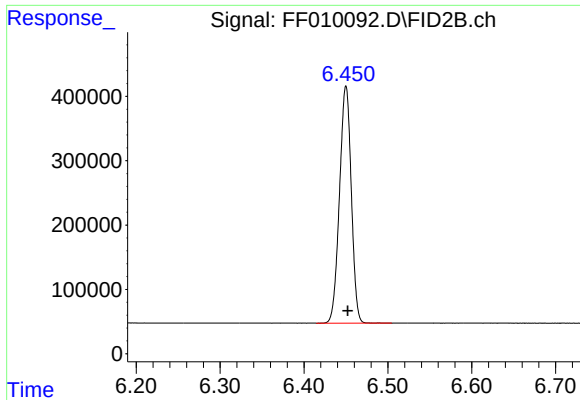


#3 N-DODECANE

R.T.: 6.450 min  
Delta R.T.: -0.002 min  
Response: 3597529  
Conc: 20.92 ug/ml

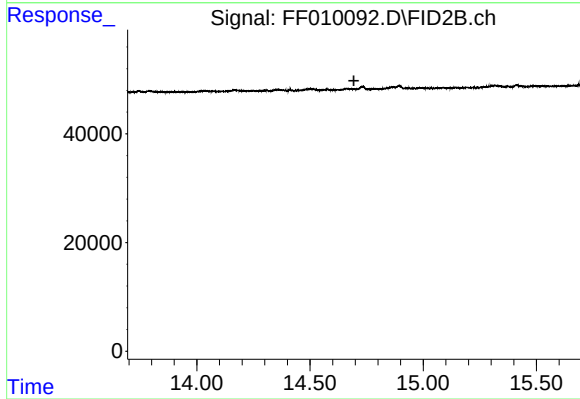


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.694 min  
Response: 0  
Conc: N.D.

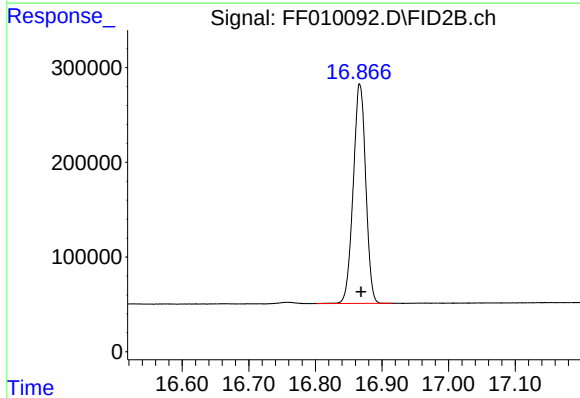


#12 N-OCTACOSANE

R.T.: 16.867 min  
Delta R.T.: -0.002 min  
Response: 3032616  
Conc: 18.95 ug/ml

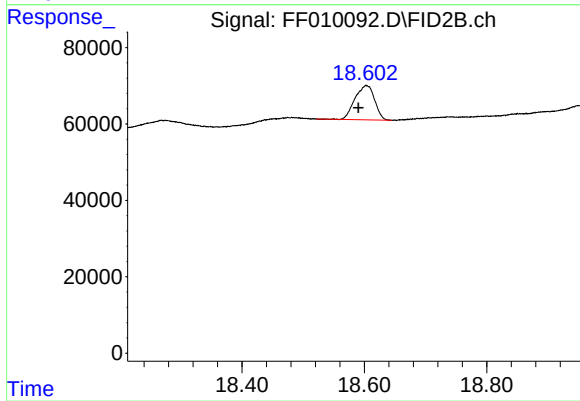


#14 N-DOTRIACONTANE

R.T.: 18.603 min  
Delta R.T.: 0.013 min  
Response: 200490  
Conc: 1.37 ug/ml

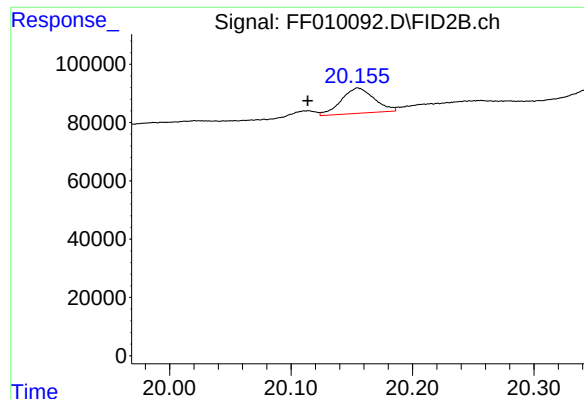

#16 N-HEXATRIACONTANE

R.T.: 20.155 min  
Delta R.T.: 0.042 min  
Response: 164243  
Conc: 1.32 ug/ml

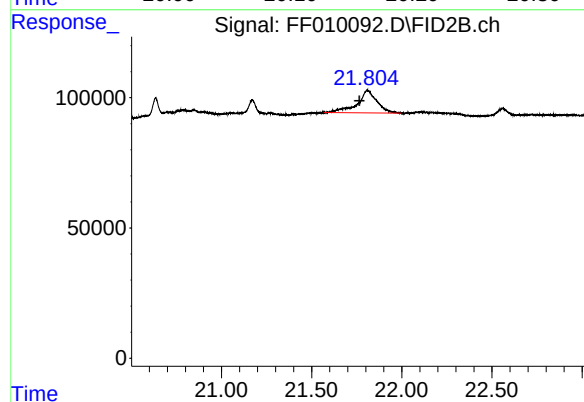

#18 N-TETRACONTANE

R.T.: 21.808 min  
Delta R.T.: 0.042 min  
Response: 653601  
Conc: 6.37 ug/ml