

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD040523AL\
Data File : FD045410.D
Signal(s) : FID2B.ch
Acq On : 05 Apr 2023 08:03
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 05 09:10:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 040523.M
Quant Title : GC Extractables
QLast Update : Wed Apr 05 05:57:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

16) T	n-Octacosane (C28)	16.677	54050	0.411 ug/ml
17) T	n-Tricontane (C30)	17.559	53161	0.408 ug/ml
18) T	n-Dotriacontane (C32)	18.384	50672	0.389 ug/ml
19) T	n-Tetratriacontane (C34)	19.163	61137	0.489 ug/ml
20) T	n-Hexatriacontane (C36)	19.896	117643	1.025 ug/ml
21) T	n-Octatriacontane (C38)	20.600	235368	2.145 ug/ml
22) T	n-Tetracontane (C40)	21.434	391048	3.645 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_D\Data\FD040523AL\
Data File : FD045410.D
Signal(s) : FID2B.ch
Acq On : 05 Apr 2023 08:03
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_D
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 05 09:10:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 040523.M
Quant Title : GC Extractables
QLast Update : Wed Apr 05 05:57:21 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

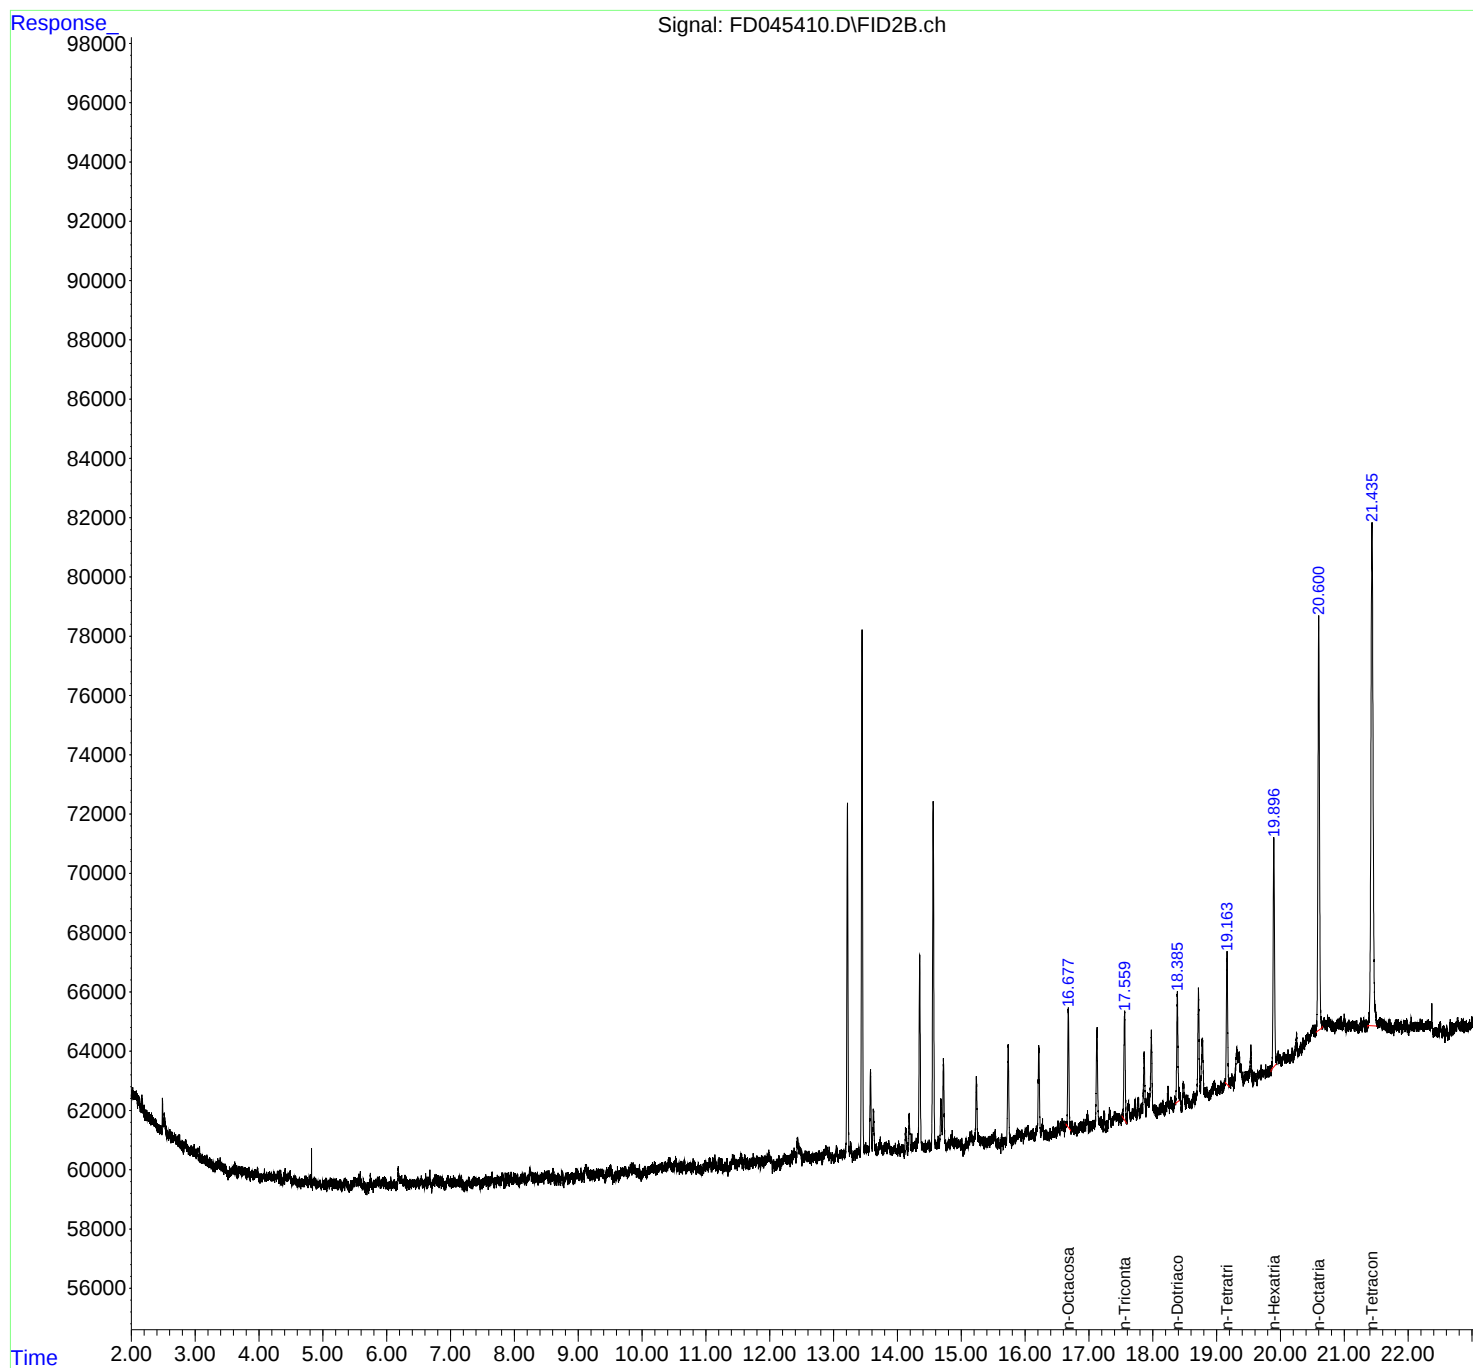


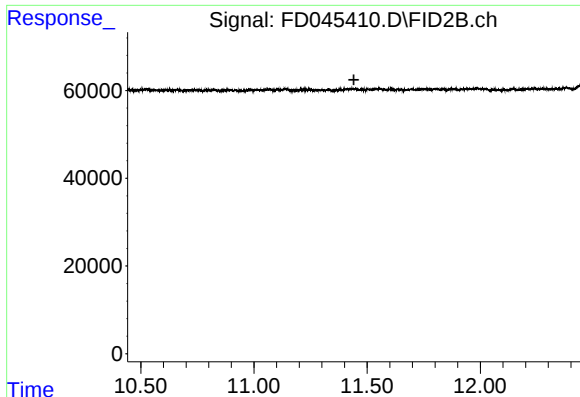

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.442 min
Response: 0
Conc: N.D.

Instrument :
FID_D
ClientSampleId :

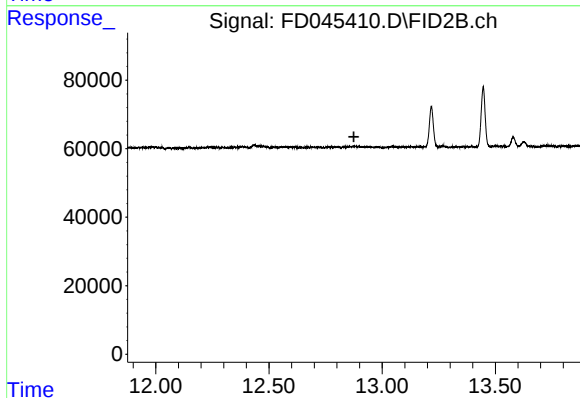


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.875 min
Response: 0
Conc: N.D.

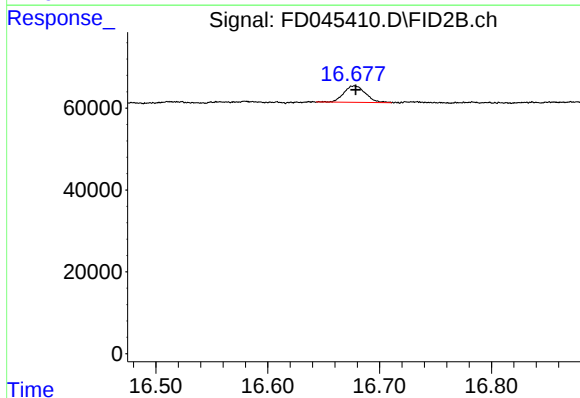


#16 n-Octacosane (C28)

R.T.: 16.677 min
Delta R.T.: -0.002 min
Response: 54050
Conc: 0.41 ug/ml

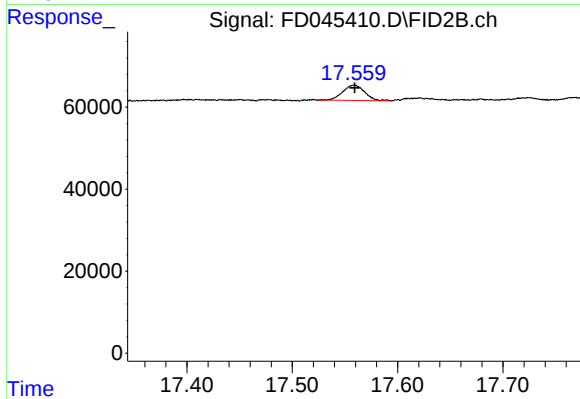

#17 n-Tricontane (C30)


R.T.: 17.559 min
Delta R.T.: 0.000 min
Response: 53161
Conc: 0.41 ug/ml

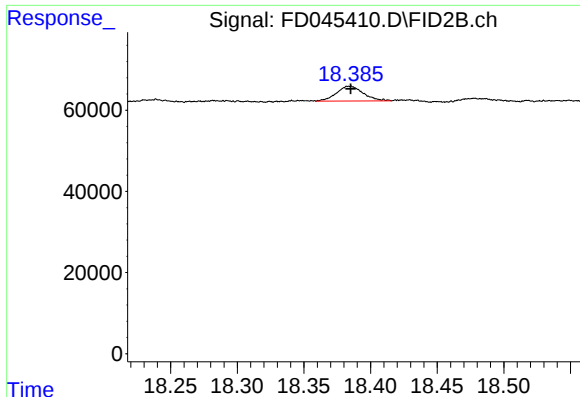

#18 n-Dotriacontane (C32)


R.T.: 18.384 min
Delta R.T.: 0.000 min
Response: 50672
Conc: 0.39 ug/ml

Instrument :
FID_D
ClientSampleId :

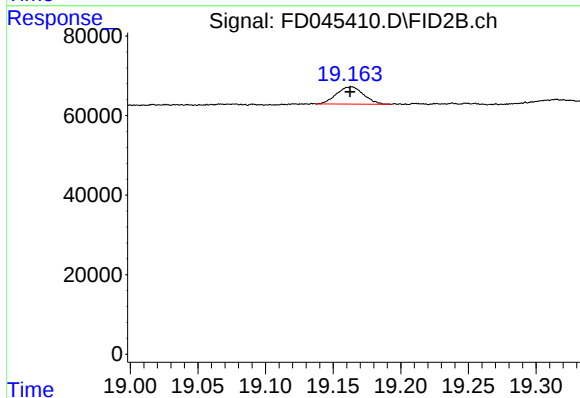


#19 n-Tetratriacontane (C34)

R.T.: 19.163 min
Delta R.T.: 0.000 min
Response: 61137
Conc: 0.49 ug/ml

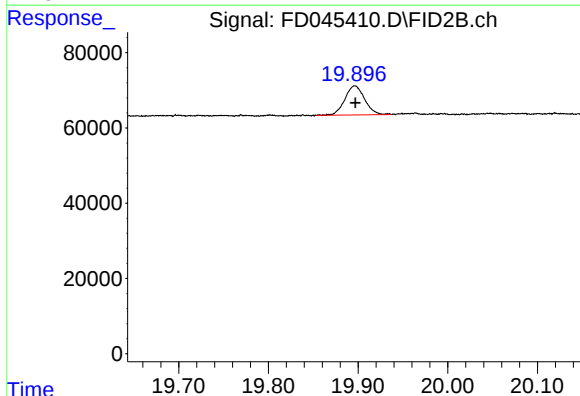


#20 n-Hexatriacontane (C36)

R.T.: 19.896 min
Delta R.T.: 0.000 min
Response: 117643
Conc: 1.03 ug/ml

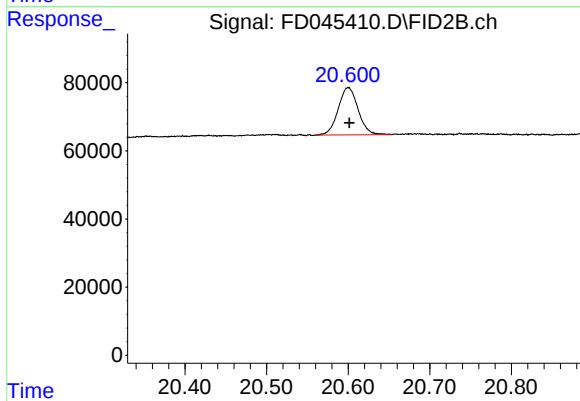

#21 n-Octatriacontane (C38)

R.T.: 20.600 min
Delta R.T.: -0.001 min
Response: 235368
Conc: 2.15 ug/ml

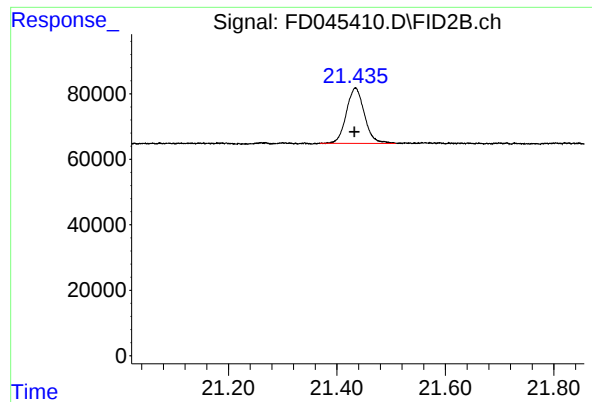

#22 n-Tetracontane (C40)

R.T.: 21.434 min
Delta R.T.: 0.002 min
Response: 391048
Conc: 3.65 ug/ml

Instrument :

FID_D

ClientSampleId :